

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
 Data File : P0068431.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2020 11:38
 Operator : DD\AJ
 Sample : L2665-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0375-AMENDED-COMP-MP-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 14:34:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.900	3.931	720354	785971	25.684	22.905m
2) SA Decachlor...	10.851	9.203	1074468	984518	27.001	25.572

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
Data File : P0068431.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2020 11:38
Operator : DD\AJ
Sample : L2665-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0375-AMENDED-COMP-MP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 14:34:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

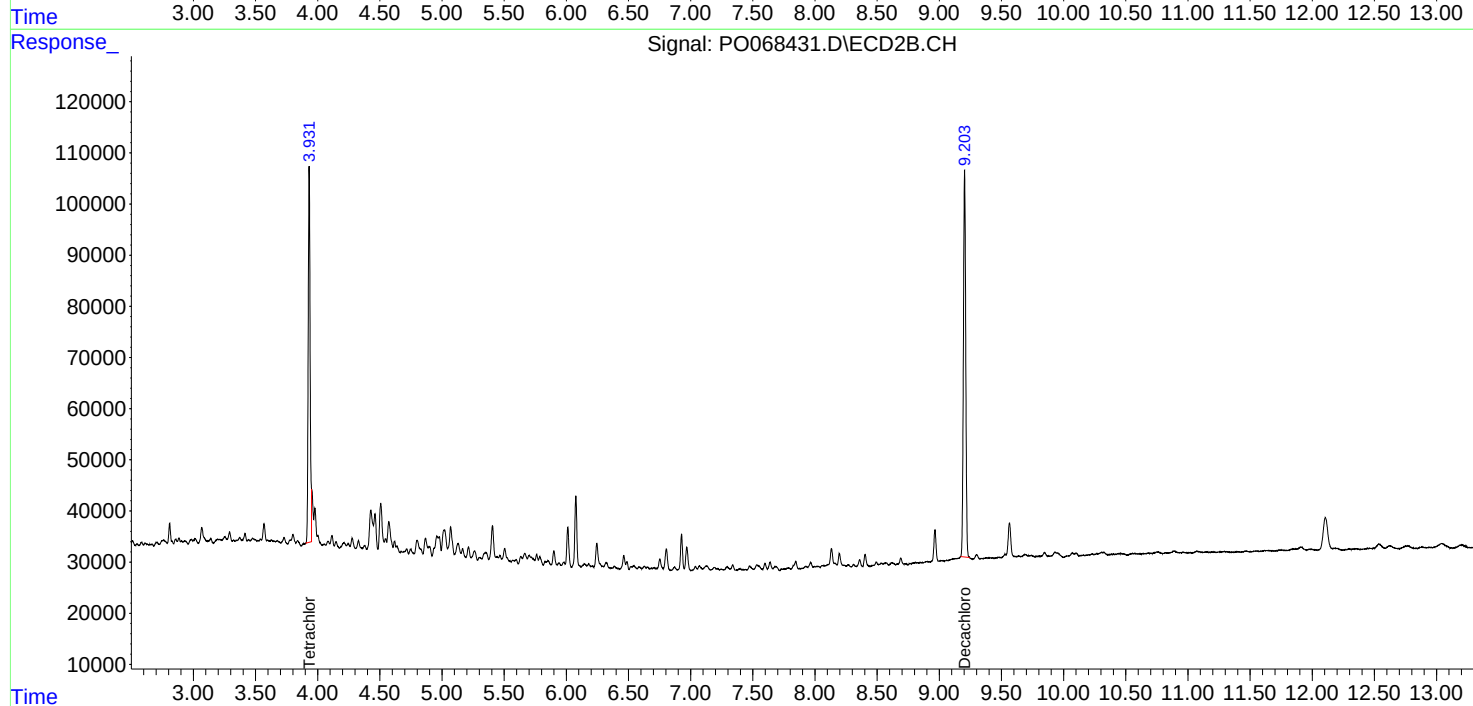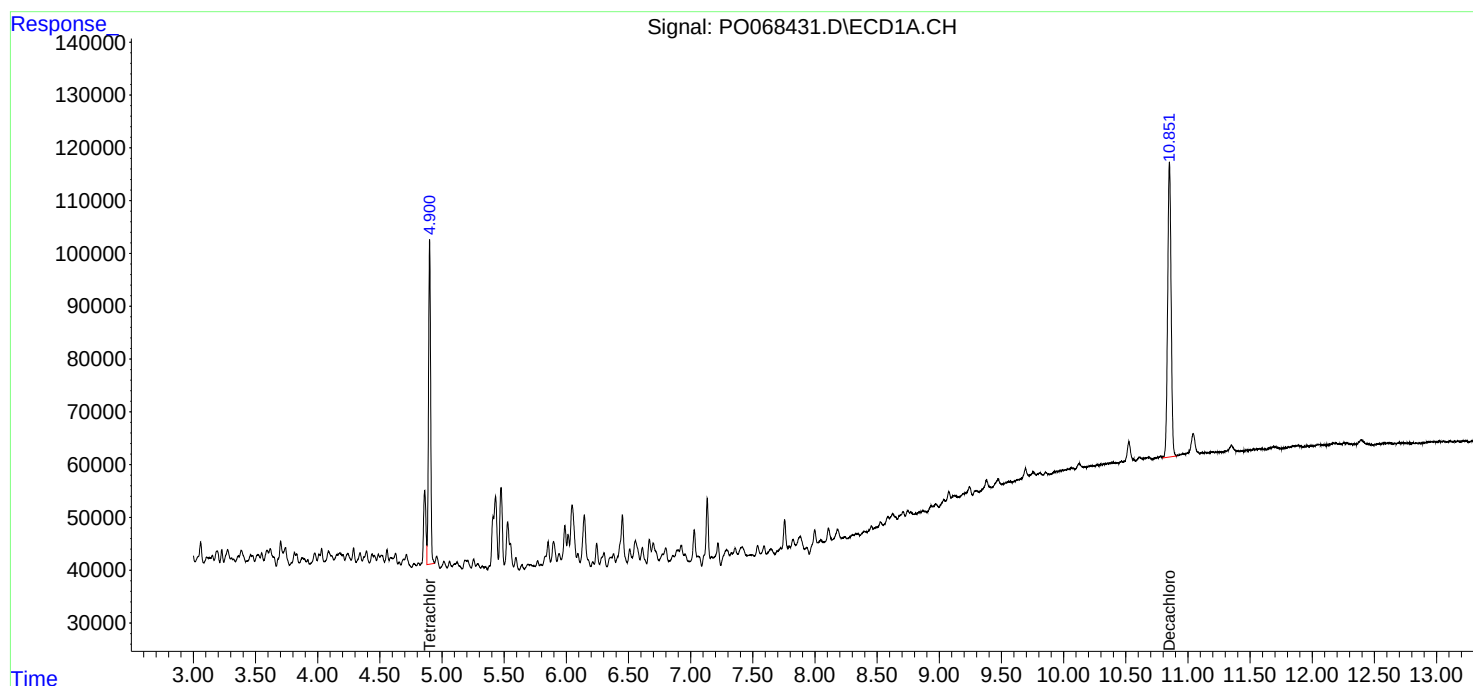


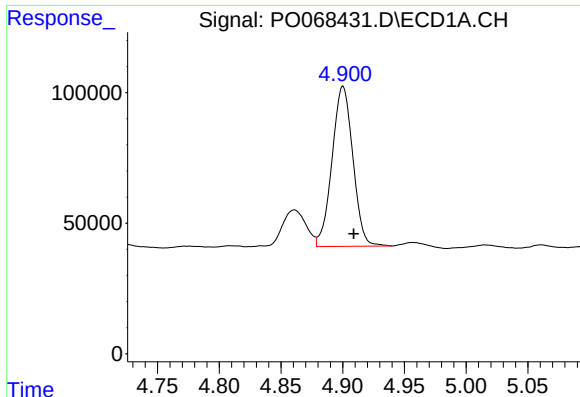

#1 Tetrachloro-m-xylene


R.T.: 4.900 min
Delta R.T.: -0.009 min
Response: 720354
Conc: 25.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
0375-AMENDED-COMP-MP-A

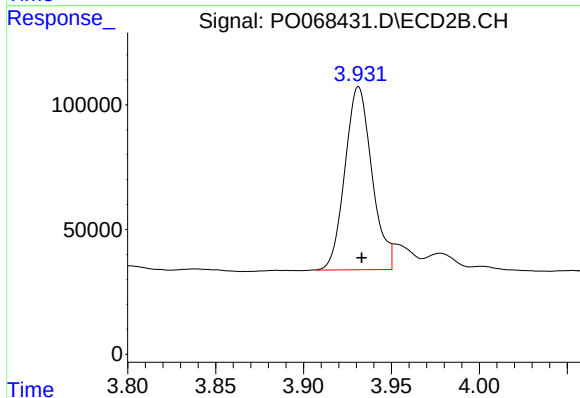


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 785971
Conc: 22.91 ng/ml m

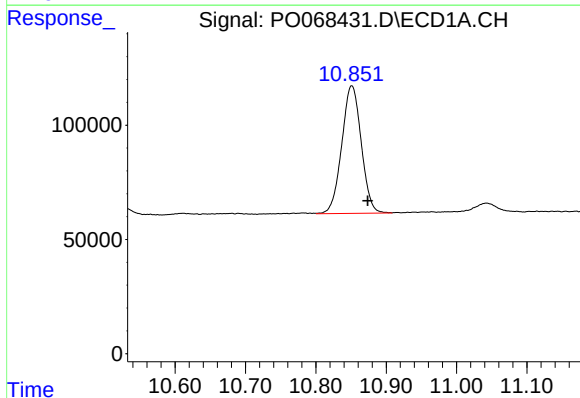

#2 Decachlorobiphenyl

R.T.: 10.851 min
Delta R.T.: -0.023 min
Response: 1074468
Conc: 27.00 ng/ml

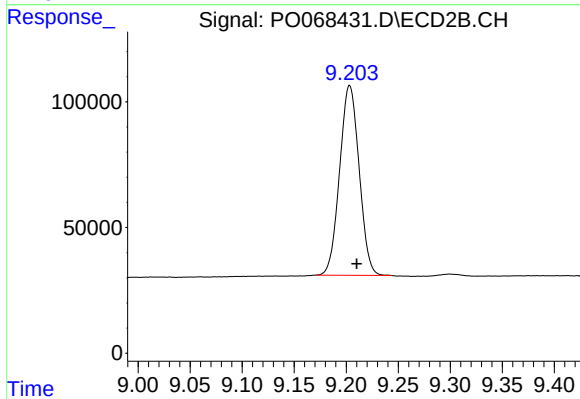

#2 Decachlorobiphenyl

R.T.: 9.203 min
Delta R.T.: -0.007 min
Response: 984518
Conc: 25.57 ng/ml