

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
 Data File : P0068439.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2020 14:27
 Operator : DD\AJ
 Sample : L2663-05 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1378

Manual Integrations
 APPROVED

Sohil
 5/19/2020 11:24:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 22:54:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.930	165477	151313	5.900m	4.410 #
2) SA Decachlor...	10.849	9.203	63748	66094	1.602m	1.717

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
Data File : P0068439.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2020 14:27
Operator : DD\AJ
Sample : L2663-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1378


Manual Integrations
APPROVED

Sohil
5/19/2020 11:24:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 22:54:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

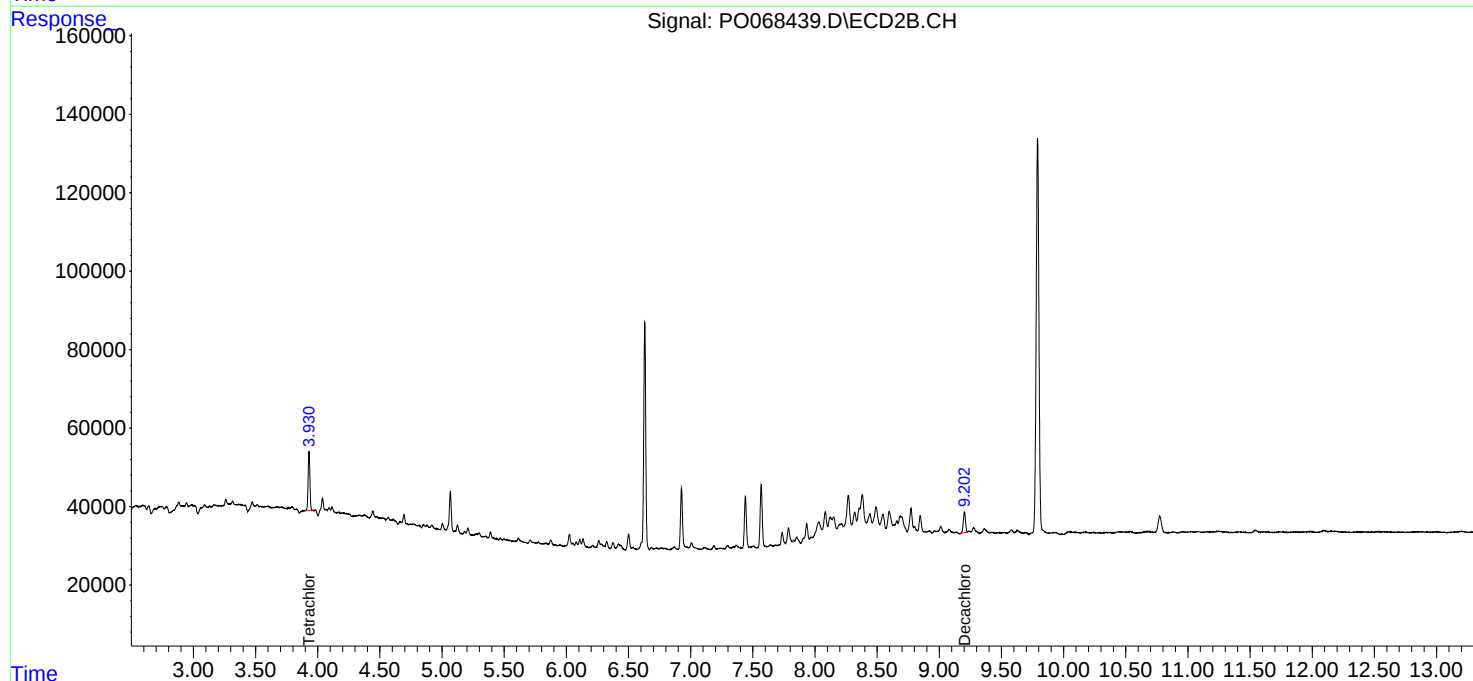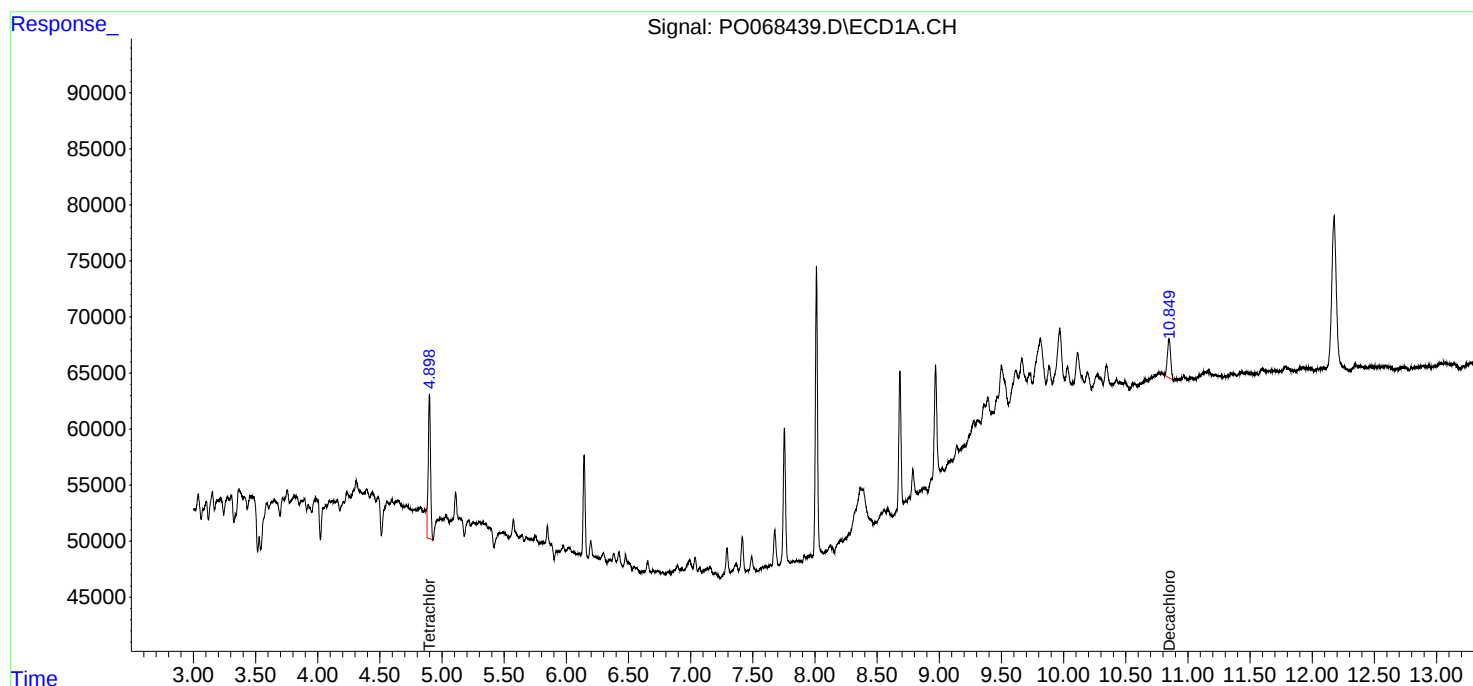

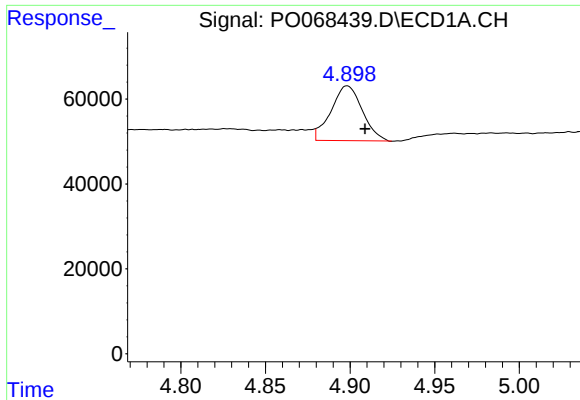


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.011 min
Response: 165477
Conc: 5.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1378


Manual Integrations
APPROVED

Sohil
5/19/2020 11:24:16 AM

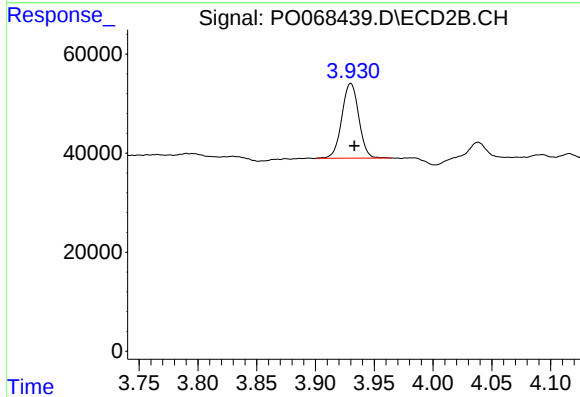


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.003 min
Response: 151313
Conc: 4.41 ng/ml

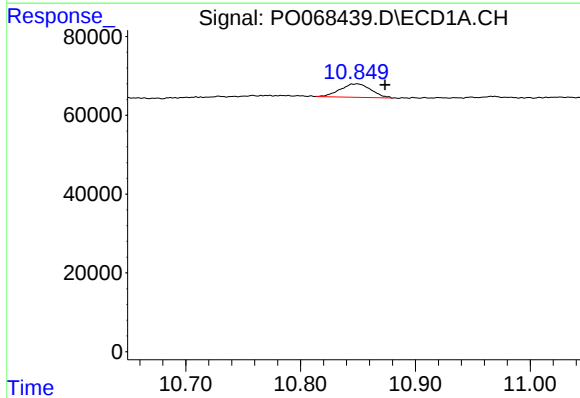

#2 Decachlorobiphenyl

R.T.: 10.849 min
Delta R.T.: -0.025 min
Response: 63748
Conc: 1.60 ng/ml m

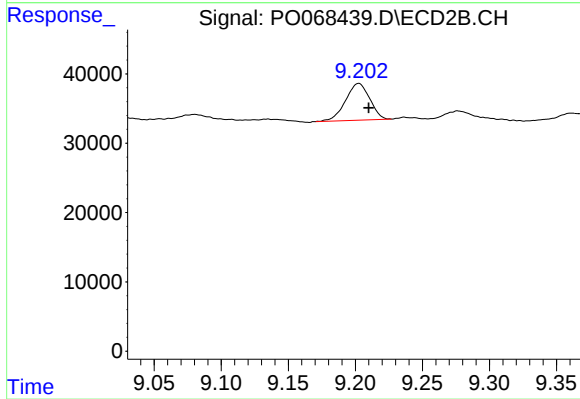

#2 Decachlorobiphenyl

R.T.: 9.203 min
Delta R.T.: -0.007 min
Response: 66094
Conc: 1.72 ng/ml