

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
 Data File : P0068457.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2020 19:20
 Operator : DD\AJ
 Sample : L2665-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-LEACHATE

Manual Integrations
 APPROVED

Sohil
 5/19/2020 11:24:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 22:59:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.931	521012	662626	18.577m	19.311
2) SA Decachlor...	10.848	9.202	870158	868842	21.867	22.568

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051820\
Data File : P0068457.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2020 19:20
Operator : DD\AJ
Sample : L2665-03
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE


Manual Integrations
APPROVED

Sohil
5/19/2020 11:24:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 22:59:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

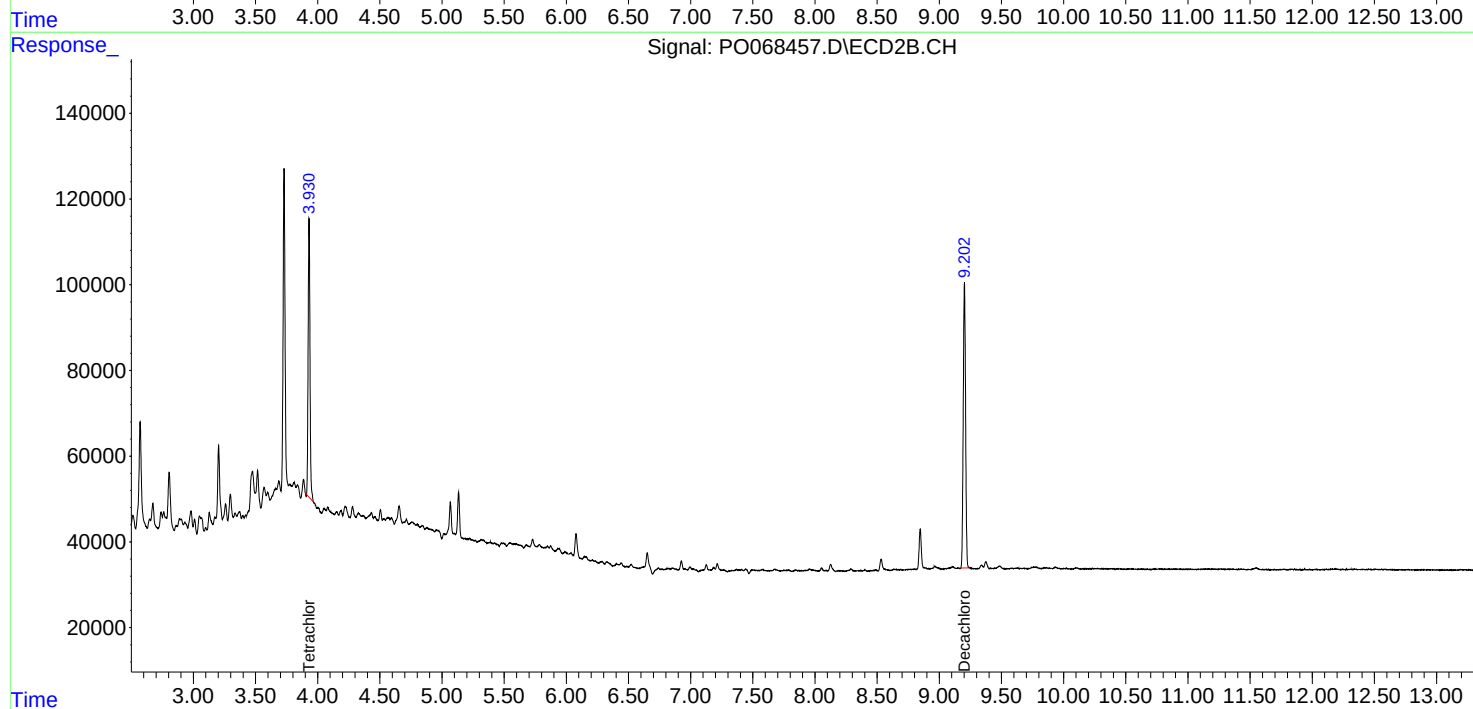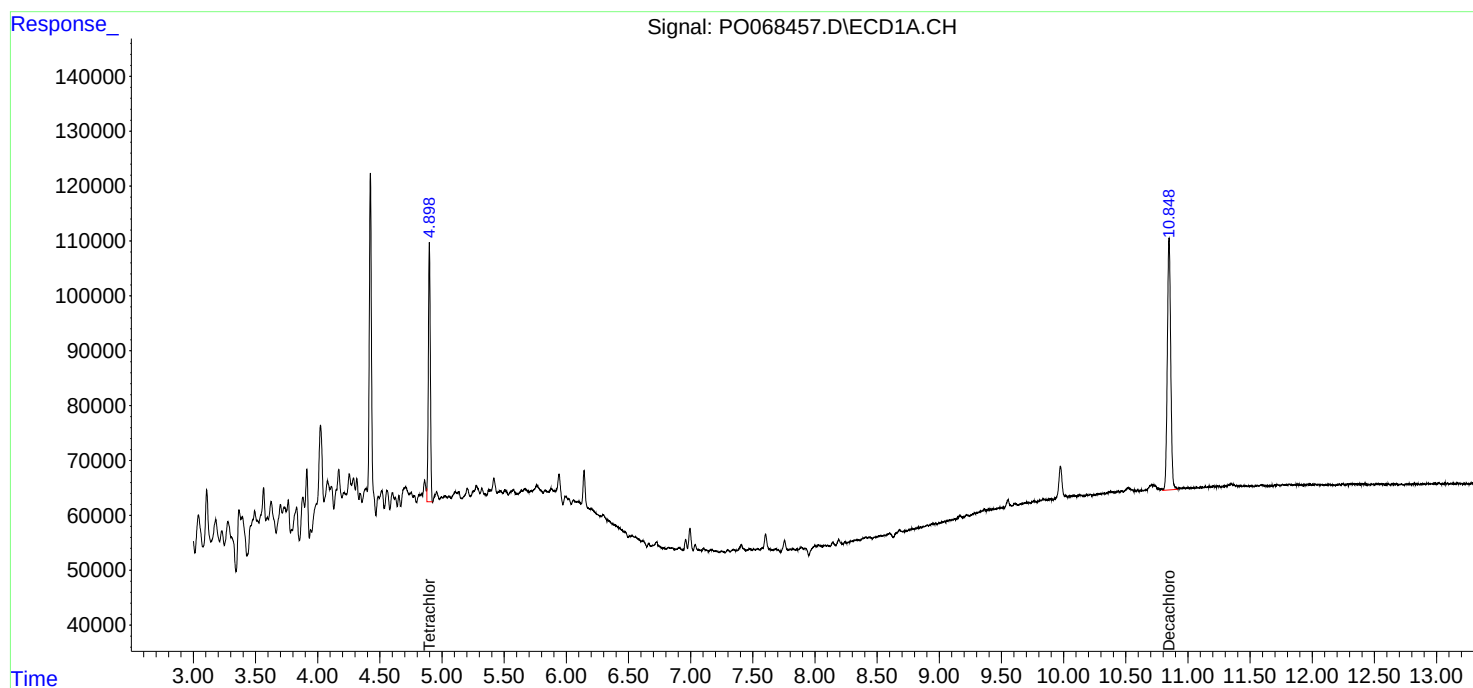

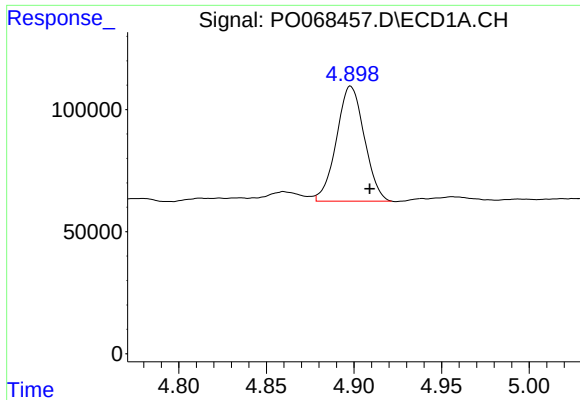


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.011 min
Response: 521012
Conc: 18.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE


Manual Integrations
APPROVED

Sohil
5/19/2020 11:24:26 AM

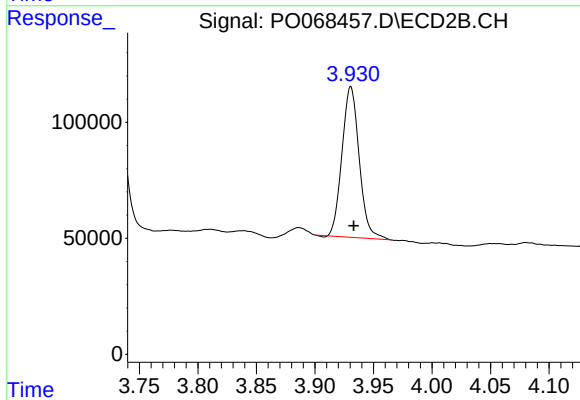


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 662626
Conc: 19.31 ng/ml

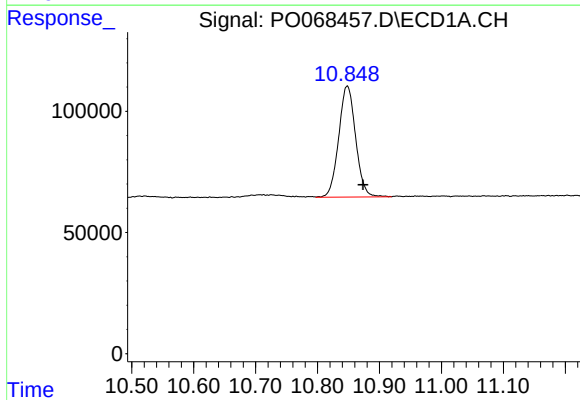

#2 Decachlorobiphenyl

R.T.: 10.848 min
Delta R.T.: -0.026 min
Response: 870158
Conc: 21.87 ng/ml

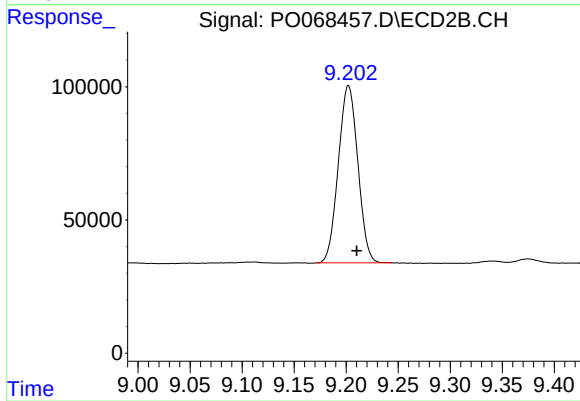

#2 Decachlorobiphenyl

R.T.: 9.202 min
Delta R.T.: -0.008 min
Response: 868842
Conc: 22.57 ng/ml