

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 19:17
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1221 LOD 40PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 03:56:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.259	3.574	428446	392003	14.876	14.535
2)	SA Decachlor...	9.848	8.516	888329	721863	17.409	16.432
Target Compounds							
10)	L2 AR-1221-3	4.631	0.000	35609	0	40.278	N.D. #
11)	L3 AR-1232-1	4.631	0.000	35609	0	31.652	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
Data File : P0056388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 19:17
Operator : SM/SJ
Sample : K2241-07
Misc : AR1221 LOD 40PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 03:56:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

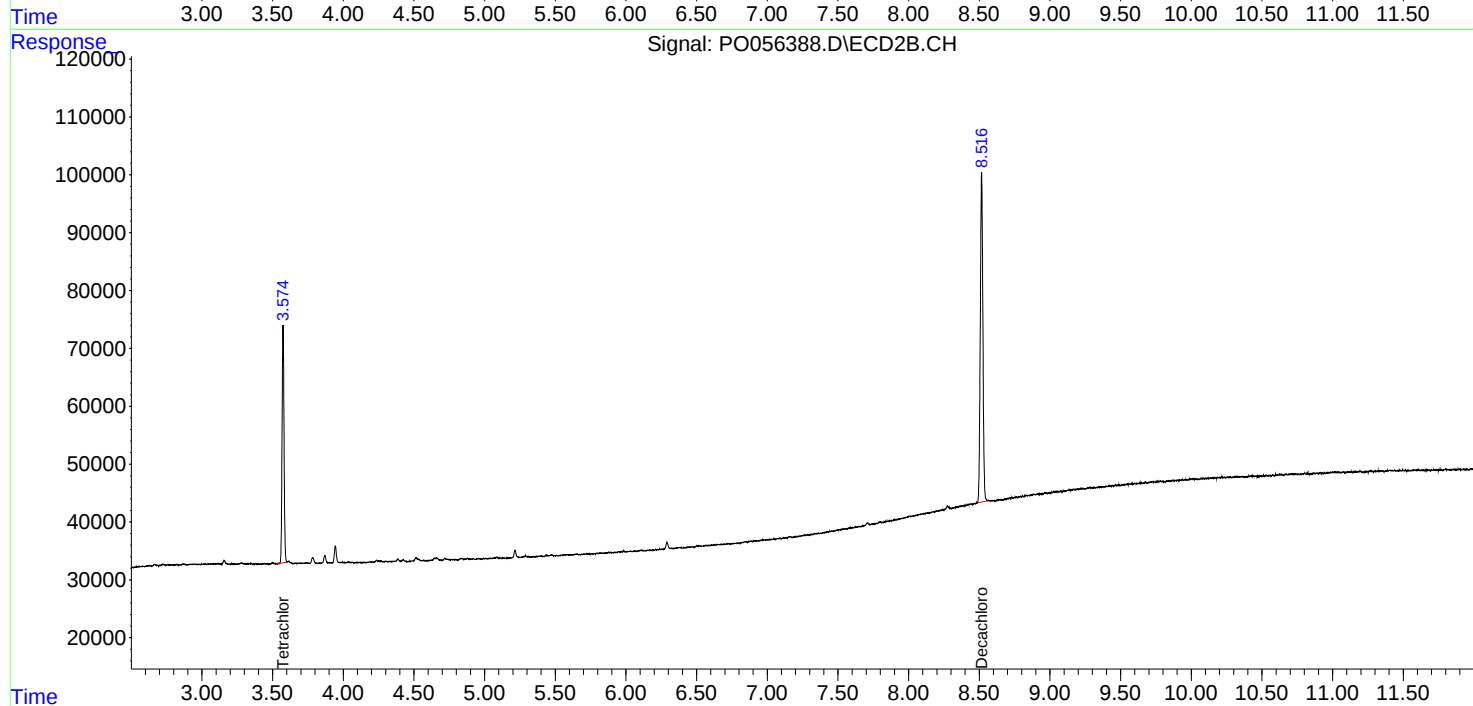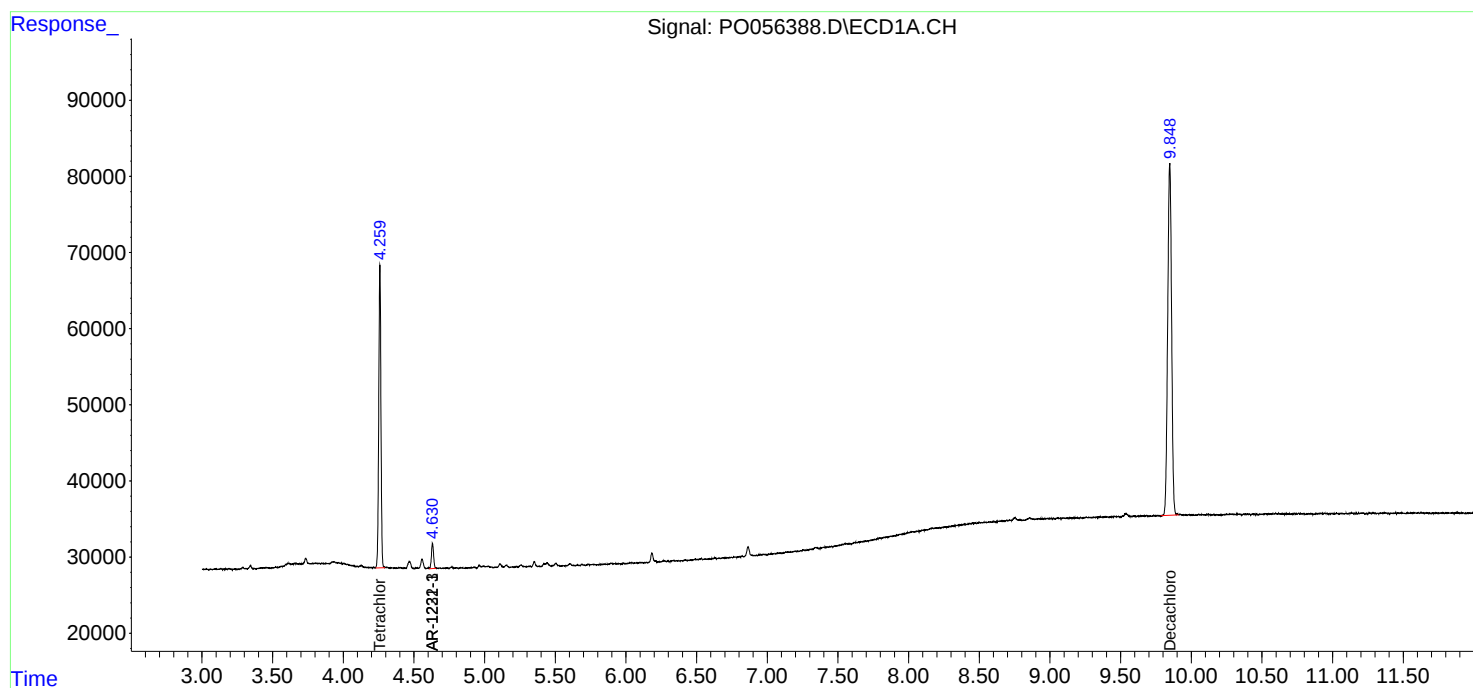


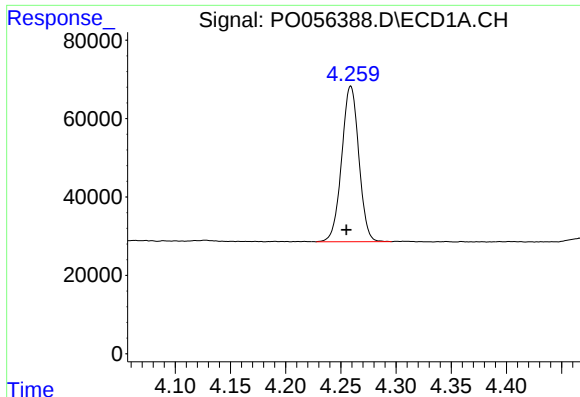

#1 Tetrachloro-m-xylene


R.T.: 4.259 min
Delta R.T.: 0.004 min
Response: 428446
Conc: 14.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

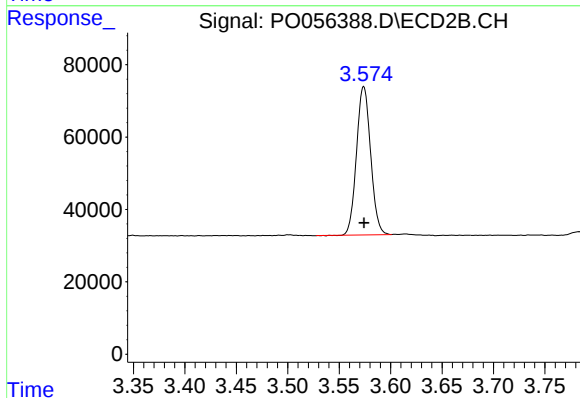


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 392003
Conc: 14.54 ng/ml

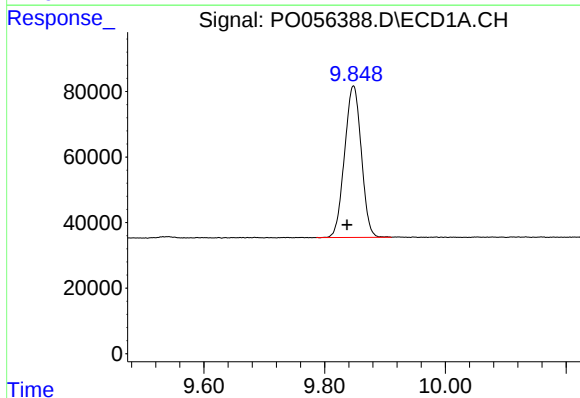


#2 Decachlorobiphenyl

R.T.: 9.848 min
Delta R.T.: 0.011 min
Response: 888329
Conc: 17.41 ng/ml

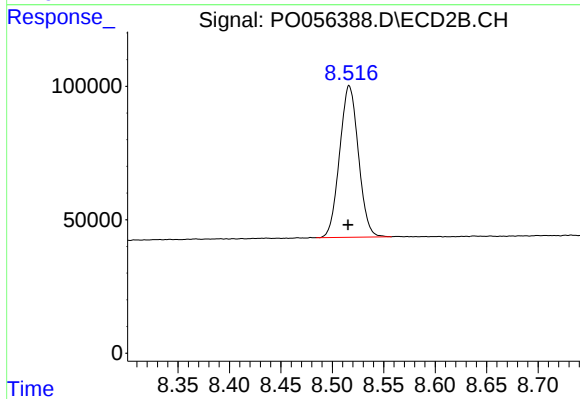

#2 Decachlorobiphenyl


R.T.: 8.516 min
Delta R.T.: 0.001 min
Response: 721863
Conc: 16.43 ng/ml

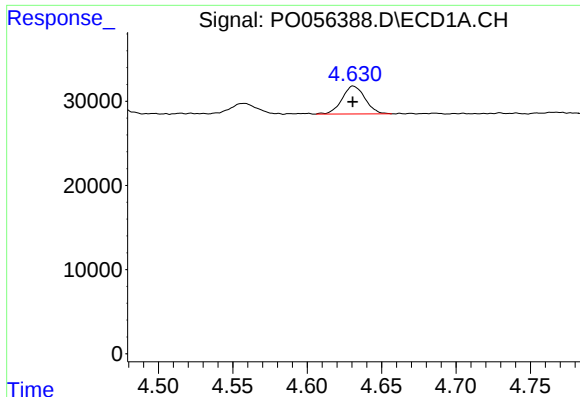

#10 AR-1221-3


R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 35609
Conc: 40.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

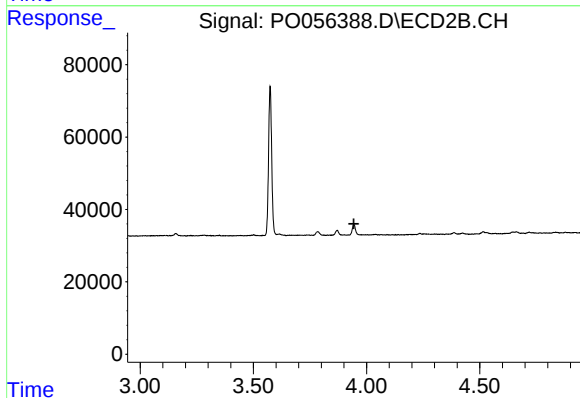


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.944 min
Response: 0
Conc: N.D.

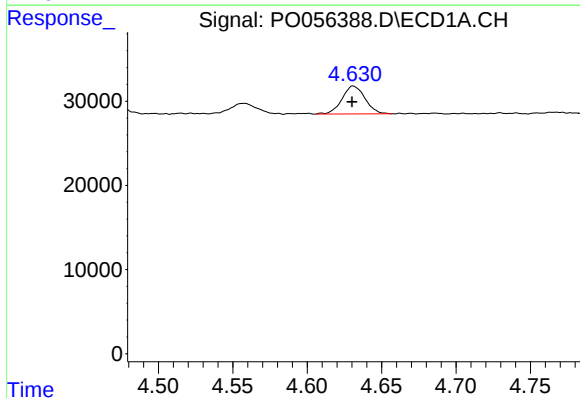

#11 AR-1232-1

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 35609
Conc: 31.65 ng/ml

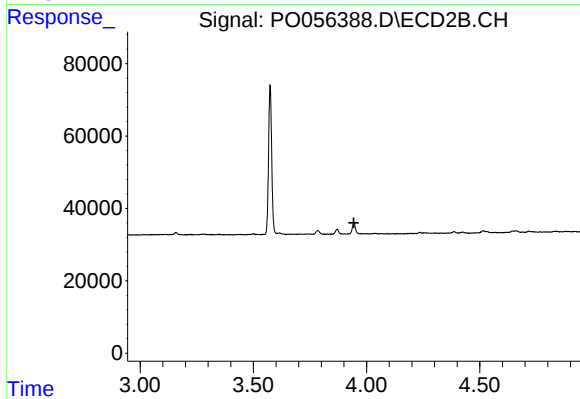

#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.944 min
Response: 0
Conc: N.D.