

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056390.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 19:55
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1232 LOD 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/21/2019 4:49:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 03:56:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.260	3.574	497185	451498	17.263	16.741
2) SA Decachlor...	9.849	8.517	921995	752152	18.069	17.121
Target Compounds						
11) L3 AR-1232-1	4.633	3.943	20142	13280	17.904m	13.492m
12) L3 AR-1232-2	5.156	4.663	10949	18746	16.554m	15.100m
13) L3 AR-1232-3	5.443	4.836	24480	9407	17.222m	13.242m
14) L3 AR-1232-4	5.603	4.917	12125	8258	16.194m	13.338m
15) L3 AR-1232-5	5.692	5.088	7368	11612	12.476m	16.311m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052019\
Data File : PO056390.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 19:55
Operator : SM/SJ
Sample : K2241-07
Misc : AR1232 LOD 25PPB
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 03:56:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

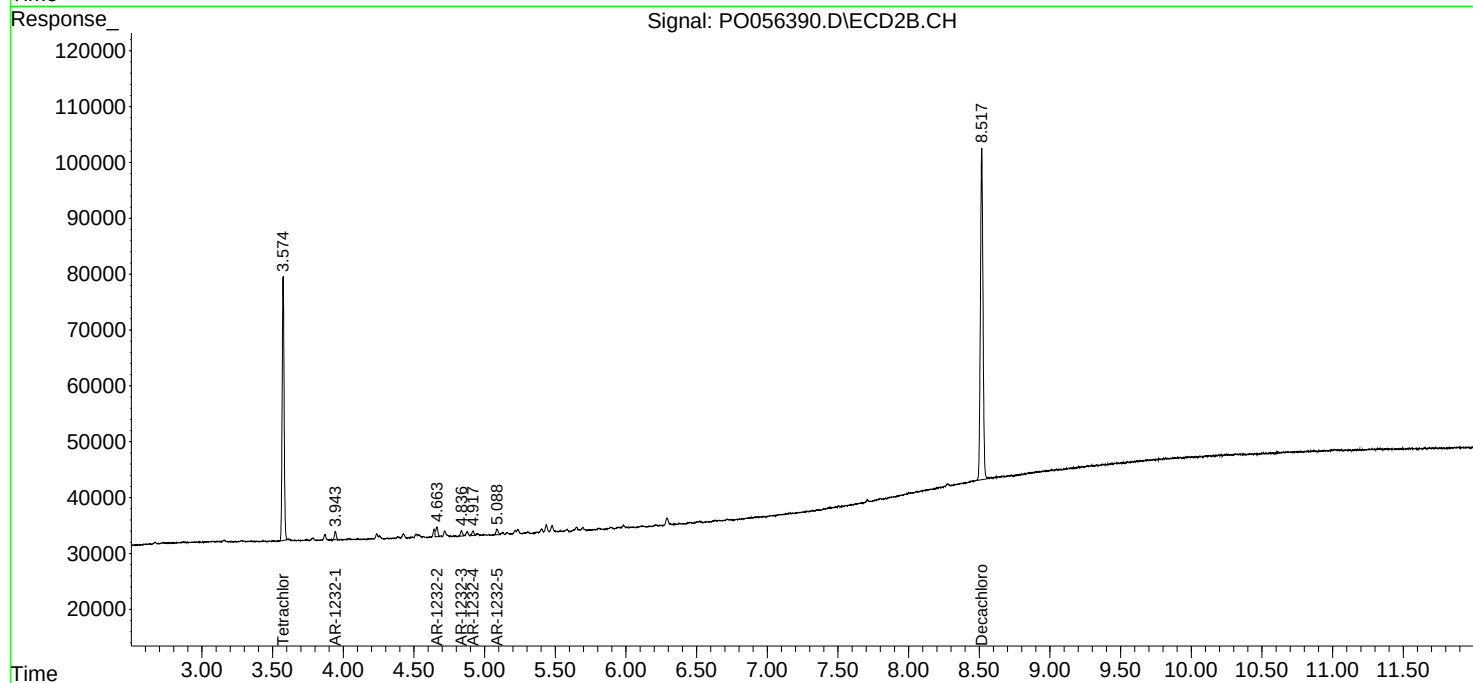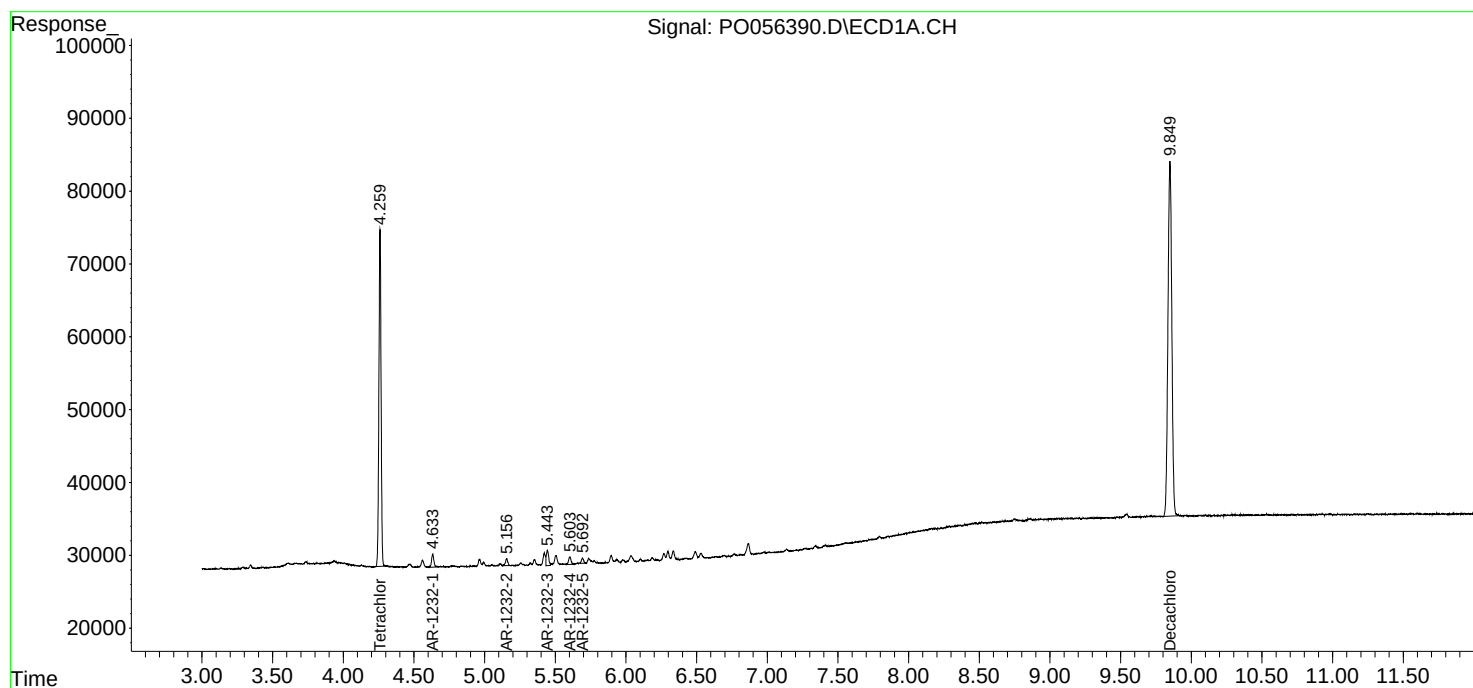

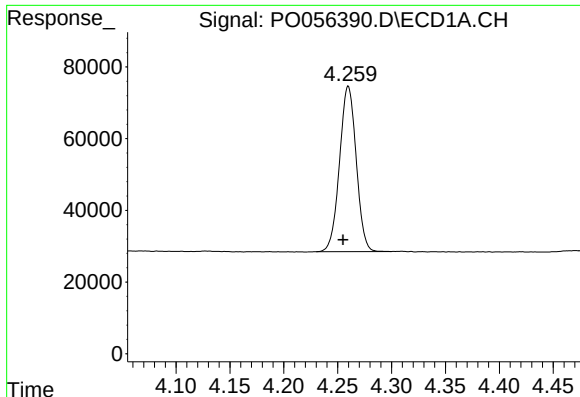


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: 0.005 min
Response: 497185
Conc: 17.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:37 PM

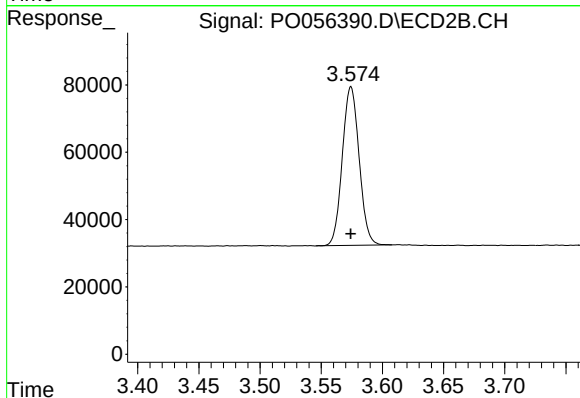


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 451498
Conc: 16.74 ng/ml

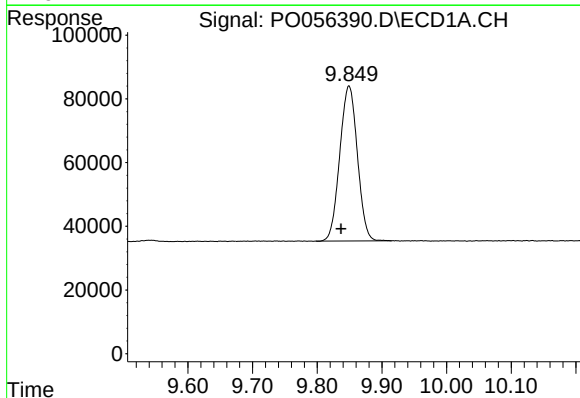


#2 Decachlorobiphenyl

R.T.: 9.849 min
Delta R.T.: 0.012 min
Response: 921995
Conc: 18.07 ng/ml

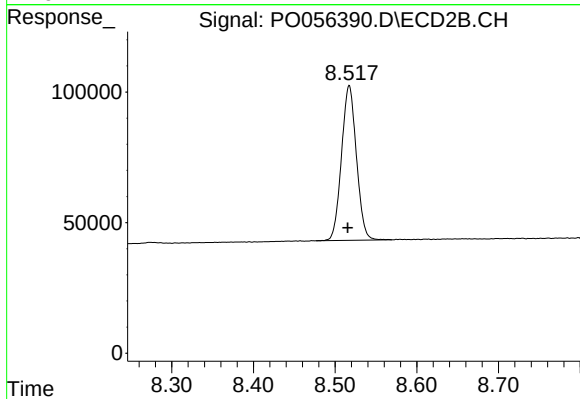

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: 0.002 min
Response: 752152
Conc: 17.12 ng/ml

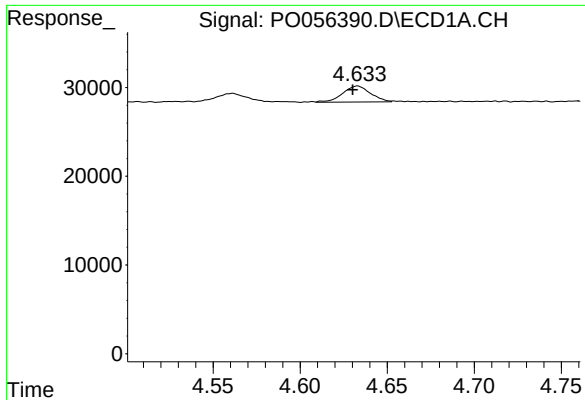


#11 AR-1232-1

R.T.: 4.633 min
Delta R.T.: 0.002 min
Response: 20142
Conc: 17.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:37 PM

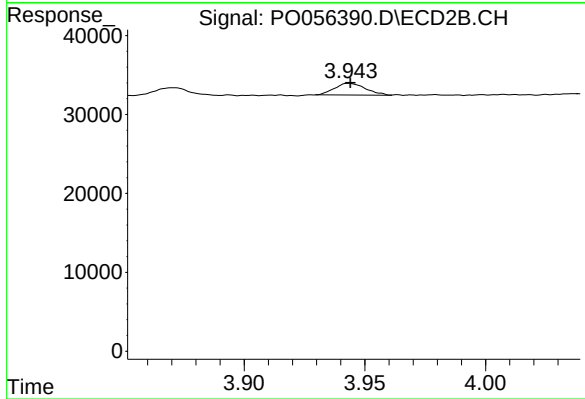


#11 AR-1232-1

R.T.: 3.943 min
Delta R.T.: -0.001 min
Response: 13280
Conc: 13.49 ng/ml m

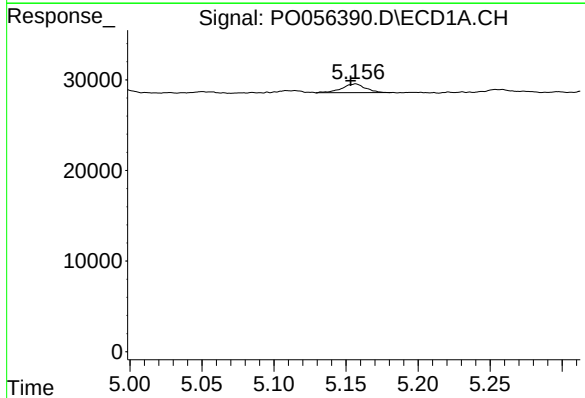


#12 AR-1232-2

R.T.: 5.156 min
Delta R.T.: 0.003 min
Response: 10949
Conc: 16.55 ng/ml m

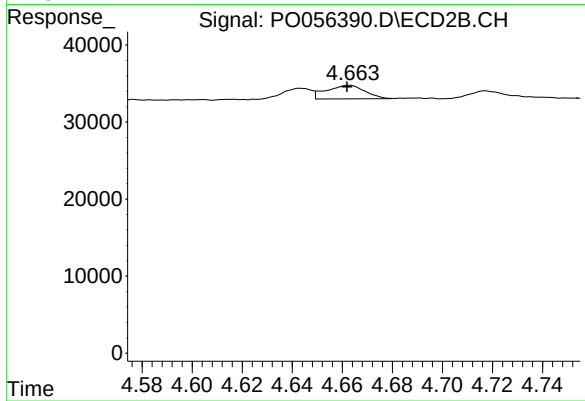

#12 AR-1232-2

R.T.: 4.663 min
Delta R.T.: 0.001 min
Response: 18746
Conc: 15.10 ng/ml m

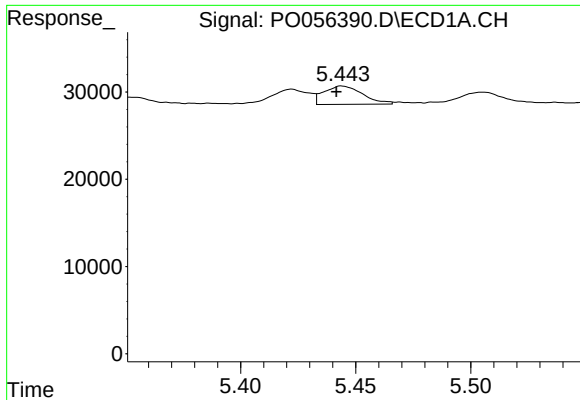


#13 AR-1232-3

R.T.: 5.443 min
Delta R.T.: 0.002 min
Response: 24480
Conc: 17.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:37 PM

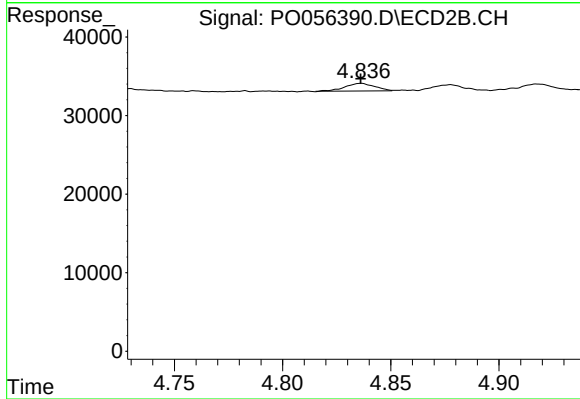


#13 AR-1232-3

R.T.: 4.836 min
Delta R.T.: 0.000 min
Response: 9407
Conc: 13.24 ng/ml m

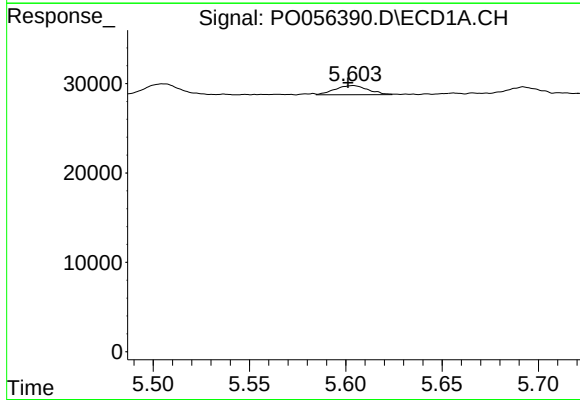


#14 AR-1232-4

R.T.: 5.603 min
Delta R.T.: 0.002 min
Response: 12125
Conc: 16.19 ng/ml m

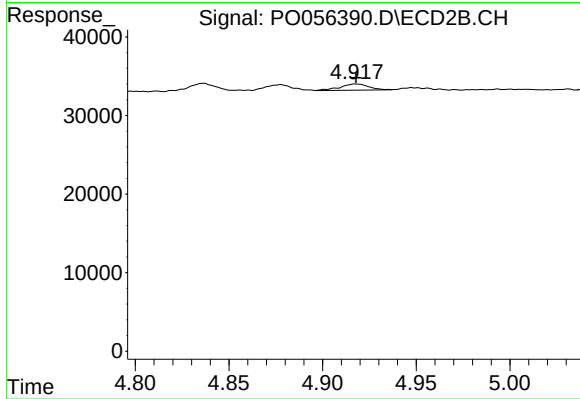

#14 AR-1232-4

R.T.: 4.917 min
Delta R.T.: -0.001 min
Response: 8258
Conc: 13.34 ng/ml m

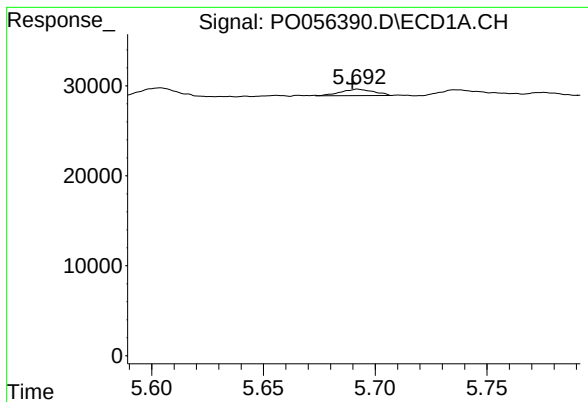


#15 AR-1232-5

R.T.: 5.692 min
Delta R.T.: 0.002 min
Response: 7368
Conc: 12.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:37 PM

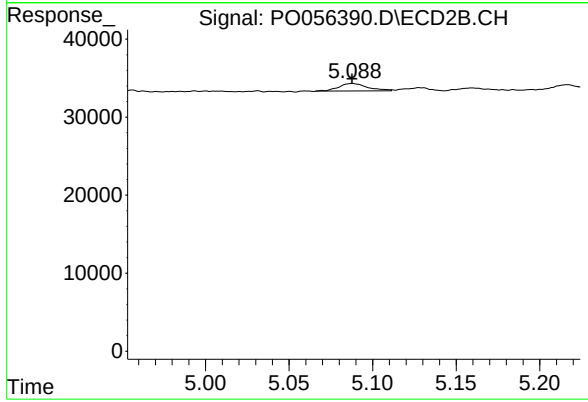

#15 AR-1232-5

R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 11612
Conc: 16.31 ng/ml m