

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056396.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 21:40
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1248 LOD 25PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/21/2019 4:49:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 03:59:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.574	551088	505733	19.135	18.752
2) SA Decachlor...	9.845	8.515	1027790	842459	20.142	19.177
Target Compounds						
21) L5 AR-1248-1	5.421	4.643	25010	18177	27.623m	22.688m
22) L5 AR-1248-2	5.691	4.876	28828	28650	21.887m	26.498m
23) L5 AR-1248-3	5.893	4.917	39383	28703	26.480m	25.503m
24) L5 AR-1248-4	6.296	5.087	49341	35414	27.058	24.875m
25) L5 AR-1248-5	6.334	5.477	46081	33346	26.246	21.775

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052019\
Data File : PO056396.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 21:40
Operator : SM/SJ
Sample : K2241-07
Misc : AR1248 LOD 25PPB
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 03:59:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

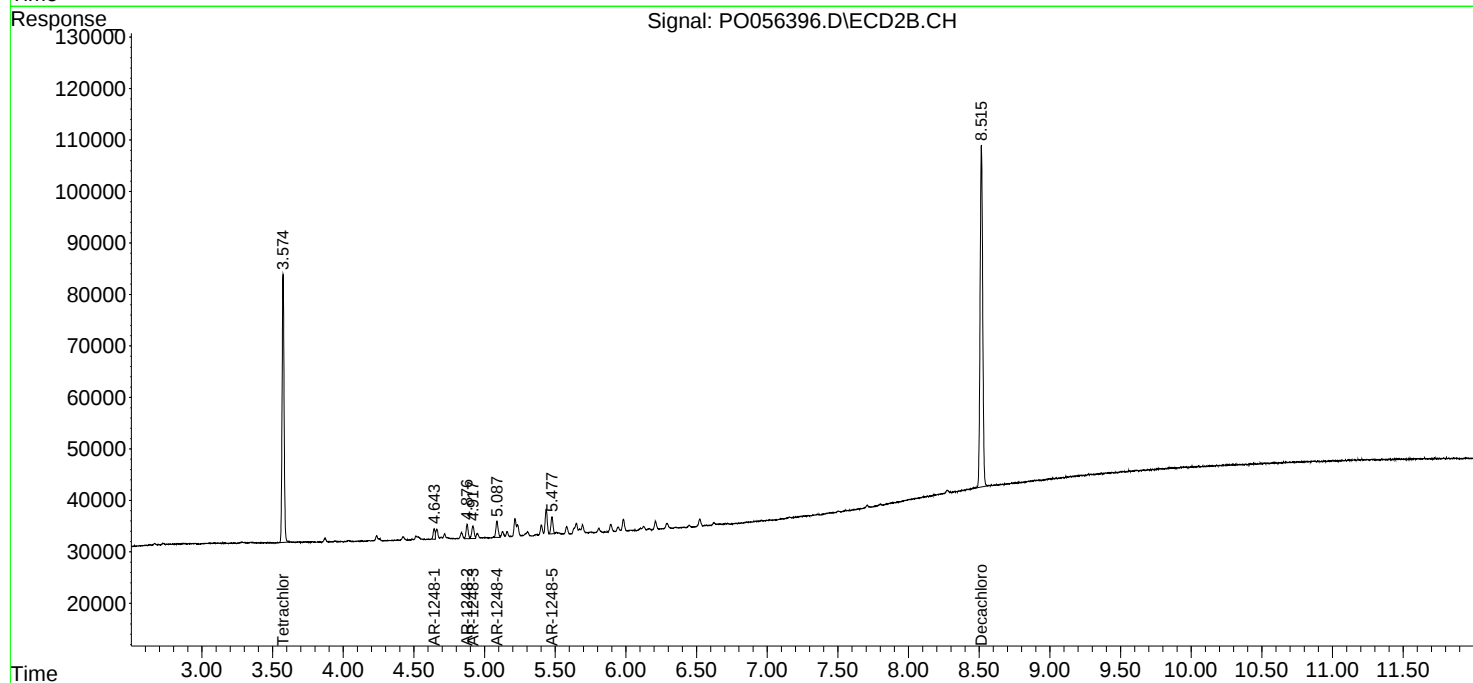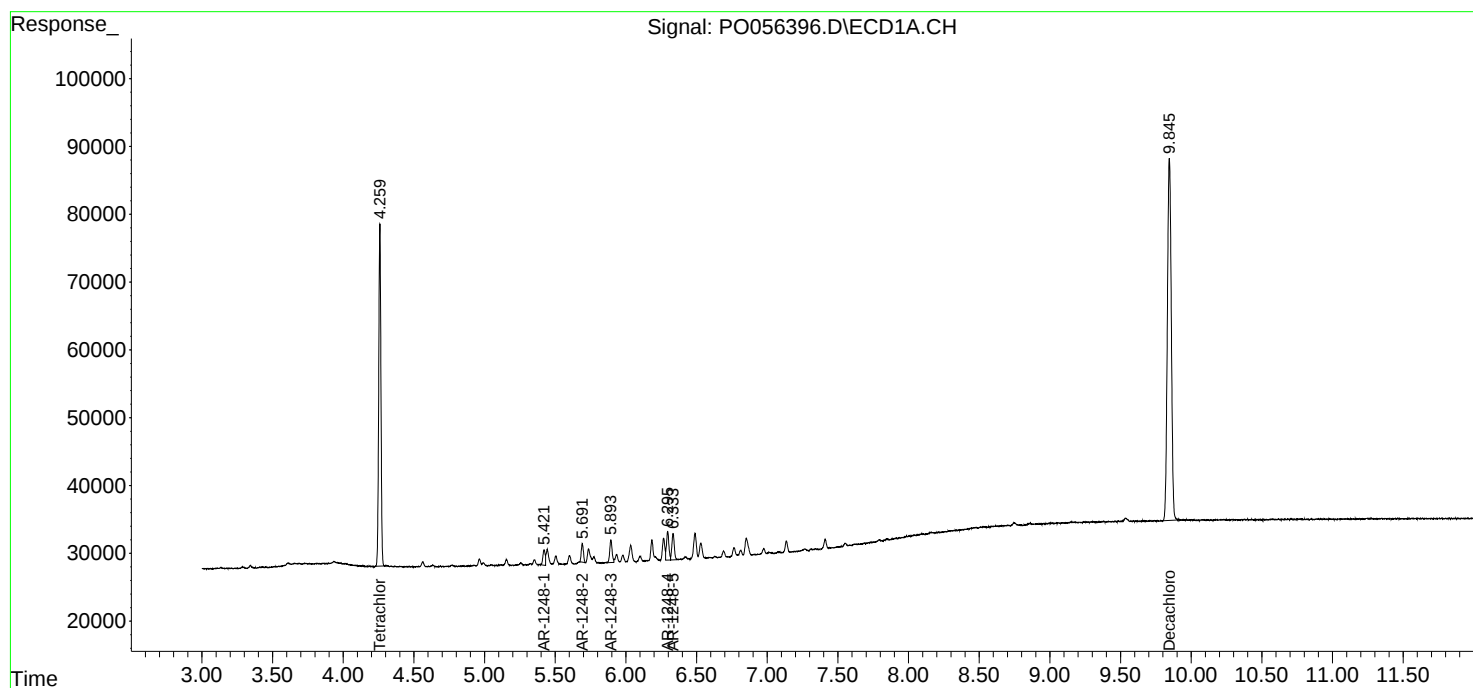

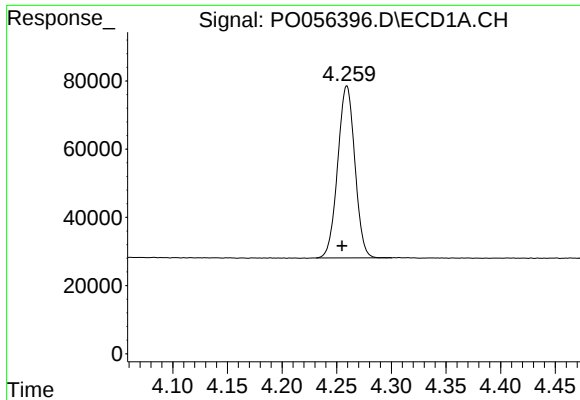


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.004 min
Response: 551088
Conc: 19.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:48 PM

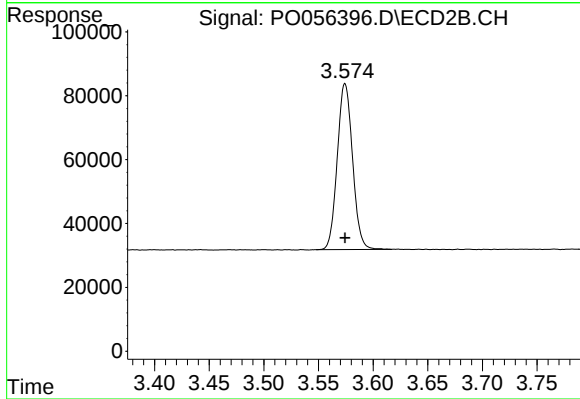


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 505733
Conc: 18.75 ng/ml

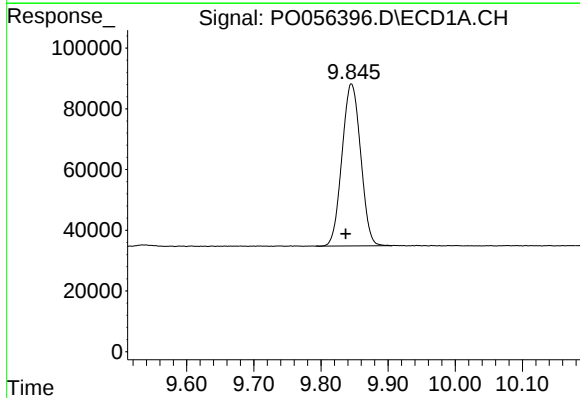


#2 Decachlorobiphenyl

R.T.: 9.845 min
Delta R.T.: 0.008 min
Response: 1027790
Conc: 20.14 ng/ml

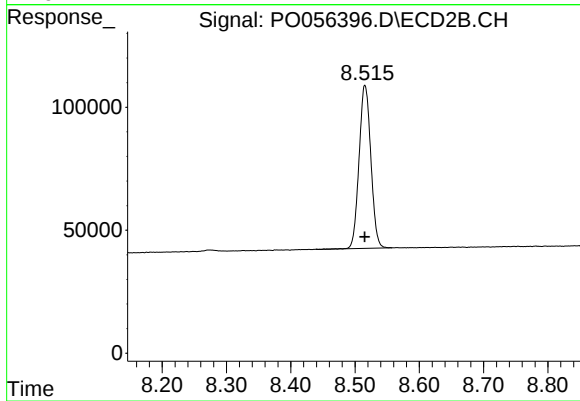

#2 Decachlorobiphenyl

R.T.: 8.515 min
Delta R.T.: 0.000 min
Response: 842459
Conc: 19.18 ng/ml

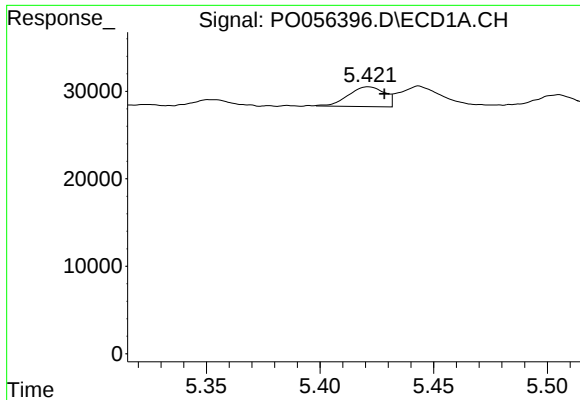


#21 AR-1248-1

R.T.: 5.421 min
Delta R.T.: -0.007 min
Response: 25010
Conc: 27.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:48 PM

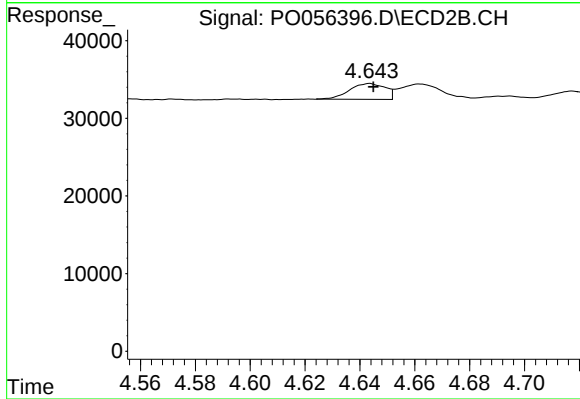


#21 AR-1248-1

R.T.: 4.643 min
Delta R.T.: -0.002 min
Response: 18177
Conc: 22.69 ng/ml m

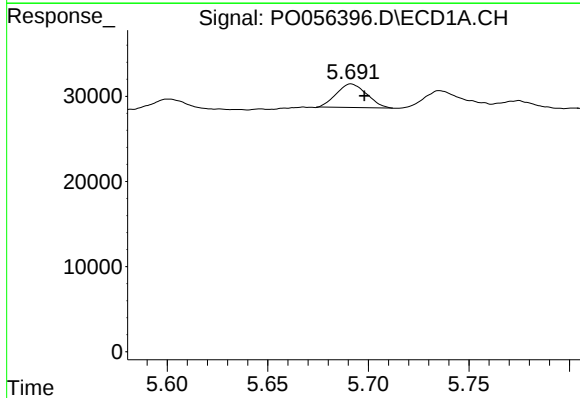


#22 AR-1248-2

R.T.: 5.691 min
Delta R.T.: -0.007 min
Response: 28828
Conc: 21.89 ng/ml m

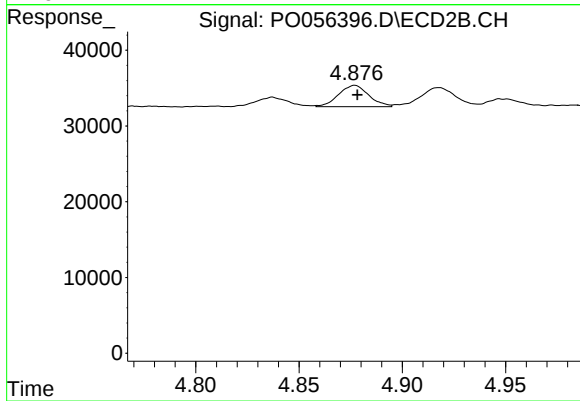

#22 AR-1248-2

R.T.: 4.876 min
Delta R.T.: -0.002 min
Response: 28650
Conc: 26.50 ng/ml m

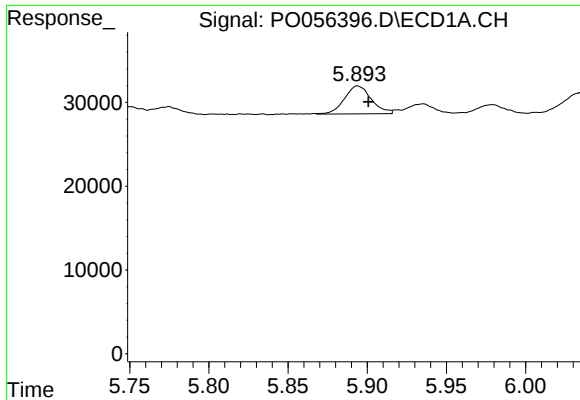


#23 AR-1248-3

R.T.: 5.893 min
Delta R.T.: -0.007 min
Response: 39383
Conc: 26.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:48 PM

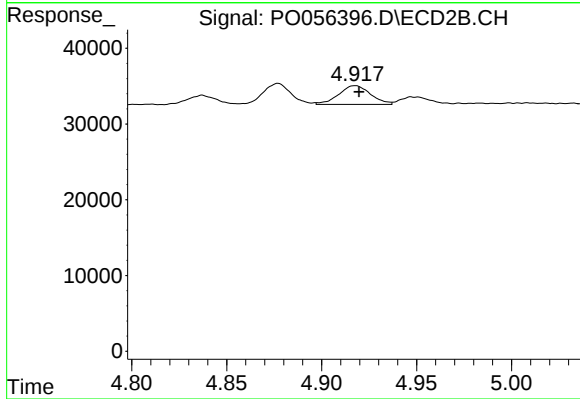


#23 AR-1248-3

R.T.: 4.917 min
Delta R.T.: -0.002 min
Response: 28703
Conc: 25.50 ng/ml m

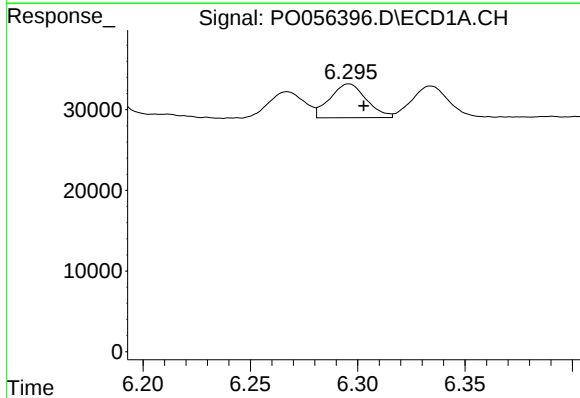


#24 AR-1248-4

R.T.: 6.296 min
Delta R.T.: -0.007 min
Response: 49341
Conc: 27.06 ng/ml

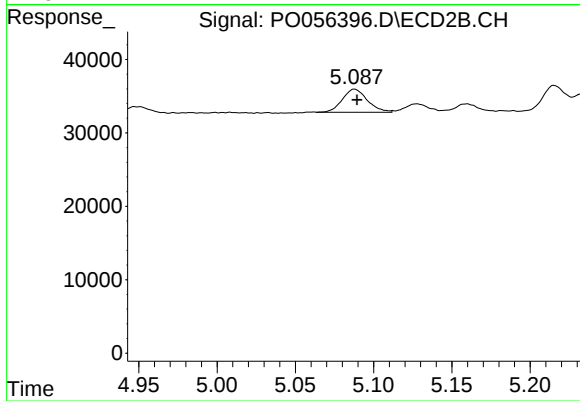

#24 AR-1248-4

R.T.: 5.087 min
Delta R.T.: -0.002 min
Response: 35414
Conc: 24.87 ng/ml m

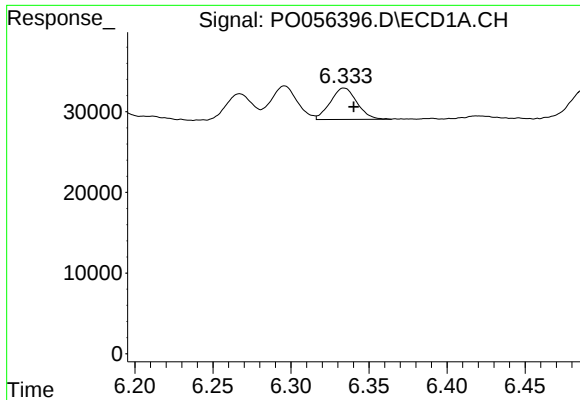


#25 AR-1248-5

R.T.: 6.334 min
Delta R.T.: -0.006 min
Response: 46081
Conc: 26.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:48 PM

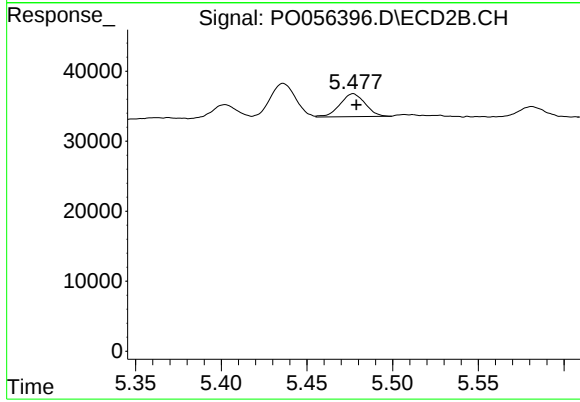

#25 AR-1248-5

R.T.: 5.477 min
Delta R.T.: -0.002 min
Response: 33346
Conc: 21.78 ng/ml