

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056399.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 22:32
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1254 LOD 25PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/21/2019 4:49:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:01:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.259	3.575	467139	432690	16.220	16.044
2)	SA Decachlor...	9.846	8.516	909705	744006	17.828	16.936
Target Compounds							
26)	L6 AR-1254-1	6.267	5.436	50113	48389	21.426m	16.084
27)	L6 AR-1254-2	6.485	5.583	73058	48176	19.527	17.845
28)	L6 AR-1254-3	6.851	5.983	85247	78000	20.357	16.913m
29)	L6 AR-1254-4	7.135	6.210	60396	50786	18.567	16.781m
30)	L6 AR-1254-5	7.551	6.624	65196	62199	18.434m	14.388m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052019\
Data File : PO056399.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 22:32
Operator : SM/SJ
Sample : K2241-07
Misc : AR1254 LOD 25PPB
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:01:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

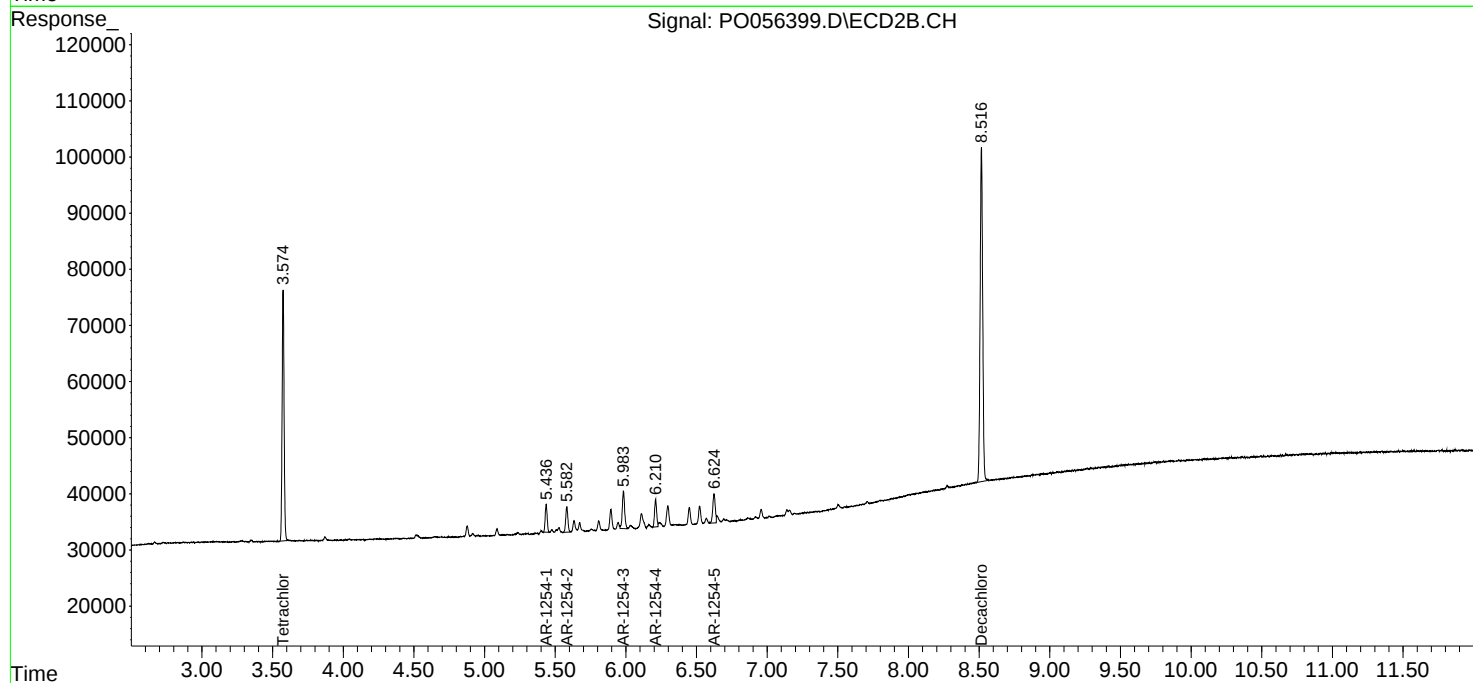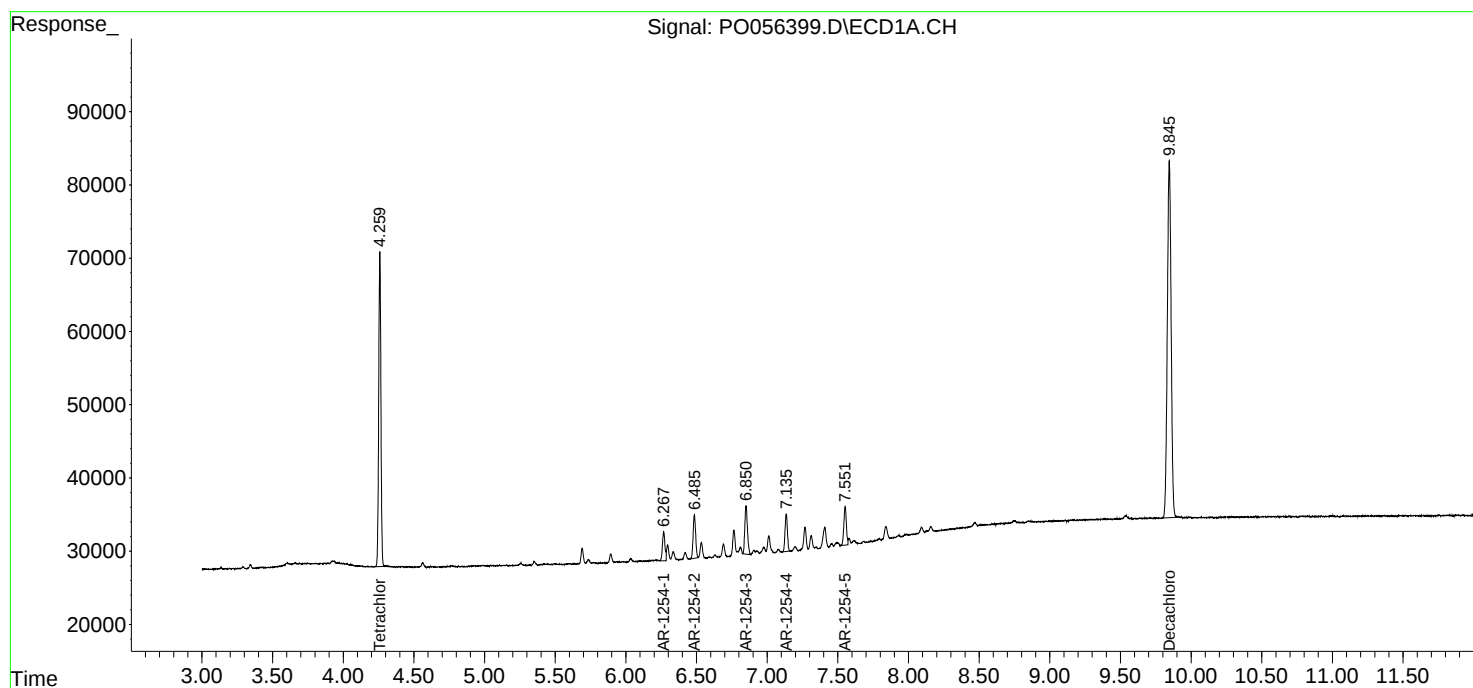

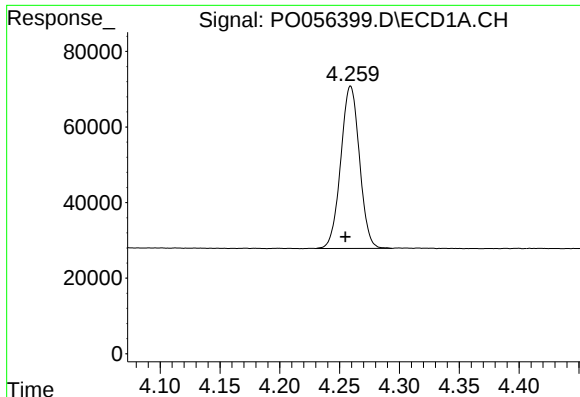


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.004 min
Response: 467139
Conc: 16.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:53 PM

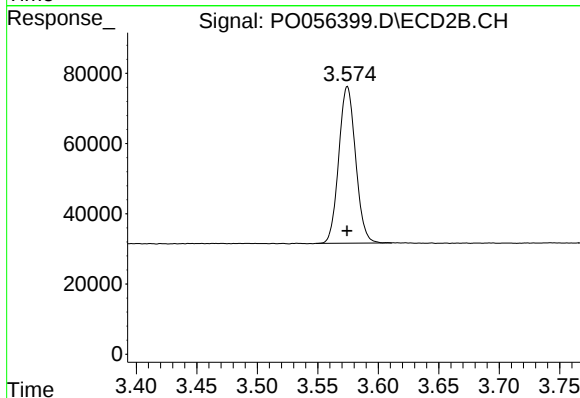


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.000 min
Response: 432690
Conc: 16.04 ng/ml

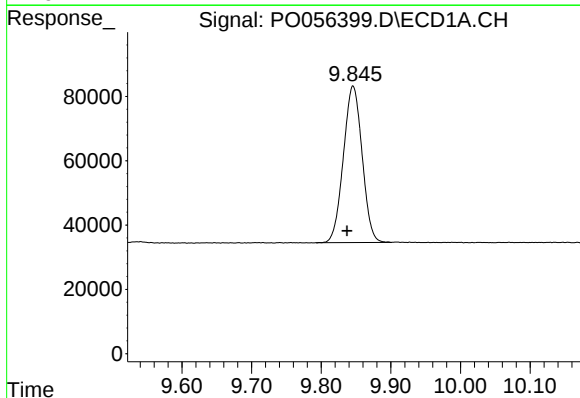


#2 Decachlorobiphenyl

R.T.: 9.846 min
Delta R.T.: 0.009 min
Response: 909705
Conc: 17.83 ng/ml

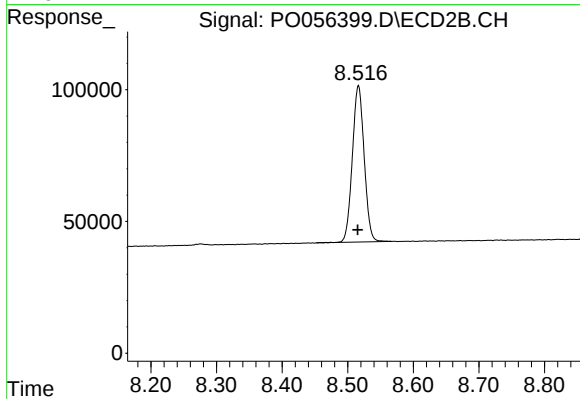

#2 Decachlorobiphenyl

R.T.: 8.516 min
Delta R.T.: 0.001 min
Response: 744006
Conc: 16.94 ng/ml

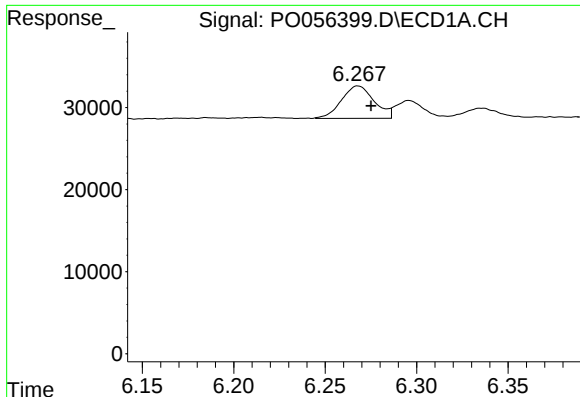


#26 AR-1254-1

R.T.: 6.267 min
Delta R.T.: -0.008 min
Response: 50113
Conc: 21.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:53 PM

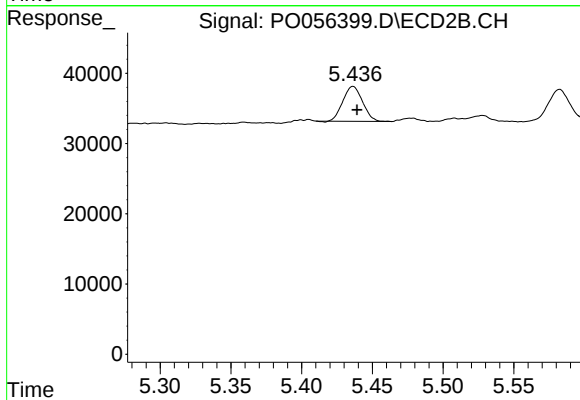


#26 AR-1254-1

R.T.: 5.436 min
Delta R.T.: -0.003 min
Response: 48389
Conc: 16.08 ng/ml

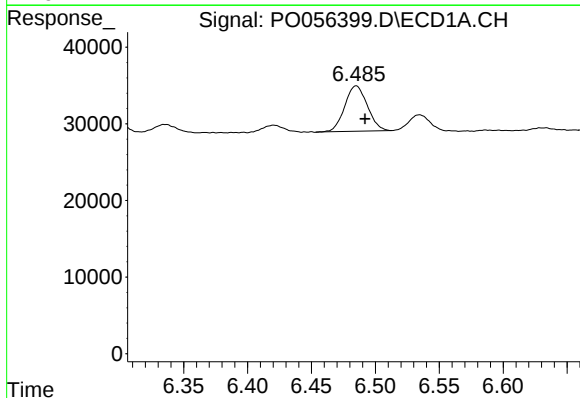


#27 AR-1254-2

R.T.: 6.485 min
Delta R.T.: -0.007 min
Response: 73058
Conc: 19.53 ng/ml

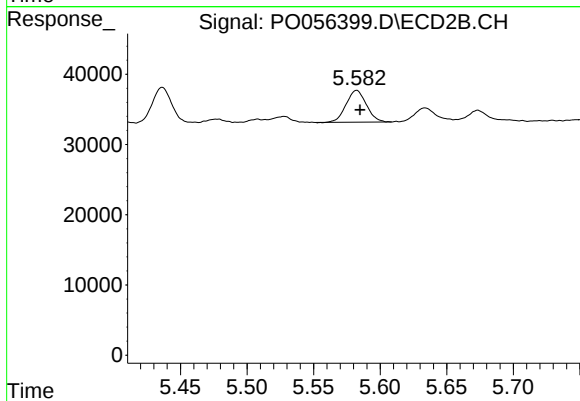

#27 AR-1254-2

R.T.: 5.583 min
Delta R.T.: -0.002 min
Response: 48176
Conc: 17.85 ng/ml

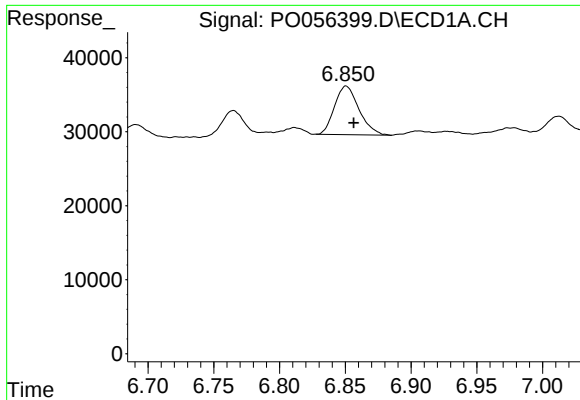


#28 AR-1254-3

R.T.: 6.851 min
Delta R.T.: -0.006 min
Response: 85247
Conc: 20.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:53 PM

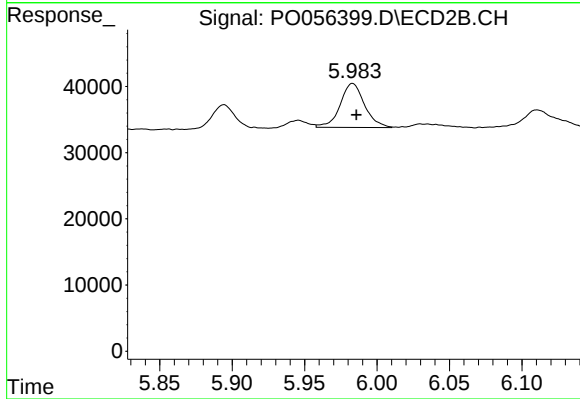


#28 AR-1254-3

R.T.: 5.983 min
Delta R.T.: -0.003 min
Response: 78000
Conc: 16.91 ng/ml m

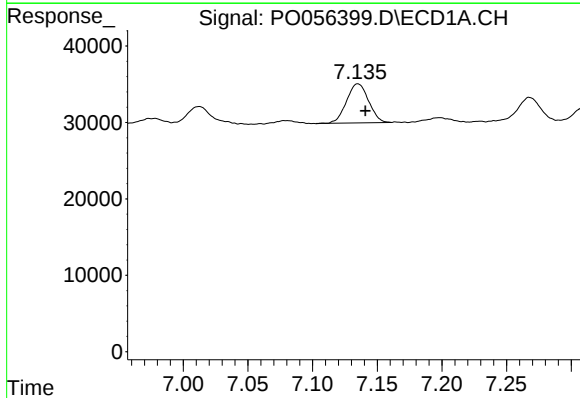


#29 AR-1254-4

R.T.: 7.135 min
Delta R.T.: -0.006 min
Response: 60396
Conc: 18.57 ng/ml

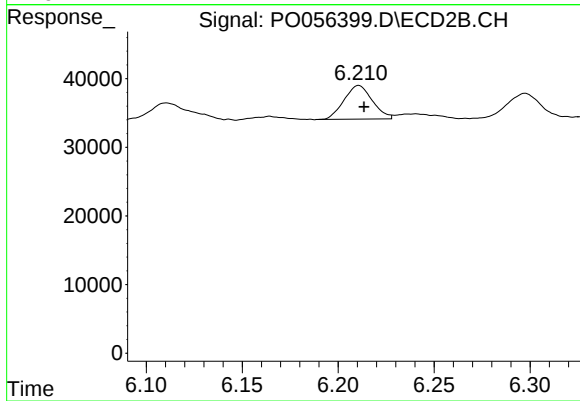

#29 AR-1254-4

R.T.: 6.210 min
Delta R.T.: -0.003 min
Response: 50786
Conc: 16.78 ng/ml m

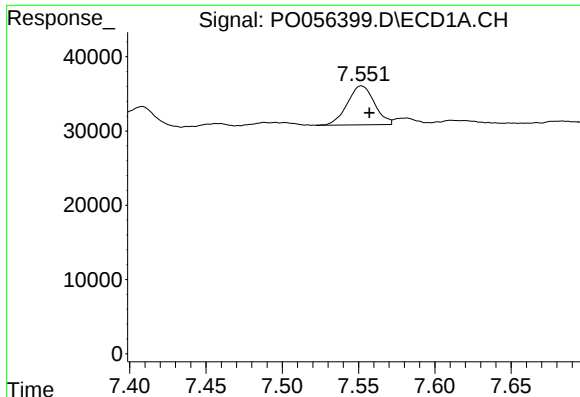


#30 AR-1254-5

R.T.: 7.551 min
Delta R.T.: -0.005 min
Response: 65196
Conc: 18.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:53 PM

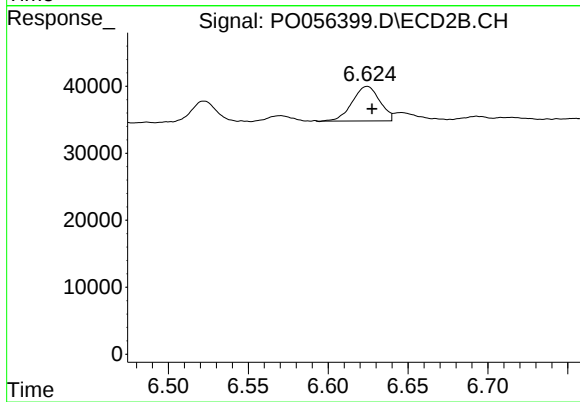

#30 AR-1254-5

R.T.: 6.624 min
Delta R.T.: -0.003 min
Response: 62199
Conc: 14.39 ng/ml m