

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056402.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 23:23
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1262 LOD 25PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/21/2019 4:49:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:02:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.574	514608	476386	17.868	17.664
2) SA Decachlor...	9.844	8.515	987376	806624	19.350	18.361
Target Compounds						
36) L8 AR-1262-1	7.624	6.660	97208	103857	28.395m	26.929
37) L8 AR-1262-2	8.158	7.159	156554	165974	26.192	25.027
38) L8 AR-1262-3	8.450	7.439	110428	68633	26.770	24.959m
39) L8 AR-1262-4	8.536	7.504	85082	117837	27.011	24.798
40) L8 AR-1262-5	9.153	7.996	53005	47765	25.083	22.406

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052019\
Data File : PO056402.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 23:23
Operator : SM/SJ
Sample : K2241-07
Misc : AR1262 LOD 25PPB
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:02:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

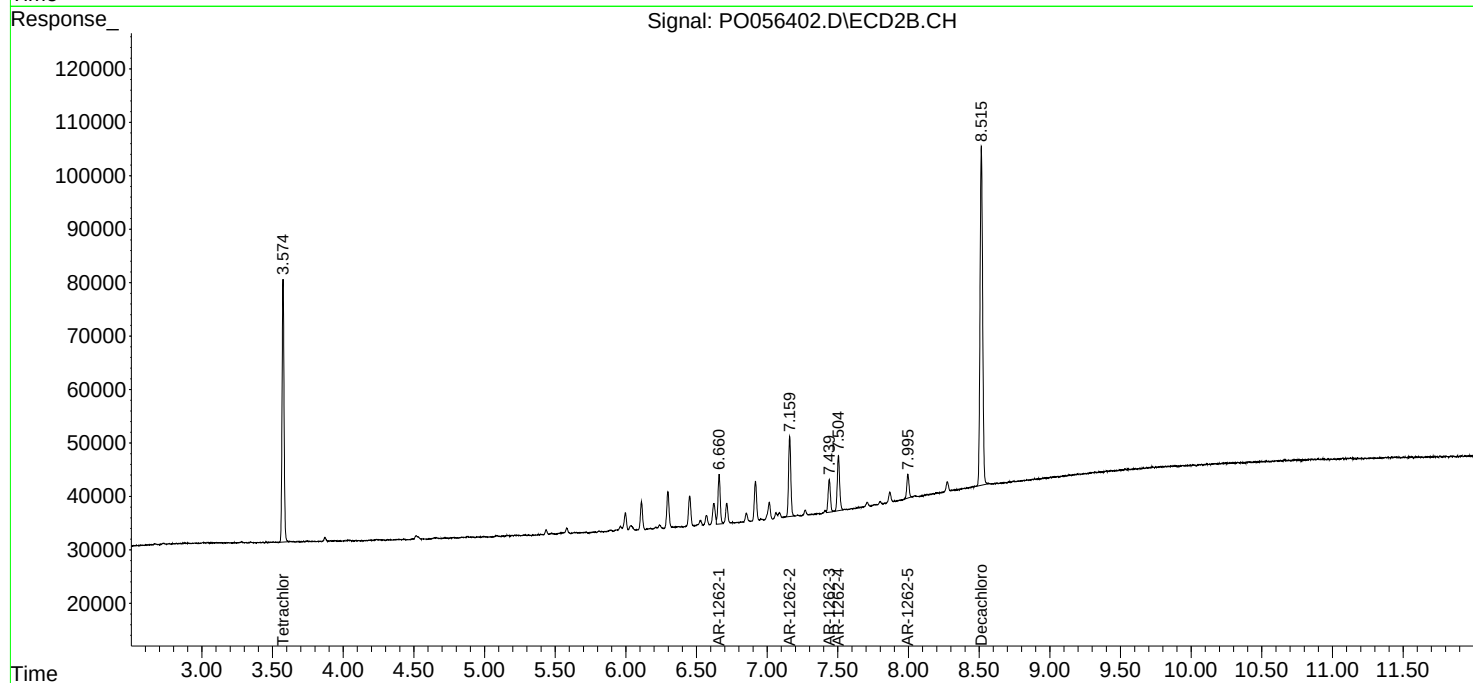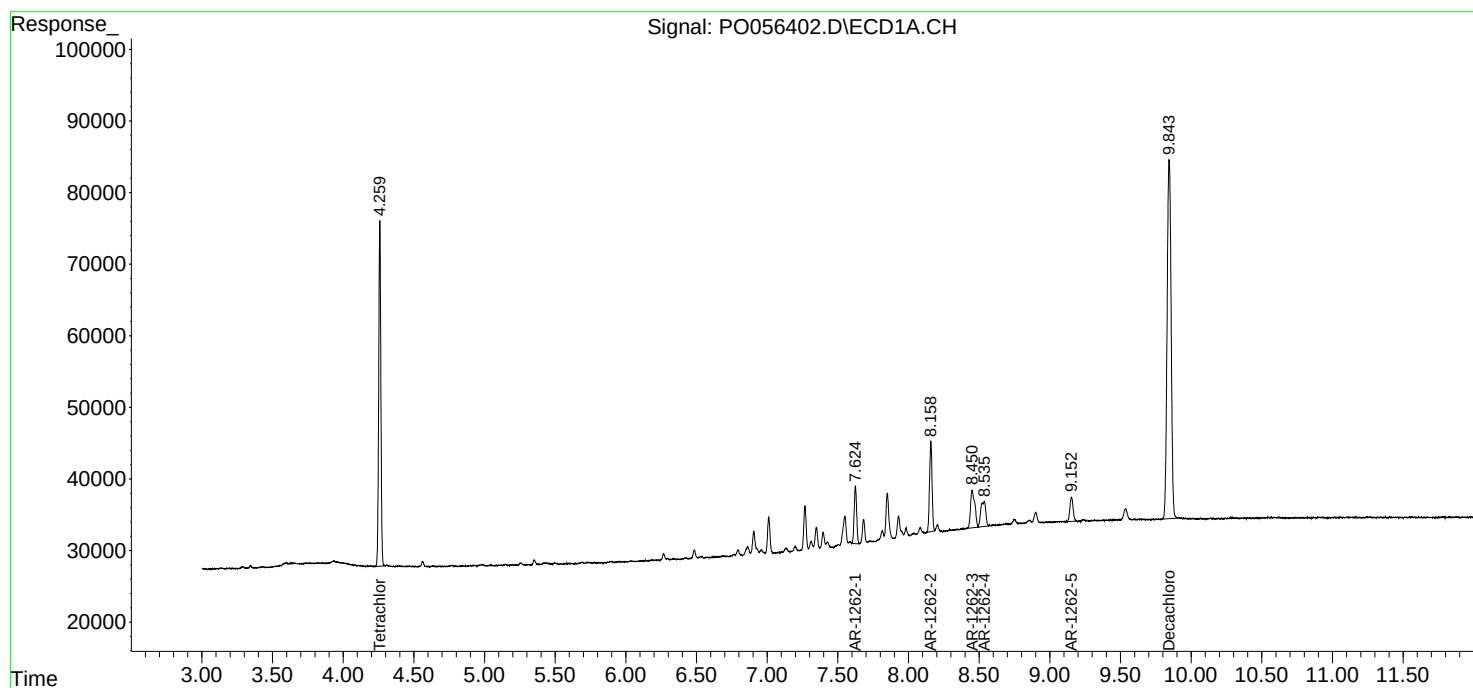

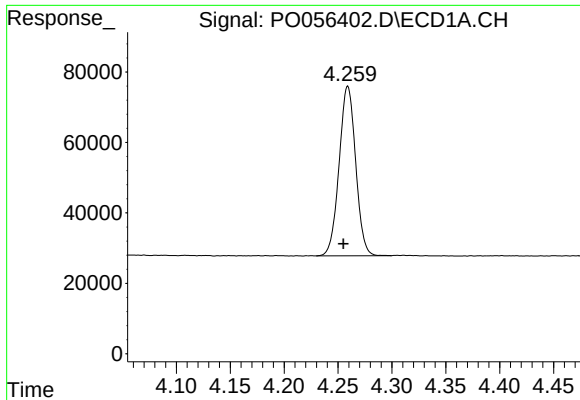


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.004 min
Response: 514608
Conc: 17.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:57 PM

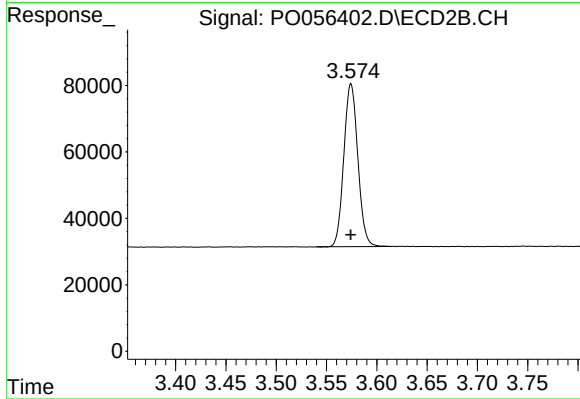


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 476386
Conc: 17.66 ng/ml

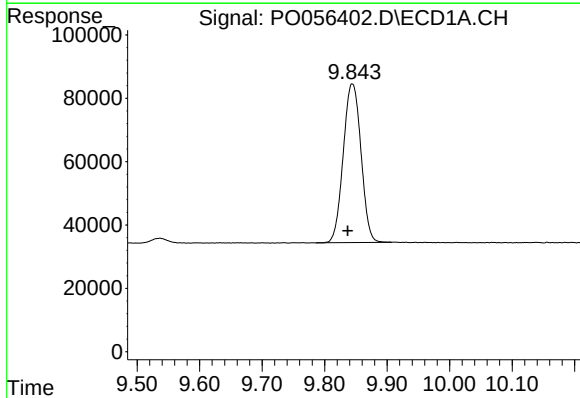


#2 Decachlorobiphenyl

R.T.: 9.844 min
Delta R.T.: 0.007 min
Response: 987376
Conc: 19.35 ng/ml

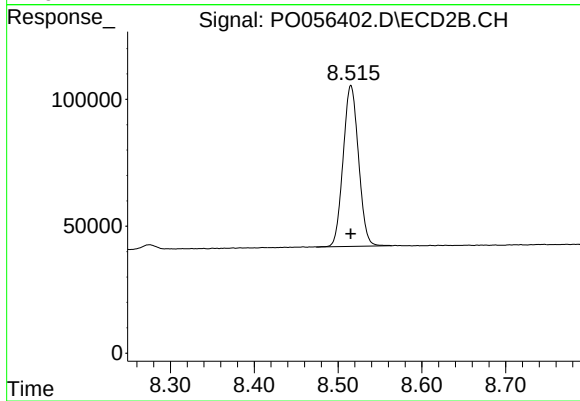

#2 Decachlorobiphenyl

R.T.: 8.515 min
Delta R.T.: 0.000 min
Response: 806624
Conc: 18.36 ng/ml

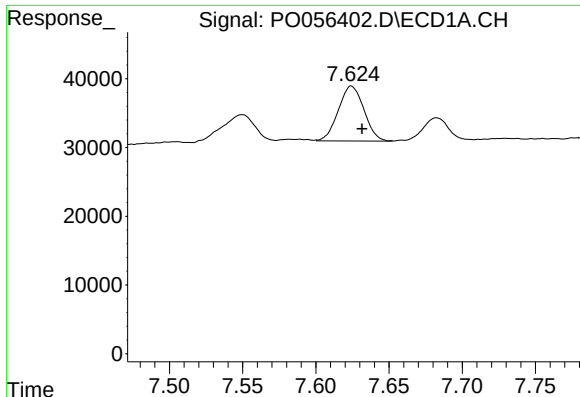


#36 AR-1262-1

R.T.: 7.624 min
Delta R.T.: -0.008 min
Response: 97208
Conc: 28.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:57 PM

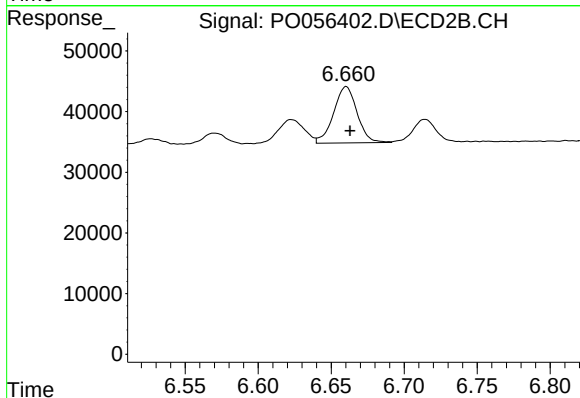


#36 AR-1262-1

R.T.: 6.660 min
Delta R.T.: -0.003 min
Response: 103857
Conc: 26.93 ng/ml

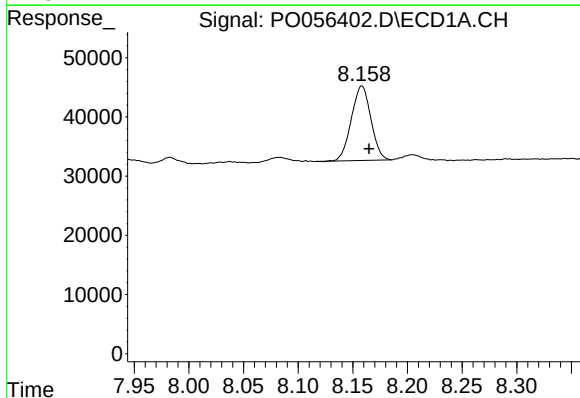


#37 AR-1262-2

R.T.: 8.158 min
Delta R.T.: -0.006 min
Response: 156554
Conc: 26.19 ng/ml

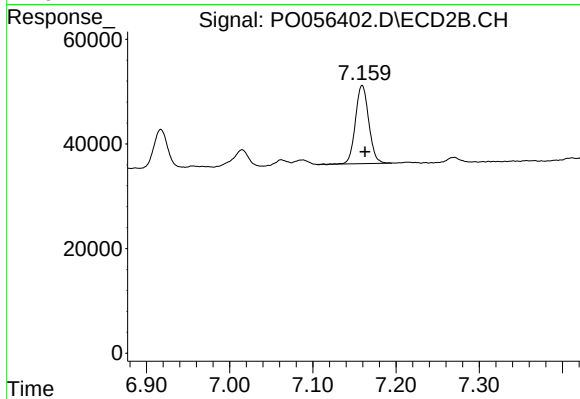

#37 AR-1262-2

R.T.: 7.159 min
Delta R.T.: -0.003 min
Response: 165974
Conc: 25.03 ng/ml

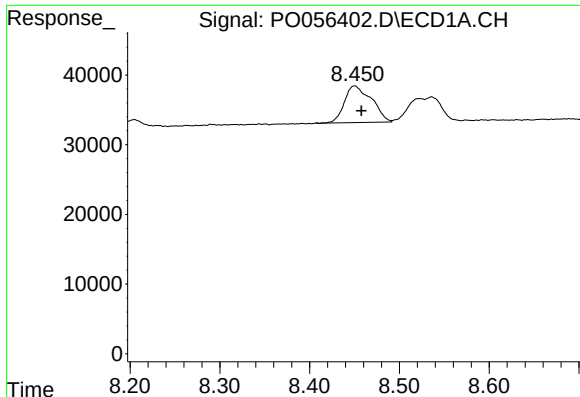


#38 AR-1262-3

R.T.: 8.450 min
Delta R.T.: -0.008 min
Response: 110428
Conc: 26.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:57 PM

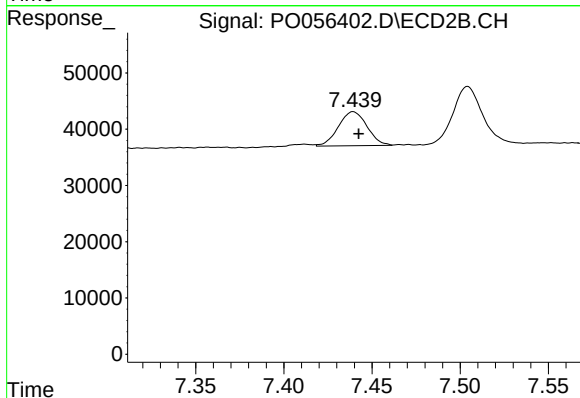


#38 AR-1262-3

R.T.: 7.439 min
Delta R.T.: -0.004 min
Response: 68633
Conc: 24.96 ng/ml m

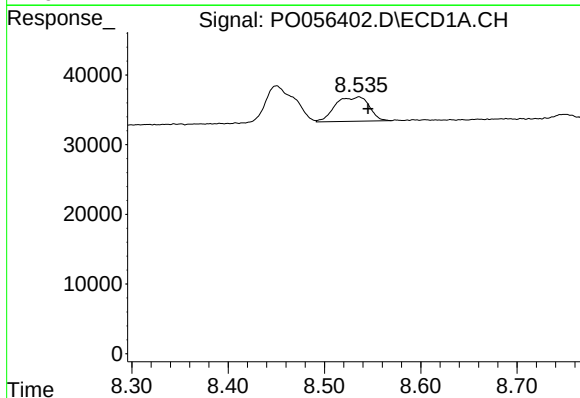


#39 AR-1262-4

R.T.: 8.536 min
Delta R.T.: -0.010 min
Response: 85082
Conc: 27.01 ng/ml

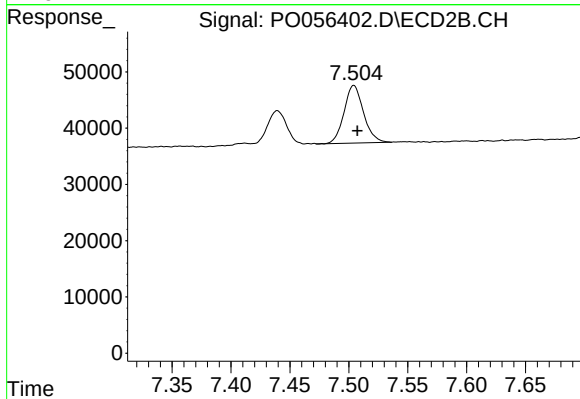

#39 AR-1262-4

R.T.: 7.504 min
Delta R.T.: -0.003 min
Response: 117837
Conc: 24.80 ng/ml

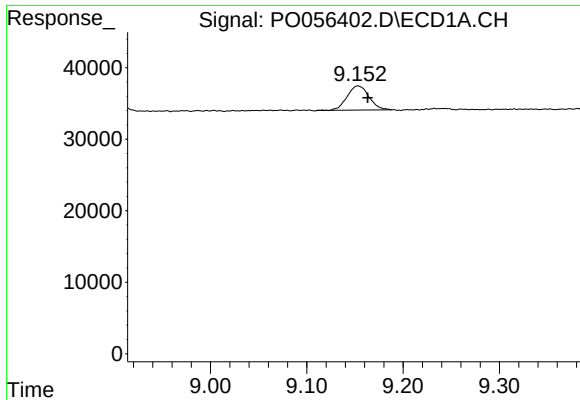


#40 AR-1262-5

R.T.: 9.153 min
Delta R.T.: -0.010 min
Response: 53005
Conc: 25.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:57 PM

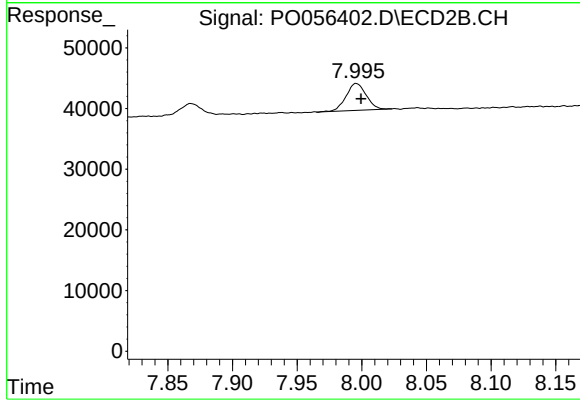

#40 AR-1262-5

R.T.: 7.996 min
Delta R.T.: -0.004 min
Response: 47765
Conc: 22.41 ng/ml