

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052019\
 Data File : P0056403.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2019 23:40
 Operator : SM/SJ
 Sample : K2241-07
 Misc : AR1262 LOD 40PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/21/2019 4:49:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:03:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.575	463910	428892	16.108	15.903
2) SA Decachlor...	9.845	8.516	886423	717810	17.372	16.340
Target Compounds						
36) L8 AR-1262-1	7.623	6.661	158753	173946	46.373m	45.103
37) L8 AR-1262-2	8.157	7.159	260289	278465	43.546	41.989
38) L8 AR-1262-3	8.449	7.438	184720	117306	44.780	42.660m
39) L8 AR-1262-4	8.536	7.504	140999	199199	44.762	41.920
40) L8 AR-1262-5	9.154	7.996	89701	78538	42.447	36.842

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052019\
Data File : PO056403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2019 23:40
Operator : SM/SJ
Sample : K2241-07
Misc : AR1262 LOD 40PPB
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:03:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

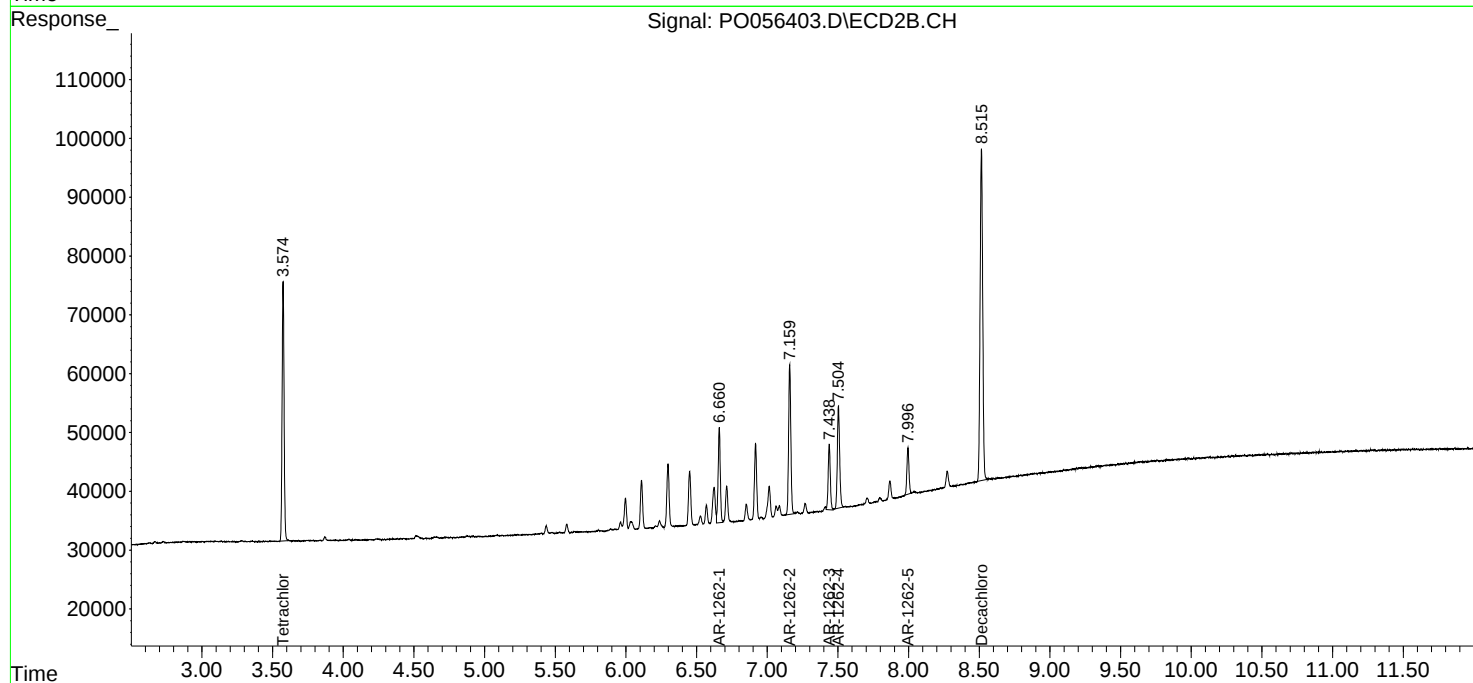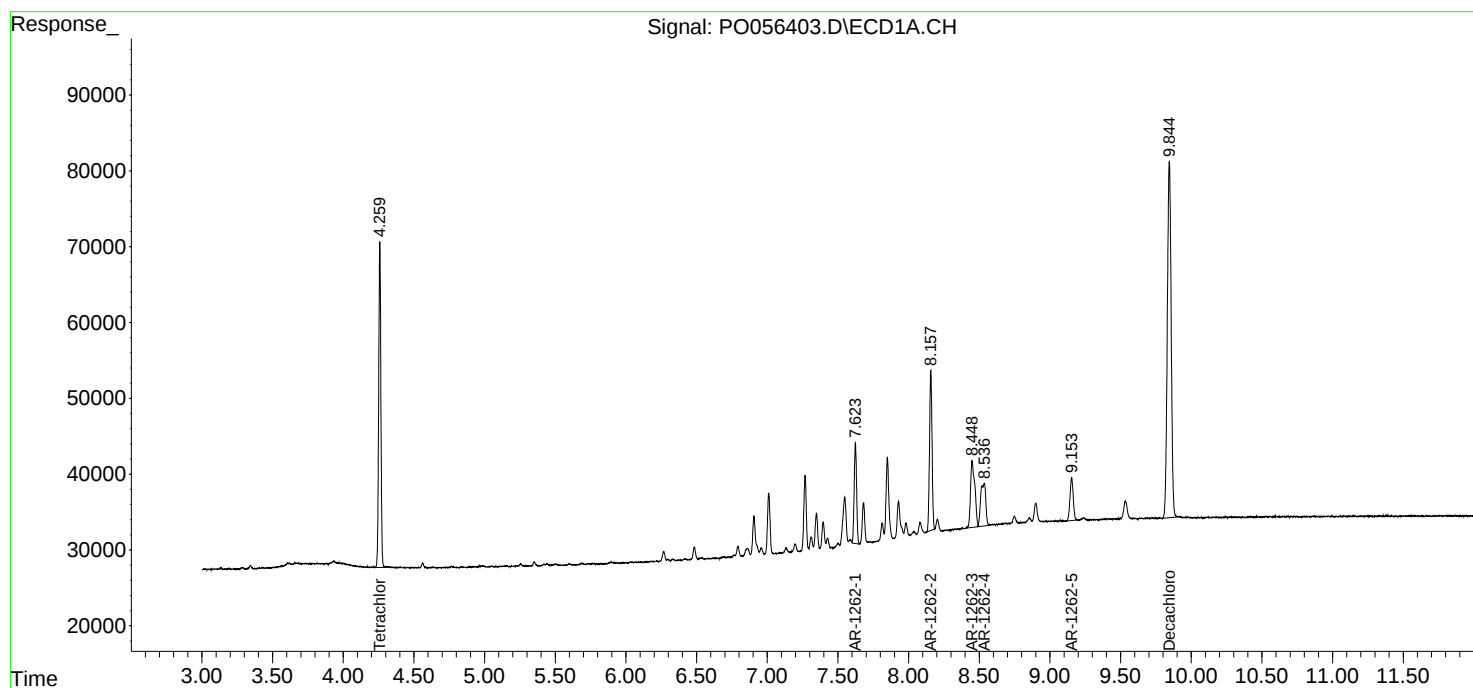

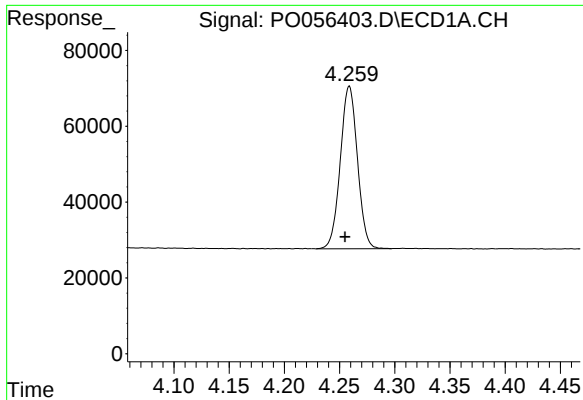


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.004 min
Response: 463910
Conc: 16.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:58 PM

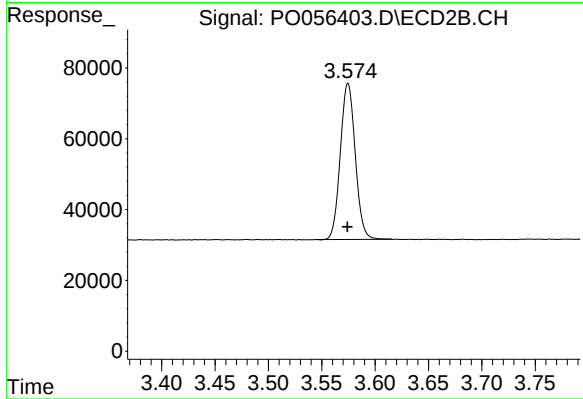


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.000 min
Response: 428892
Conc: 15.90 ng/ml

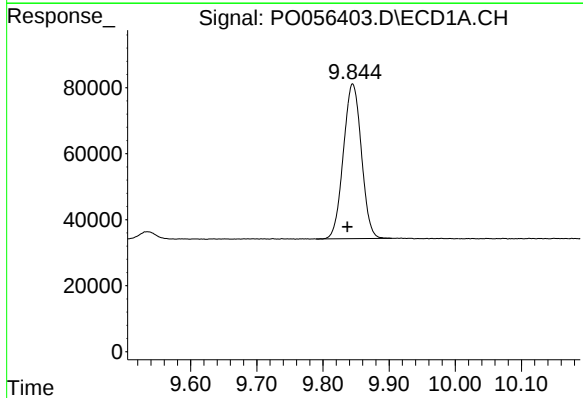


#2 Decachlorobiphenyl

R.T.: 9.845 min
Delta R.T.: 0.008 min
Response: 886423
Conc: 17.37 ng/ml

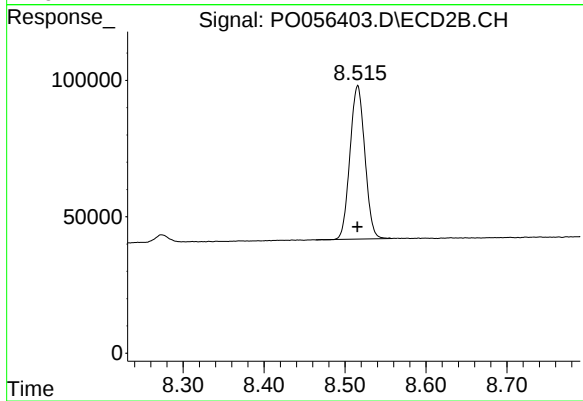

#2 Decachlorobiphenyl

R.T.: 8.516 min
Delta R.T.: 0.000 min
Response: 717810
Conc: 16.34 ng/ml

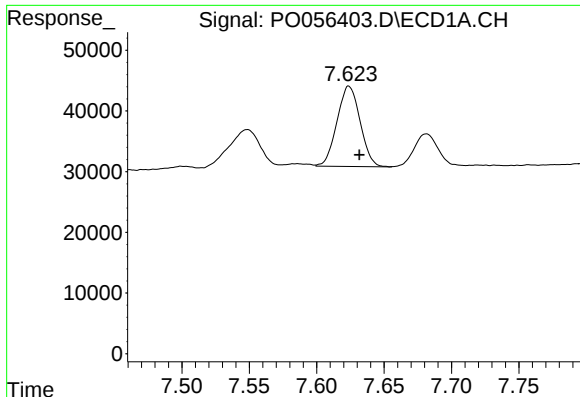


#36 AR-1262-1

R.T.: 7.623 min
Delta R.T.: -0.009 min
Response: 158753
Conc: 46.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:58 PM

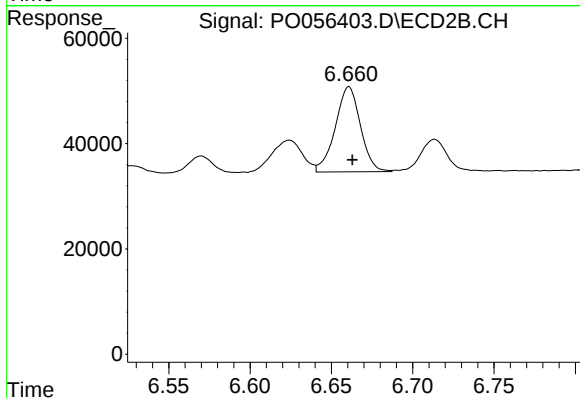


#36 AR-1262-1

R.T.: 6.661 min
Delta R.T.: -0.002 min
Response: 173946
Conc: 45.10 ng/ml

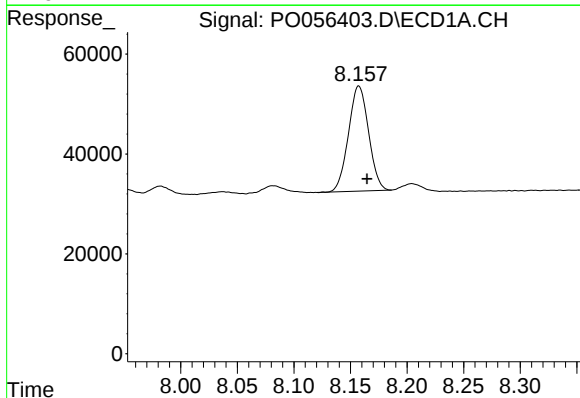


#37 AR-1262-2

R.T.: 8.157 min
Delta R.T.: -0.007 min
Response: 260289
Conc: 43.55 ng/ml

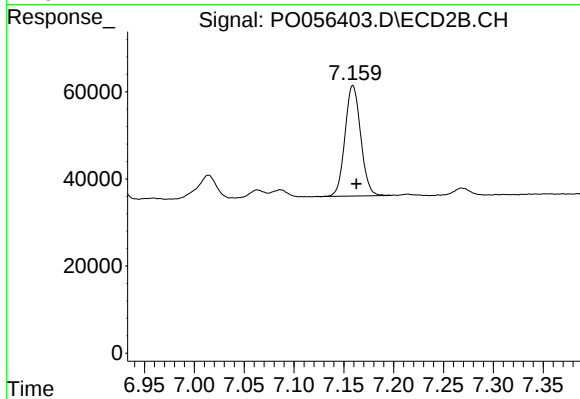

#37 AR-1262-2

R.T.: 7.159 min
Delta R.T.: -0.003 min
Response: 278465
Conc: 41.99 ng/ml

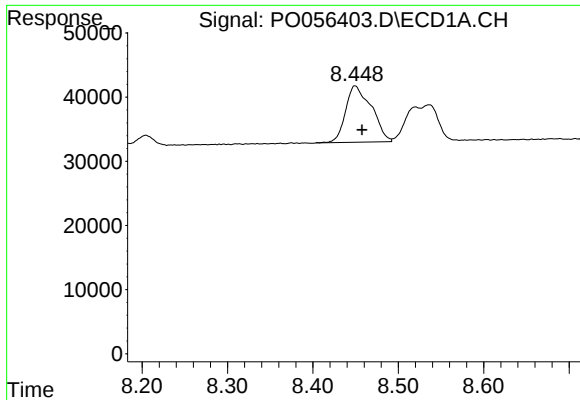


#38 AR-1262-3

R.T.: 8.449 min
Delta R.T.: -0.008 min
Response: 184720
Conc: 44.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019


Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:58 PM

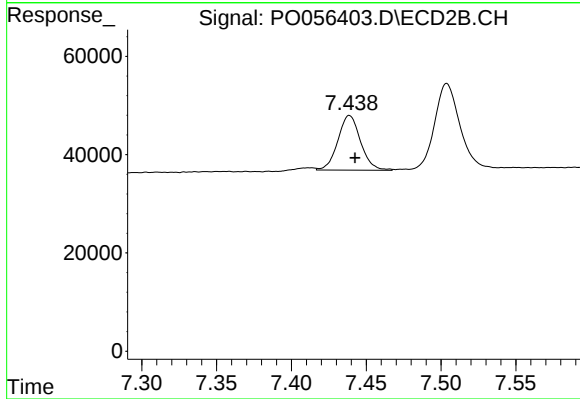


#38 AR-1262-3

R.T.: 7.438 min
Delta R.T.: -0.004 min
Response: 117306
Conc: 42.66 ng/ml m

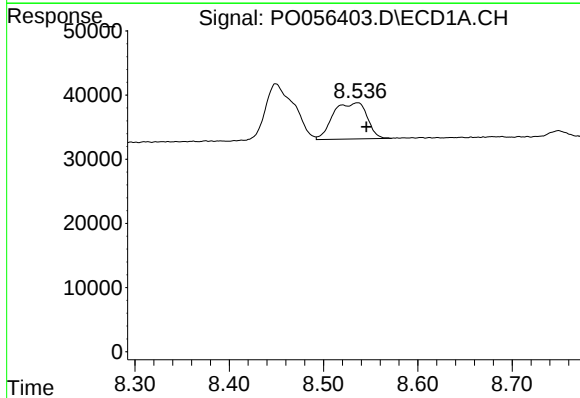


#39 AR-1262-4

R.T.: 8.536 min
Delta R.T.: -0.009 min
Response: 140999
Conc: 44.76 ng/ml

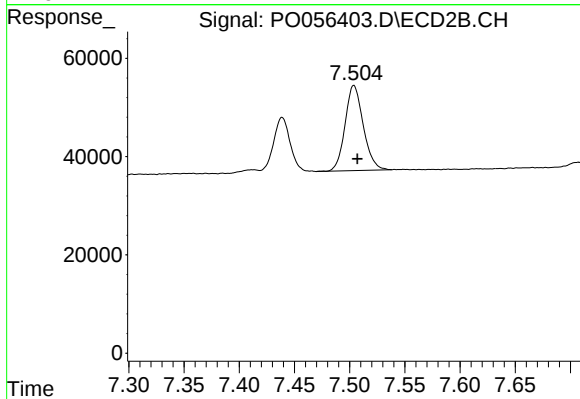

#39 AR-1262-4

R.T.: 7.504 min
Delta R.T.: -0.003 min
Response: 199199
Conc: 41.92 ng/ml

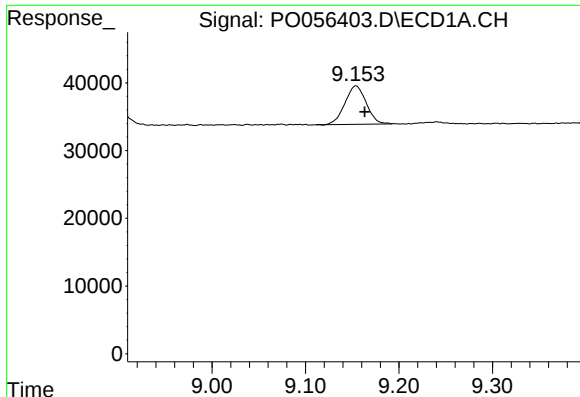


#40 AR-1262-5

R.T.: 9.154 min
Delta R.T.: -0.009 min
Response: 89701
Conc: 42.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Manual Integrations
APPROVED

Ankita
5/21/2019 4:49:58 PM

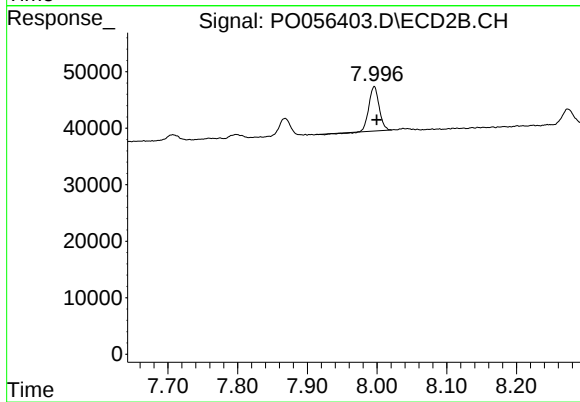

#40 AR-1262-5

R.T.: 7.996 min
Delta R.T.: -0.003 min
Response: 78538
Conc: 36.84 ng/ml