

Data Path : P:\HPCHEM1\ECD 0\Data\P0052118\
 Data File : P0044888.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2018 15:11
 Operator : SM/UA
 Sample : J2954-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-026

Manual Integrations
 APPROVED

ugo
 5/23/2018 10:05:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 15:52:24 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 15 15:44:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.028	3.290	4547242	5482600	29.674m	22.871
2) SA Decachlor...	9.337	8.026	1946691	2540269	9.468	9.028m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO052118\
Data File : PO044888.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2018 15:11
Operator : SM/UA
Sample : J2954-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-026


Manual Integrations
APPROVED

ugo
5/23/2018 10:05:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 15:52:24 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

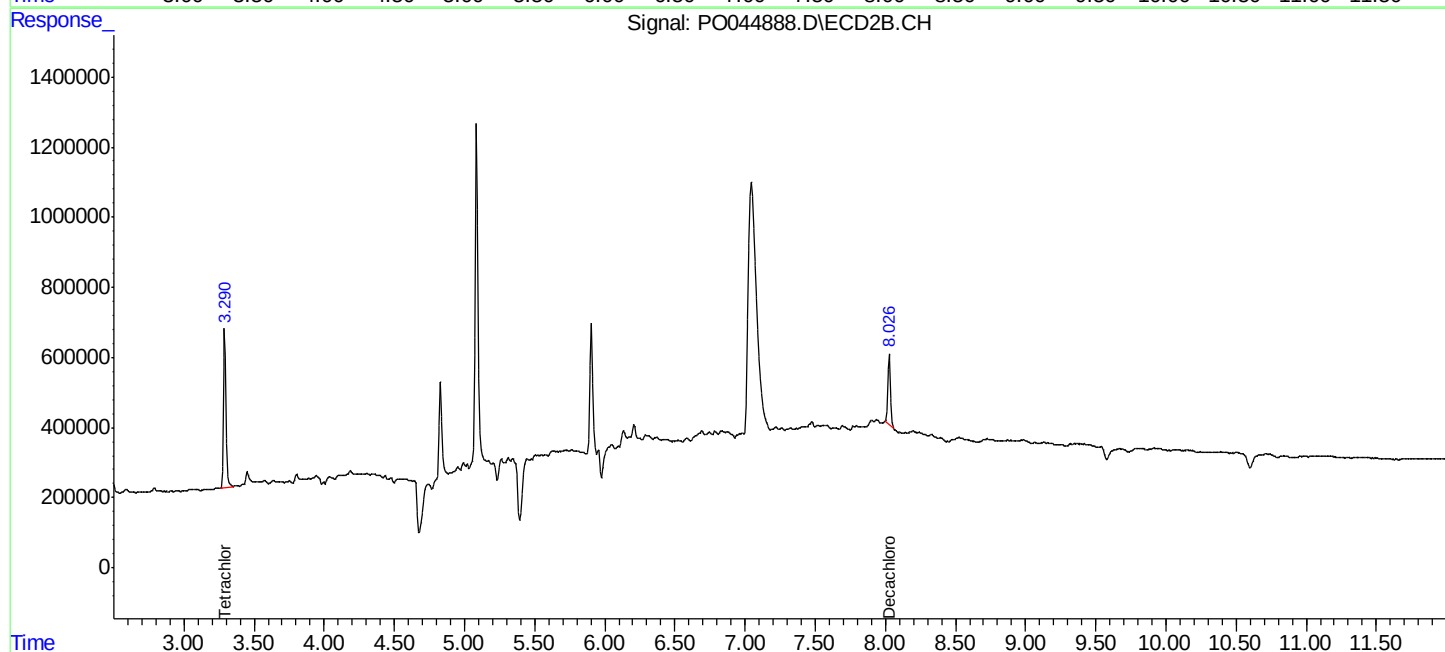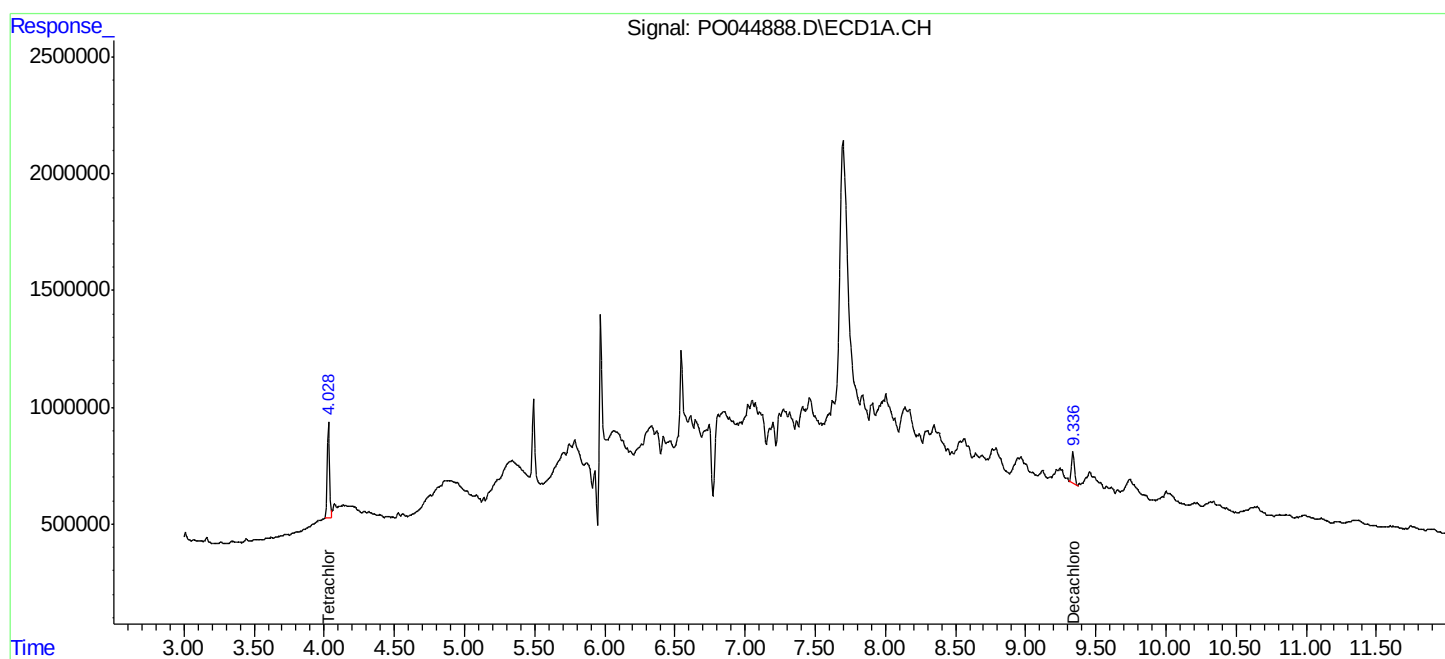

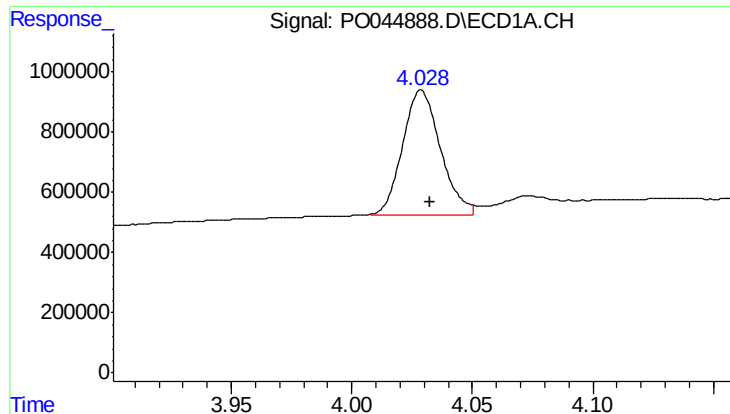


#1 Tetrachloro-m-xylene

R.T.: 4.028 min
Delta R.T.: -0.004 min
Response: 4547242
Conc: 29.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-026


Manual Integrations
APPROVED

ugo
5/23/2018 10:05:20 AM

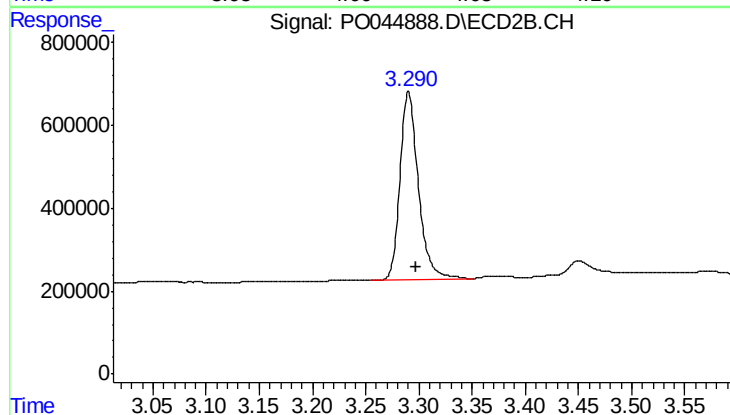


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: -0.008 min
Response: 5482600
Conc: 22.87 ng/ml

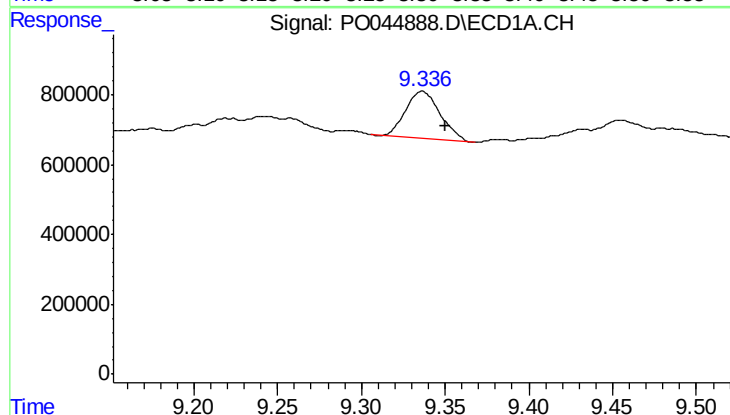

#2 Decachlorobiphenyl

R.T.: 9.337 min
Delta R.T.: -0.014 min
Response: 1946691
Conc: 9.47 ng/ml

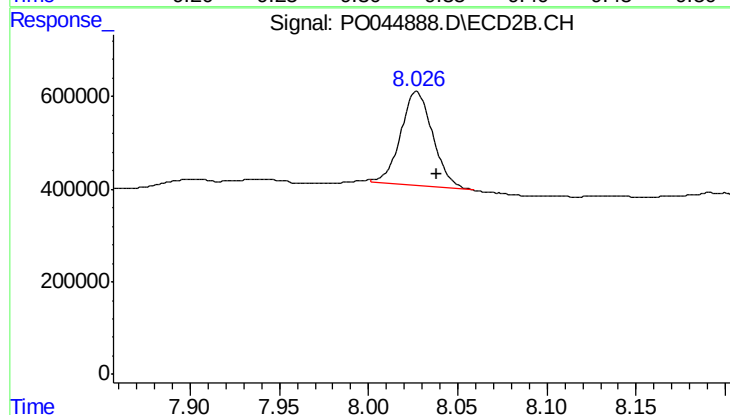

#2 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: -0.012 min
Response: 2540269
Conc: 9.03 ng/ml m