

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052120\
 Data File : P0068515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2020 12:51
 Operator : DD\AJ
 Sample : L2497-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-02-051920

Manual Integrations
 APPROVED

Sohil
 5/26/2020 4:07:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:31:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.929	791878	957692	28.235	27.910m
2) SA Decachlor...	10.840	9.199	924384	865868	23.230m	22.491

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052120\
Data File : P0068515.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2020 12:51
Operator : DD\AJ
Sample : L2497-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-02-051920


Manual Integrations
APPROVED

Sohil
5/26/2020 4:07:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:31:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

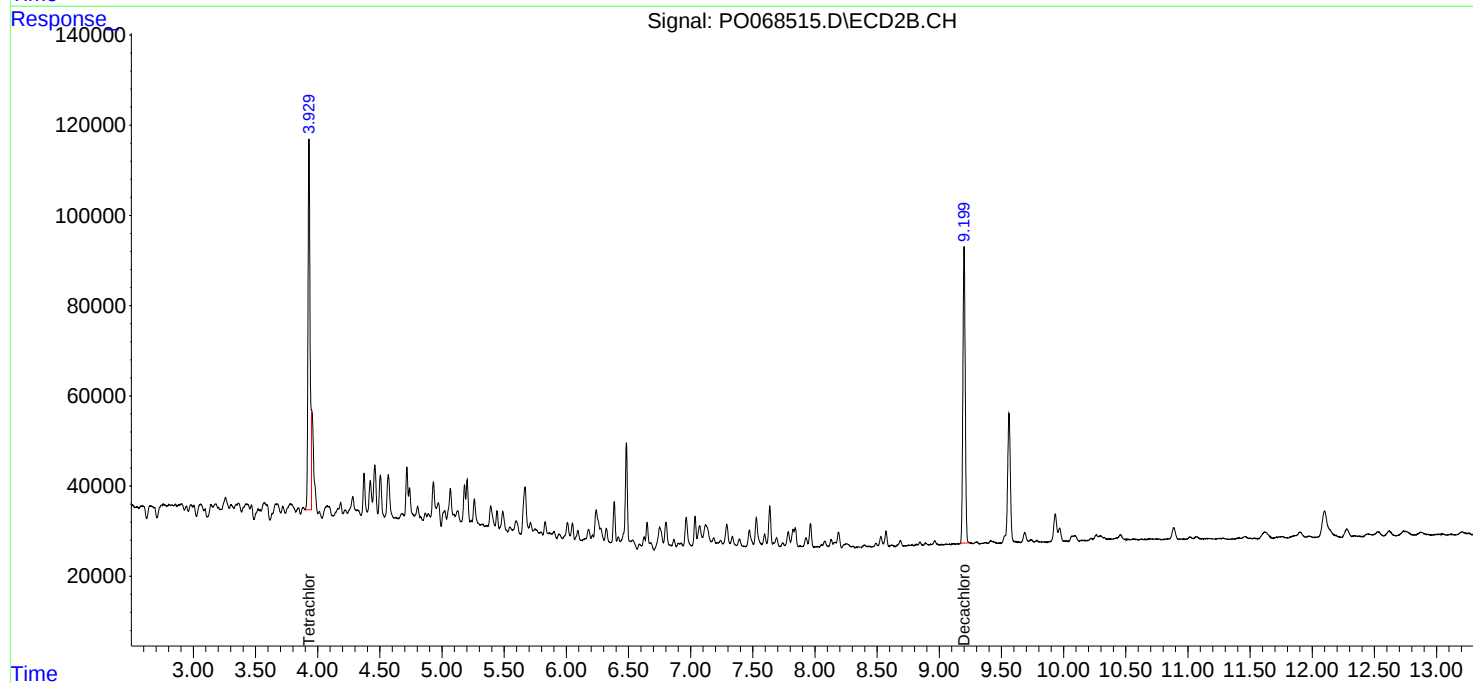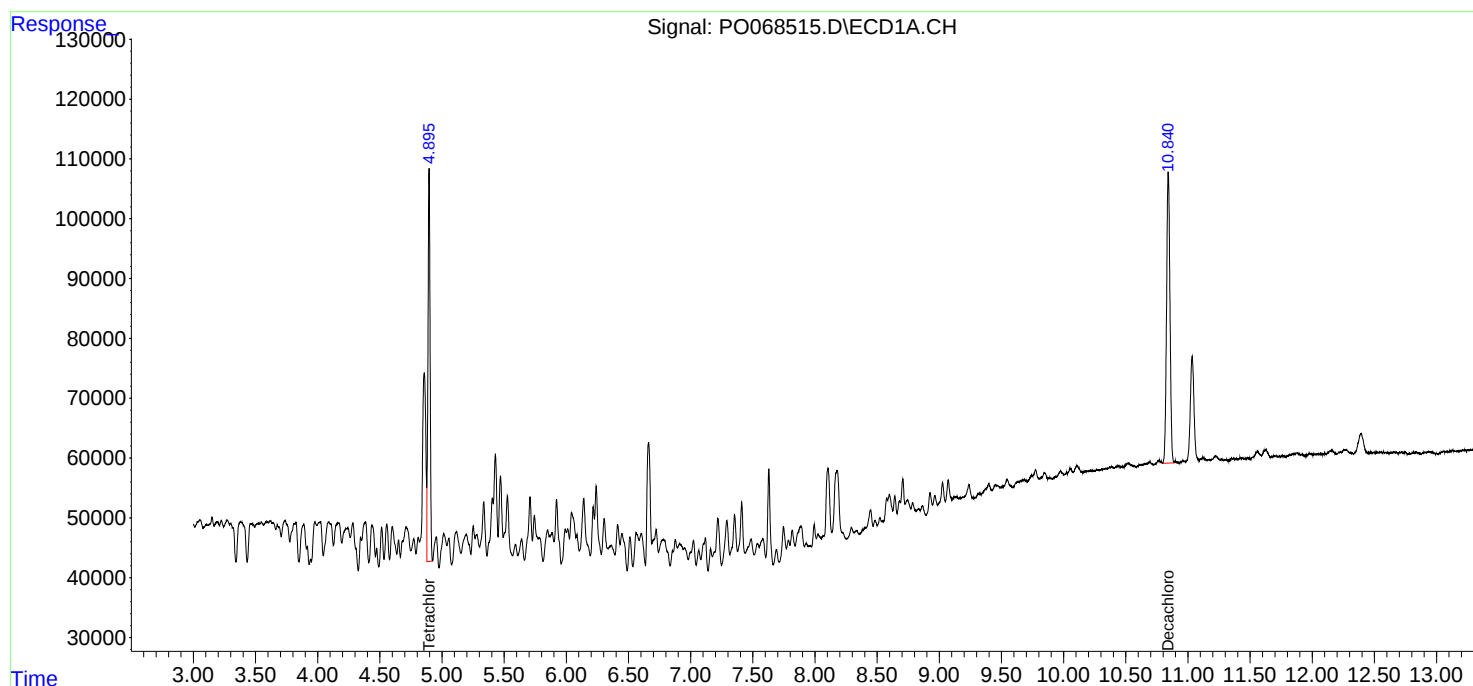

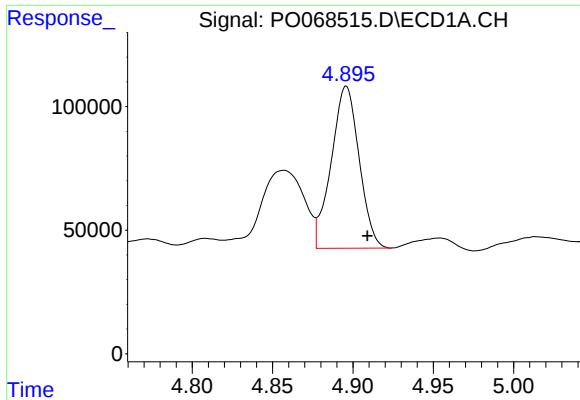


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: -0.013 min
Response: 791878
Conc: 28.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-02-051920


Manual Integrations
APPROVED

Sohil
5/26/2020 4:07:58 PM

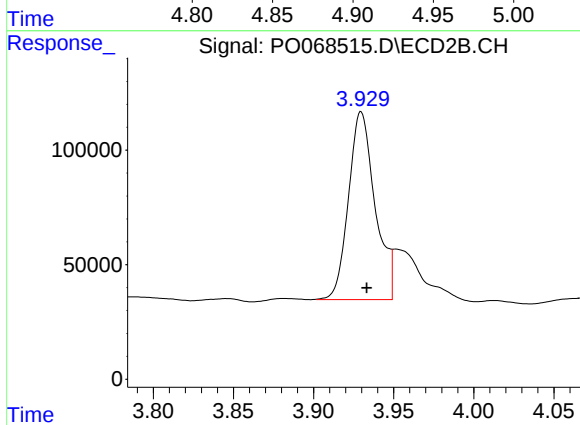


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.004 min
Response: 957692
Conc: 27.91 ng/ml m

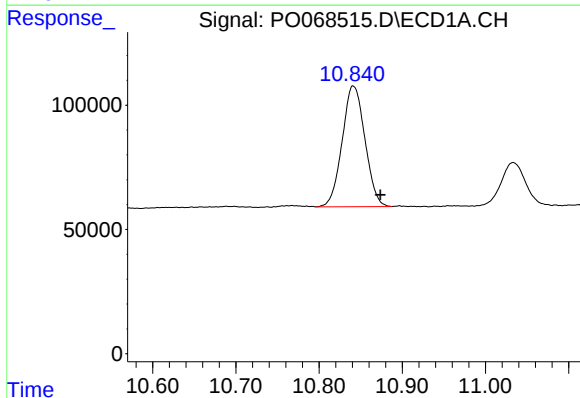

#2 Decachlorobiphenyl

R.T.: 10.840 min
Delta R.T.: -0.034 min
Response: 924384
Conc: 23.23 ng/ml m

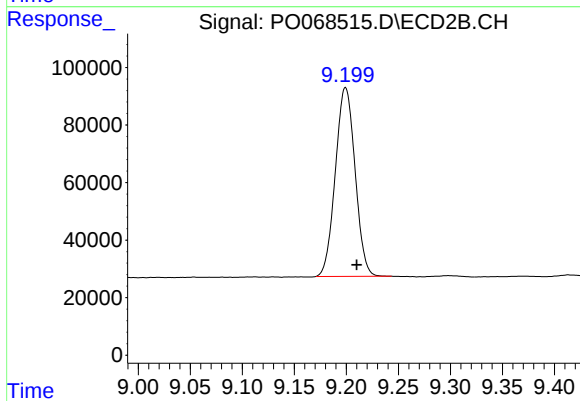

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.011 min
Response: 865868
Conc: 22.49 ng/ml