

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052120\
 Data File : P0068526.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2020 15:58
 Operator : DD\AJ
 Sample : L2722-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 17:07:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.931	778323	925067	27.751	26.959
2) SA Decachlor...	10.842	9.201	911521	920563	22.907	23.911

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052120\
Data File : P0068526.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2020 15:58
Operator : DD\AJ
Sample : L2722-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 17:07:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

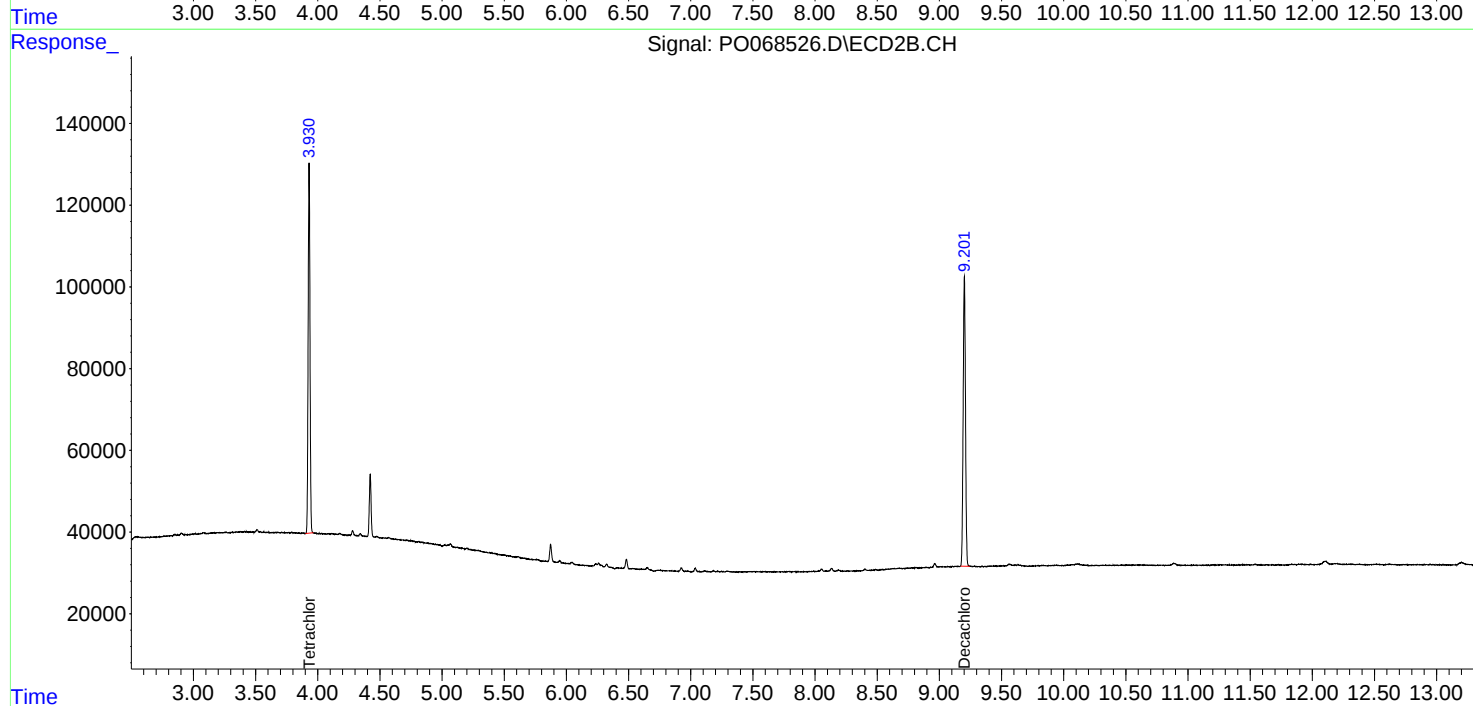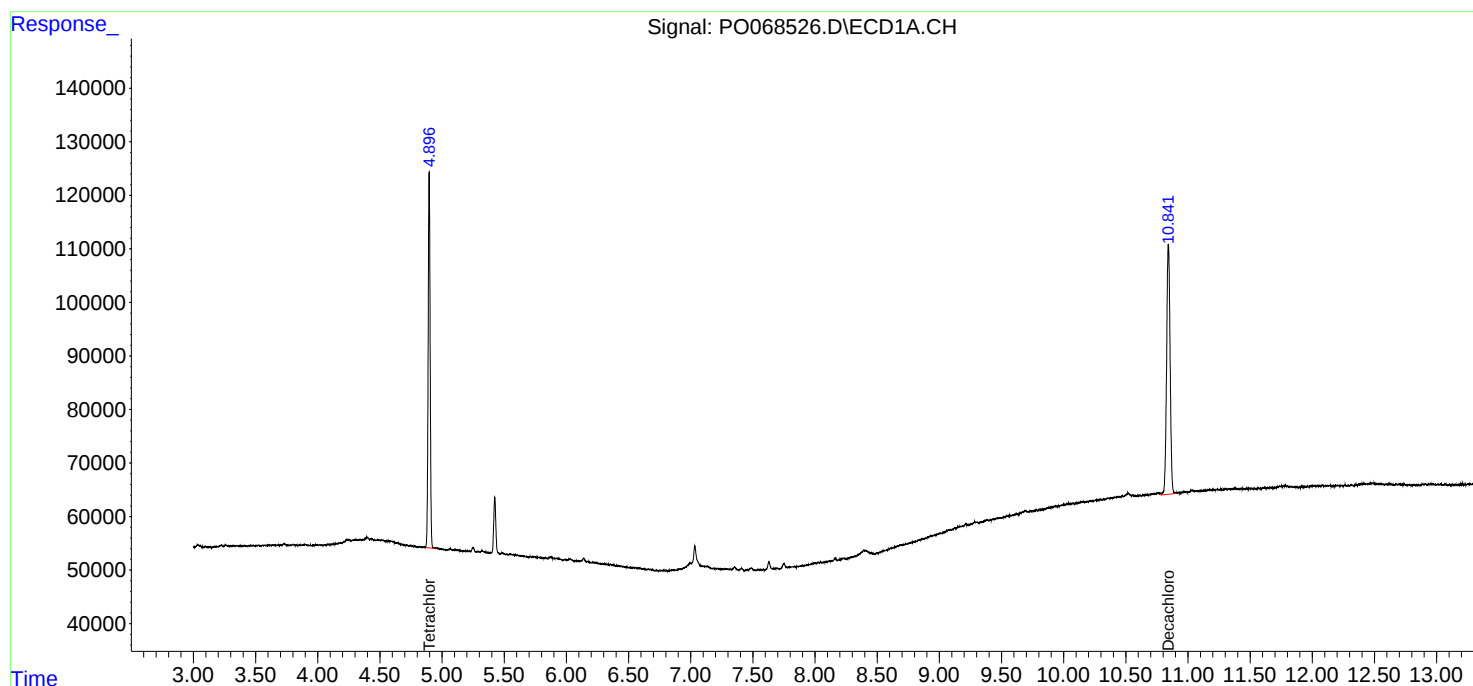


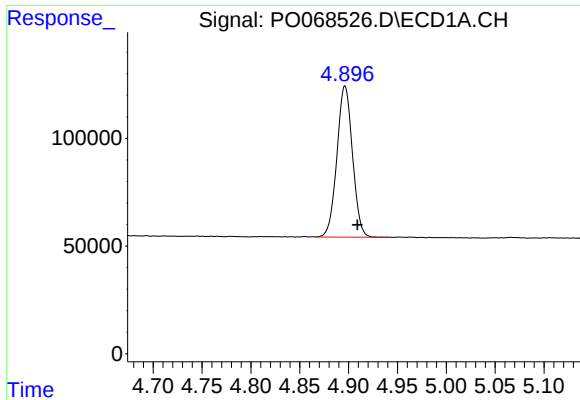

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: -0.013 min
Response: 778323
Conc: 27.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3

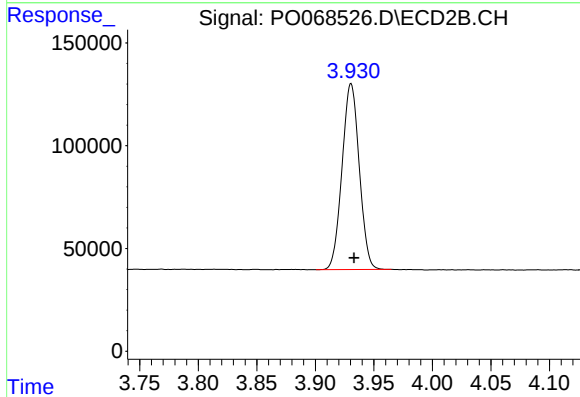


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.003 min
Response: 925067
Conc: 26.96 ng/ml

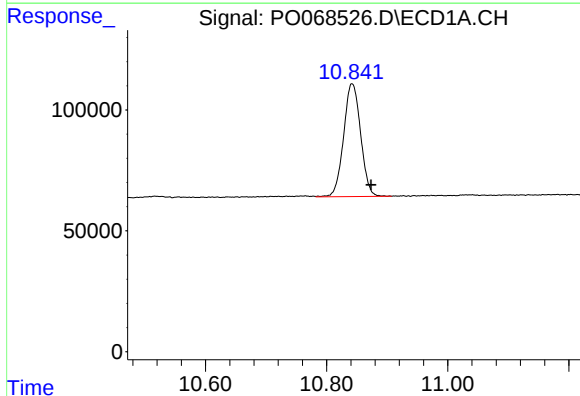

#2 Decachlorobiphenyl

R.T.: 10.842 min
Delta R.T.: -0.031 min
Response: 911521
Conc: 22.91 ng/ml

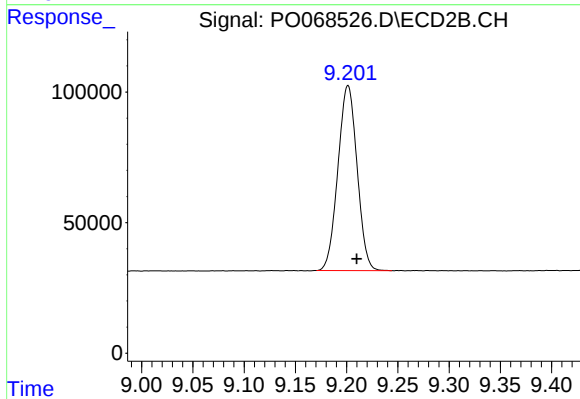

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.009 min
Response: 920563
Conc: 23.91 ng/ml