

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD 0\Data\P0052218\
 Data File : P0044911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 May 2018 13:37
 Operator : SM/UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Sohil
 5/24/2018 1:15:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 14:00:29 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 15 15:44:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.021	3.293	6060825	6941251	39.551	28.955 #
2) SA Decachlor...	9.321	8.022	4217899	4325148	20.514m	15.371m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD 0\Data\P0052218\
Data File : P0044911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2018 13:37
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
5/24/2018 1:15:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 14:00:29 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

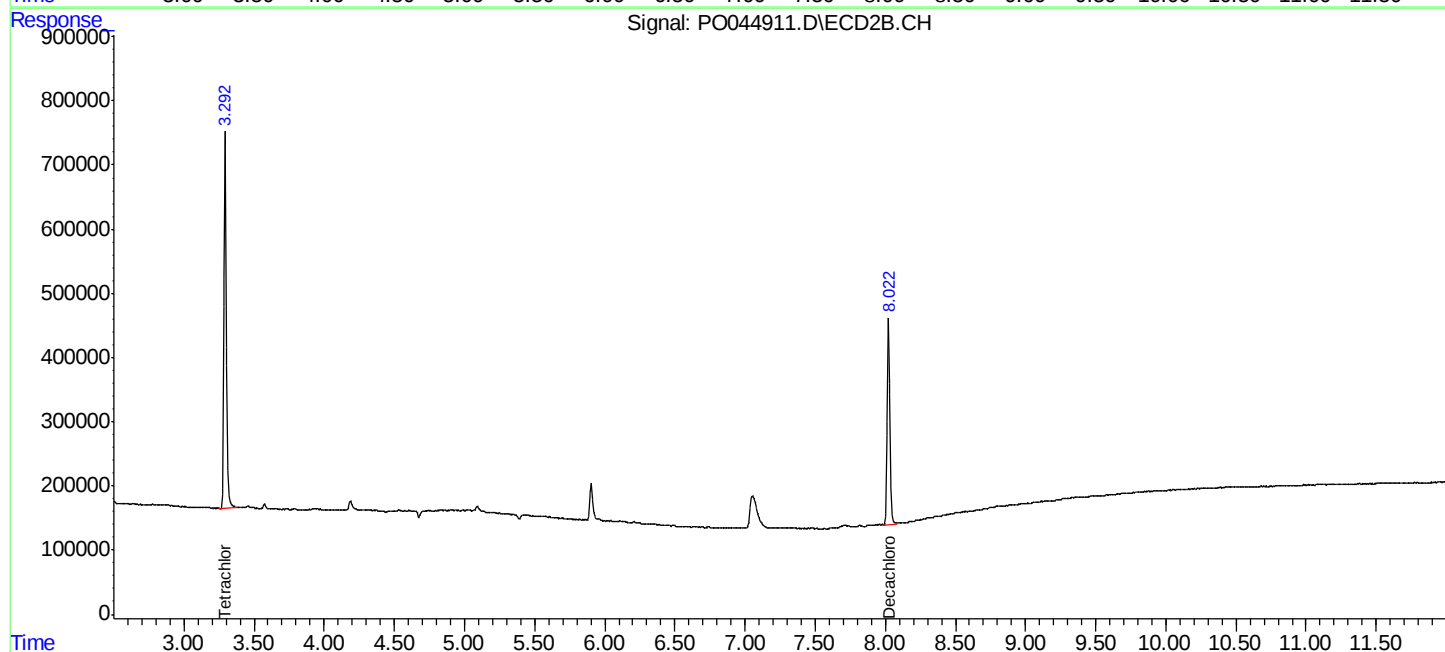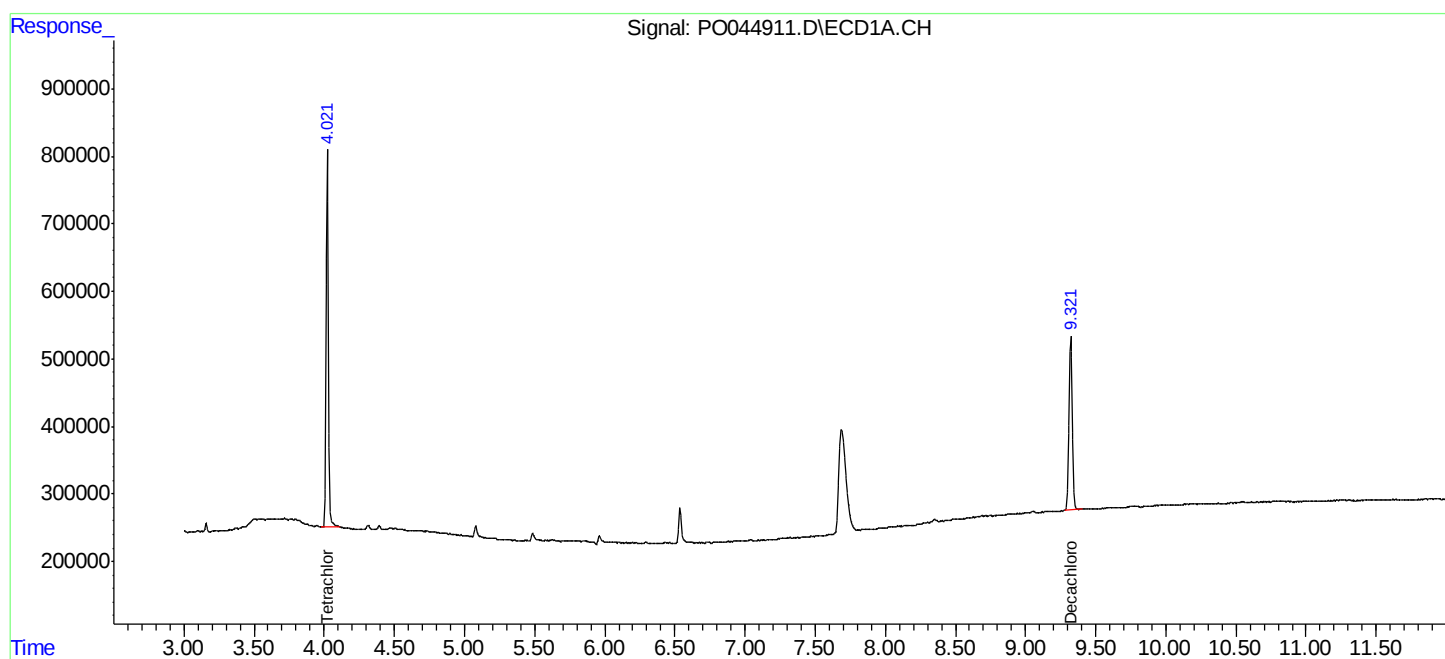

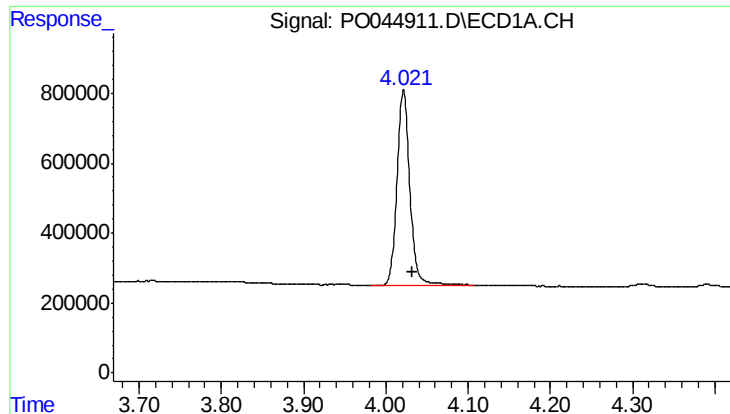


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: -0.011 min
Response: 6060825
Conc: 39.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
5/24/2018 1:15:25 AM

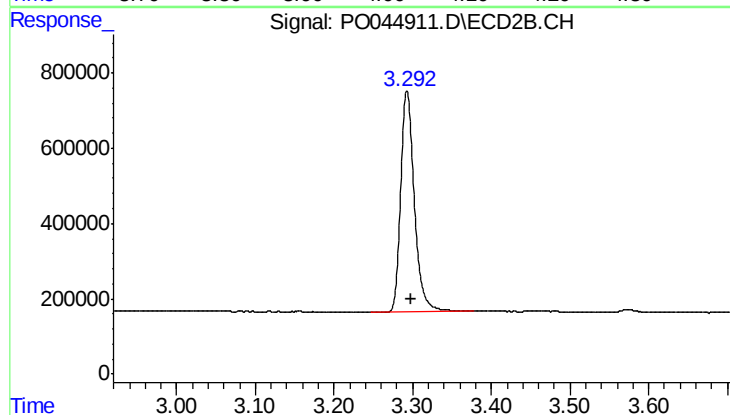


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: -0.005 min
Response: 6941251
Conc: 28.96 ng/ml

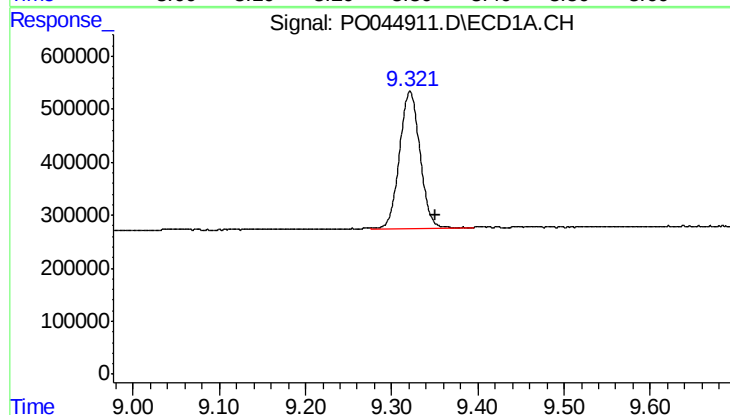

#2 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: -0.030 min
Response: 4217899
Conc: 20.51 ng/ml m

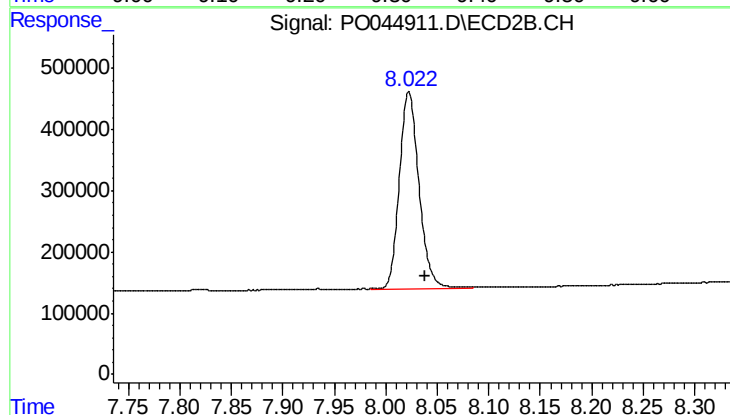

#2 Decachlorobiphenyl

R.T.: 8.022 min
Delta R.T.: -0.016 min
Response: 4325148
Conc: 15.37 ng/ml m