

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052219\
 Data File : P0056473.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 May 2019 14:13
 Operator : SM/SJ
 Sample : K2896-07RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-20-SRE

Manual Integrations
 APPROVED

Ankita
 5/24/2019 9:56:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 14:28:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.265	3.576	452885	421261	15.725	15.620
2) SA Decachlor...	9.846	8.515	400234	311633	7.844	7.094
Target Compounds						
31) L7 AR-1260-1	7.013	6.110	42978	44045	17.332m	17.959
32) L7 AR-1260-2	7.271	6.298	44748	45358	14.542	14.271
33) L7 AR-1260-3	7.626	6.450	48229	47119	20.021	16.368
34) L7 AR-1260-4	7.849	6.917	55810	38961	20.173m	15.614
35) L7 AR-1260-5	8.158	7.159	81095	101866	15.039	16.604

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052219\
Data File : P0056473.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2019 14:13
Operator : SM/SJ
Sample : K2896-07RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-20-SRE


Manual Integrations
APPROVED

Ankita
5/24/2019 9:56:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 14:28:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

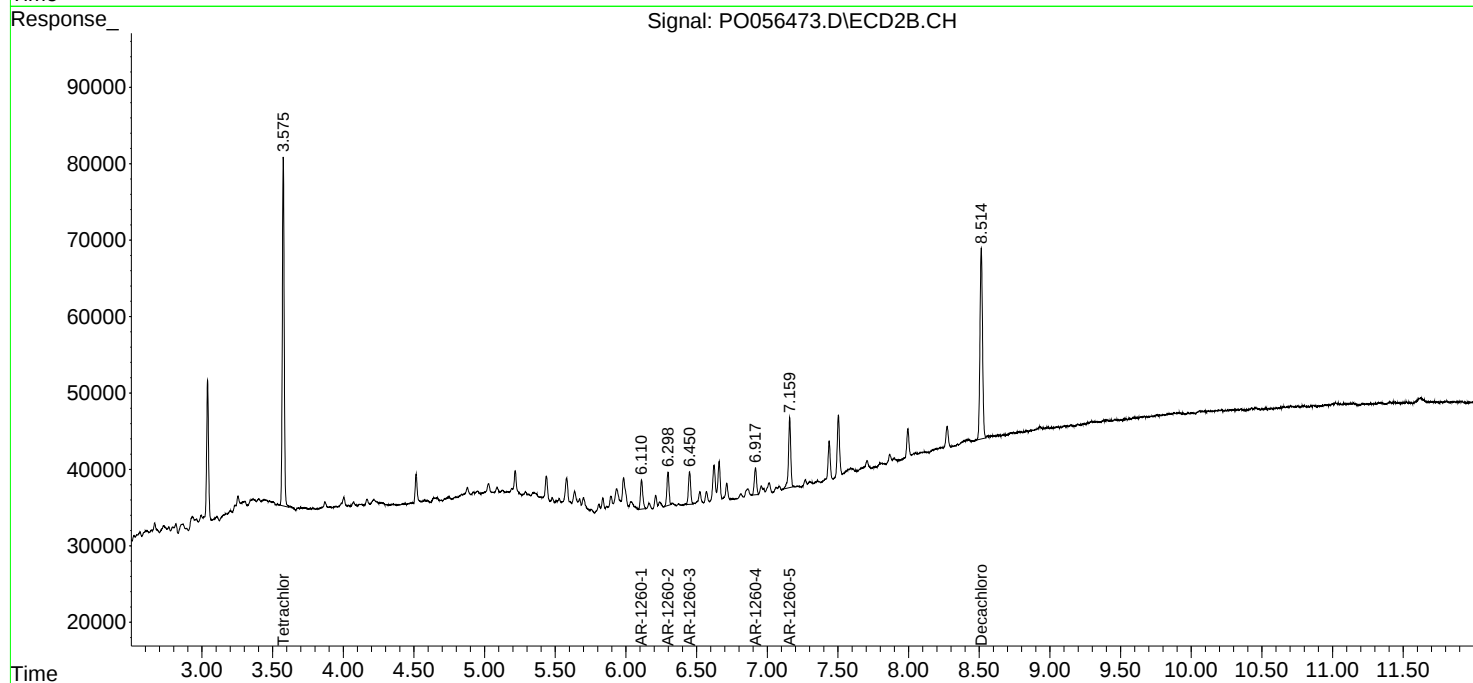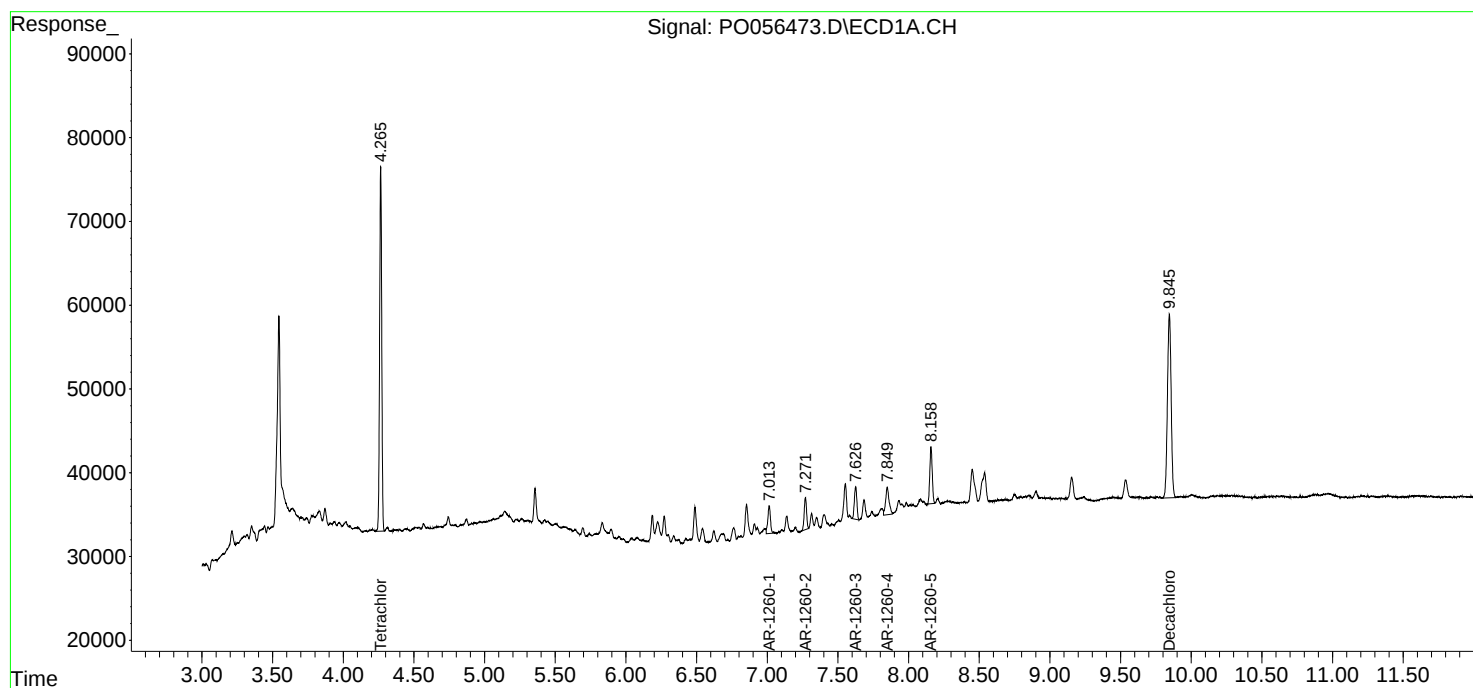

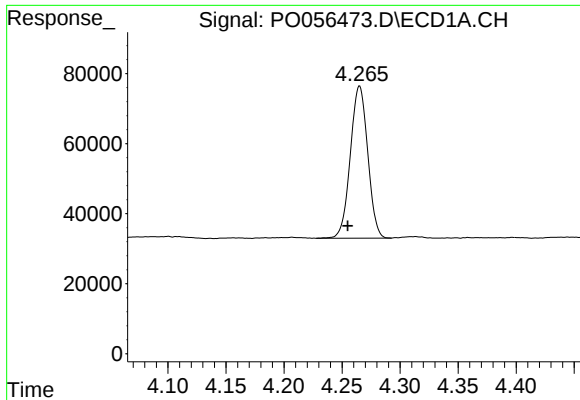


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: 0.010 min
Response: 452885
Conc: 15.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-SRE


Manual Integrations
APPROVED

Ankita
5/24/2019 9:56:57 AM

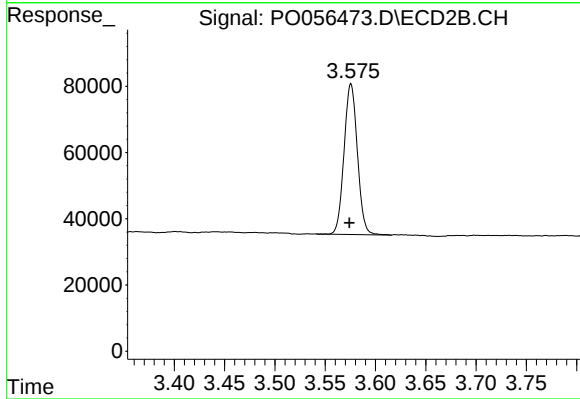


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: 0.002 min
Response: 421261
Conc: 15.62 ng/ml

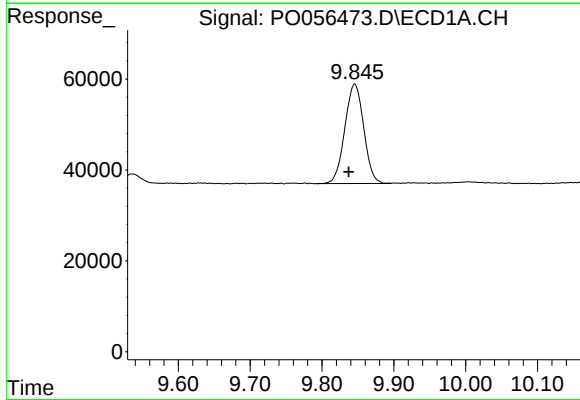


#2 Decachlorobiphenyl

R.T.: 9.846 min
Delta R.T.: 0.009 min
Response: 400234
Conc: 7.84 ng/ml

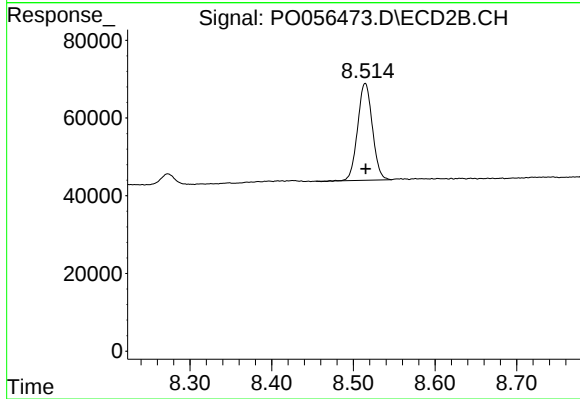

#2 Decachlorobiphenyl

R.T.: 8.515 min
Delta R.T.: 0.000 min
Response: 311633
Conc: 7.09 ng/ml

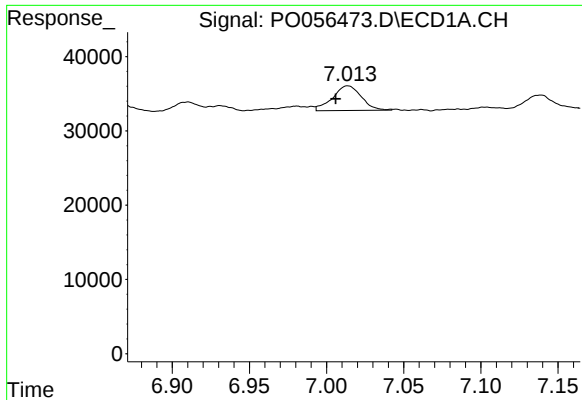


#31 AR-1260-1

R.T.: 7.013 min
Delta R.T.: 0.008 min
Response: 42978
Conc: 17.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-20-SRE


Manual Integrations
APPROVED

Ankita
5/24/2019 9:56:57 AM

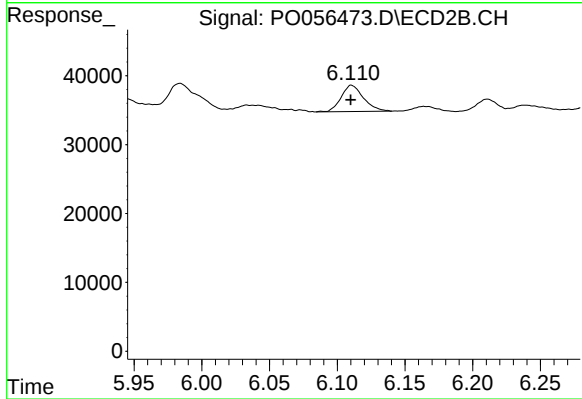


#31 AR-1260-1

R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 44045
Conc: 17.96 ng/ml

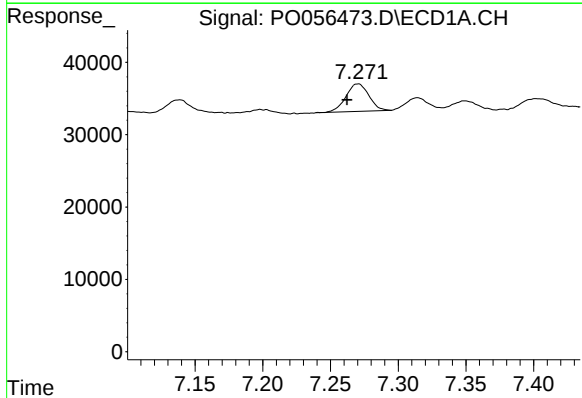


#32 AR-1260-2

R.T.: 7.271 min
Delta R.T.: 0.009 min
Response: 44748
Conc: 14.54 ng/ml

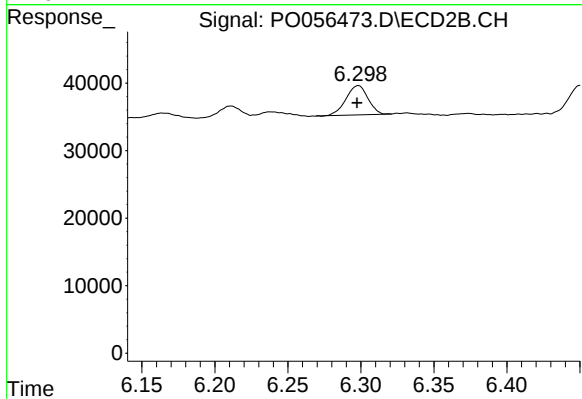

#32 AR-1260-2

R.T.: 6.298 min
Delta R.T.: 0.000 min
Response: 45358
Conc: 14.27 ng/ml

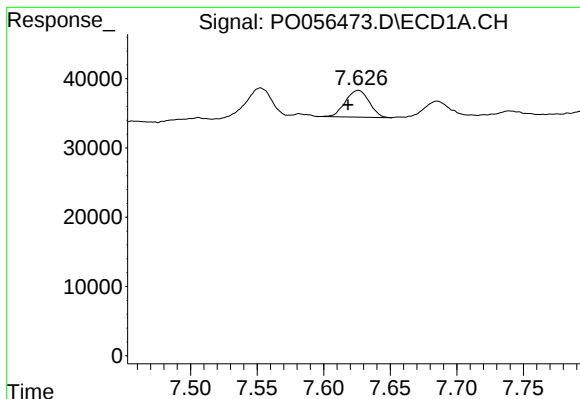


#33 AR-1260-3

R.T.: 7.626 min
Delta R.T.: 0.008 min
Response: 48229
Conc: 20.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-SRE


Manual Integrations
APPROVED

Ankita
5/24/2019 9:56:57 AM

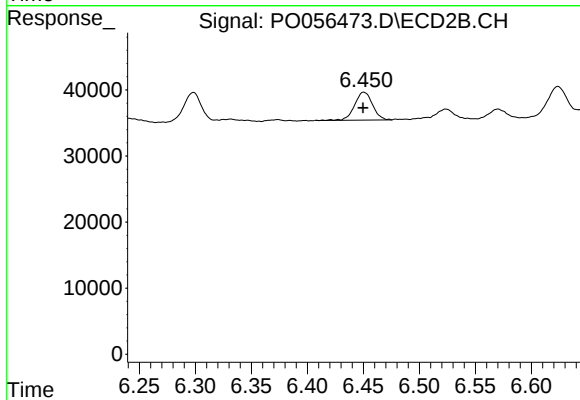


#33 AR-1260-3

R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 47119
Conc: 16.37 ng/ml

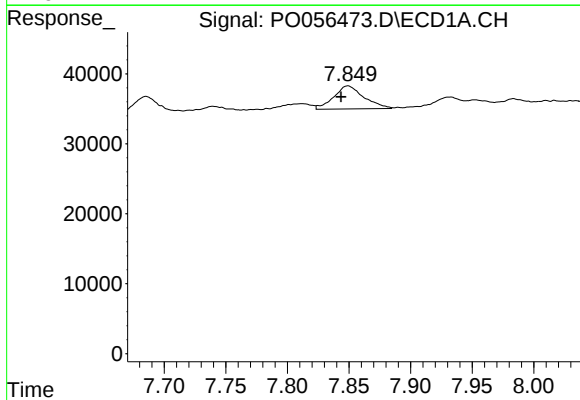


#34 AR-1260-4

R.T.: 7.849 min
Delta R.T.: 0.005 min
Response: 55810
Conc: 20.17 ng/ml m

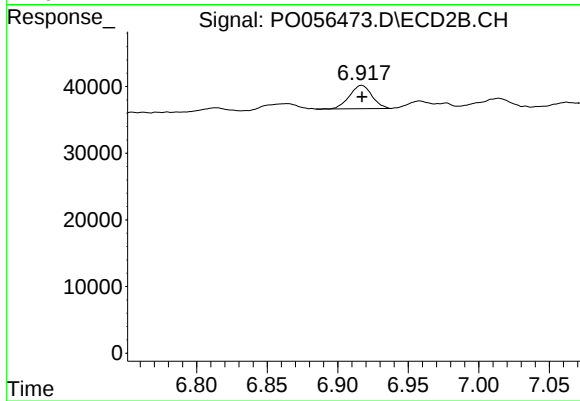

#34 AR-1260-4

R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 38961
Conc: 15.61 ng/ml

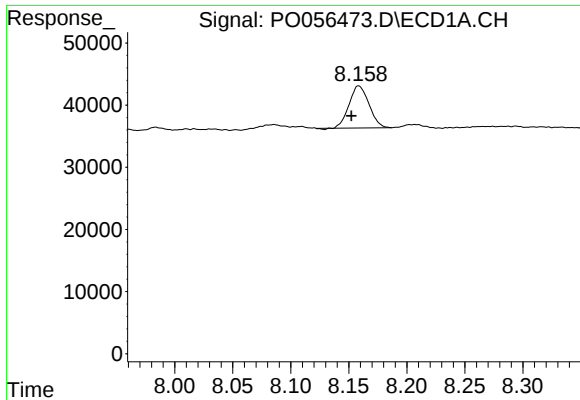


#35 AR-1260-5

R.T.: 8.158 min
Delta R.T.: 0.006 min
Response: 81095
Conc: 15.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-SRE

Manual Integrations
APPROVED

Ankita
5/24/2019 9:56:57 AM

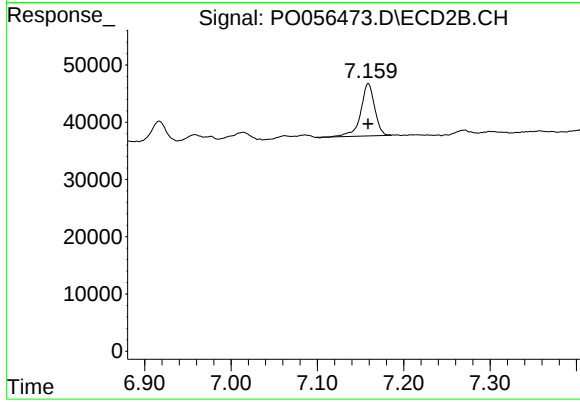

#35 AR-1260-5

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 101866
Conc: 16.60 ng/ml