

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052219\
 Data File : P0056508.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 May 2019 1:05
 Operator : SM/SJ
 Sample : K2971-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SUP-2A-C-2-052019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:52:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.257	3.575	807003	778269	28.021	28.858
2) SA Decachlor...	9.834	8.510	743760	578113	14.576	13.160

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052219\
Data File : P0056508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2019 1:05
Operator : SM/SJ
Sample : K2971-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SUP-2A-C-2-052019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:52:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

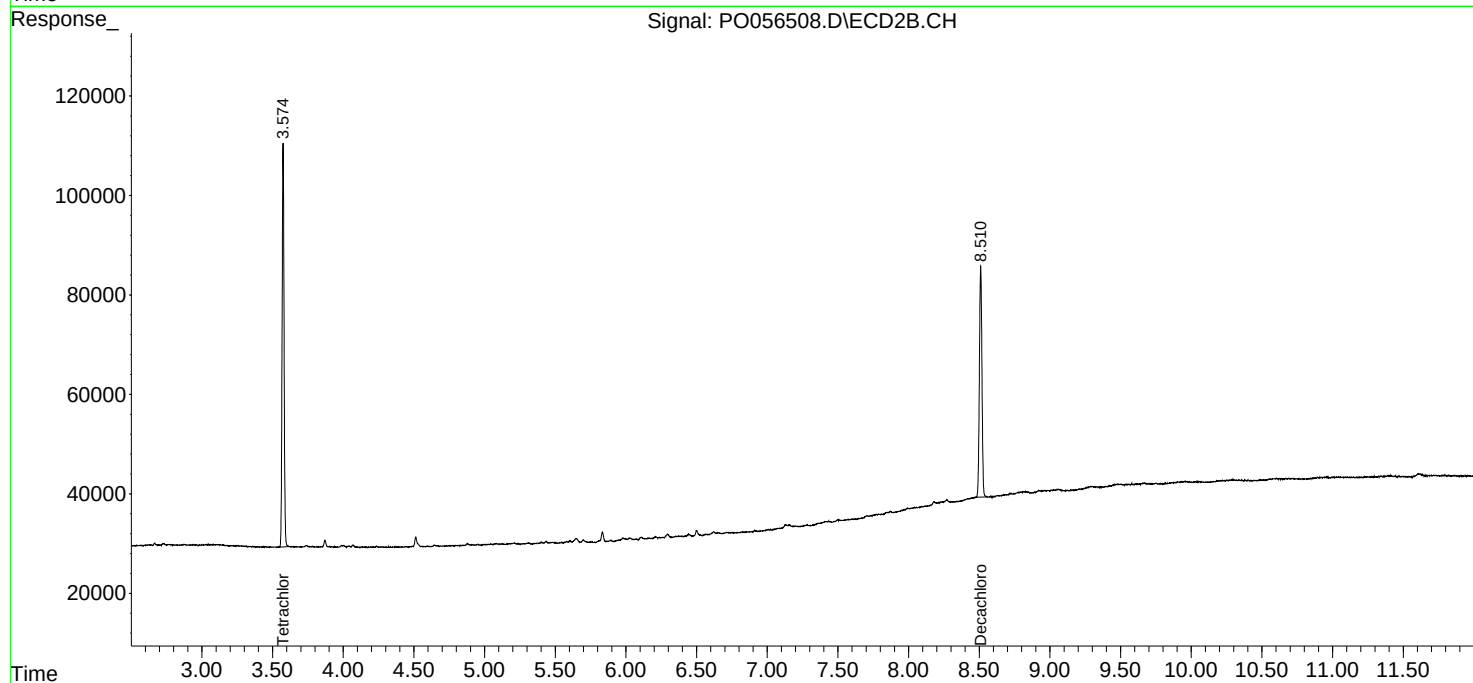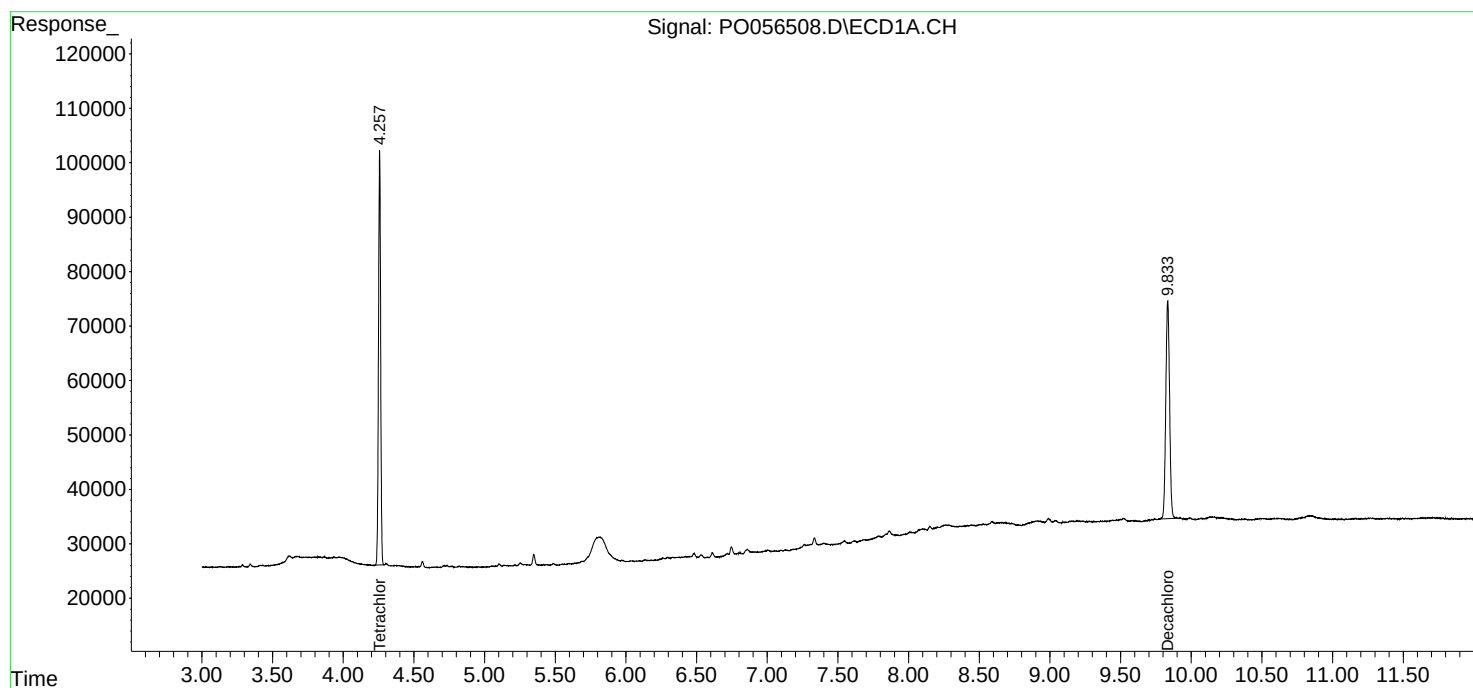


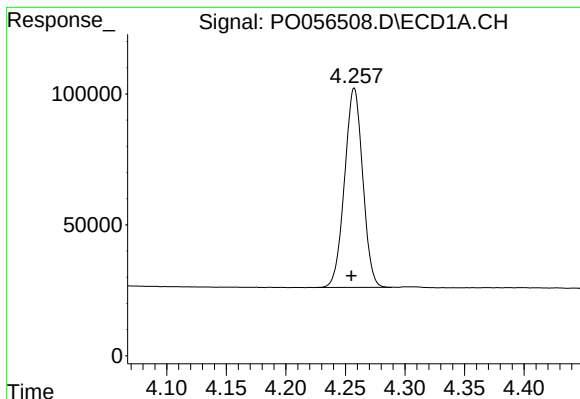

#1 Tetrachloro-m-xylene


R.T.: 4.257 min
Delta R.T.: 0.002 min
Response: 807003
Conc: 28.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
SUP-2A-C-2-052019

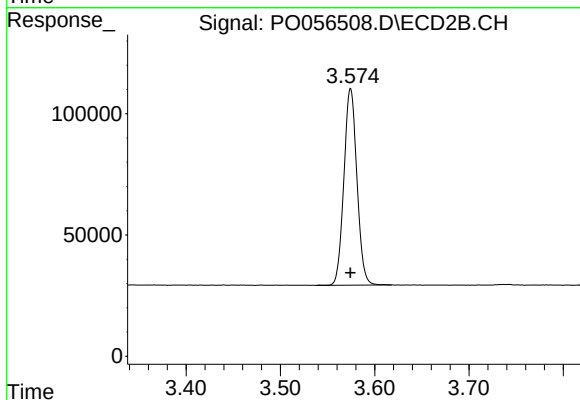


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.000 min
Response: 778269
Conc: 28.86 ng/ml

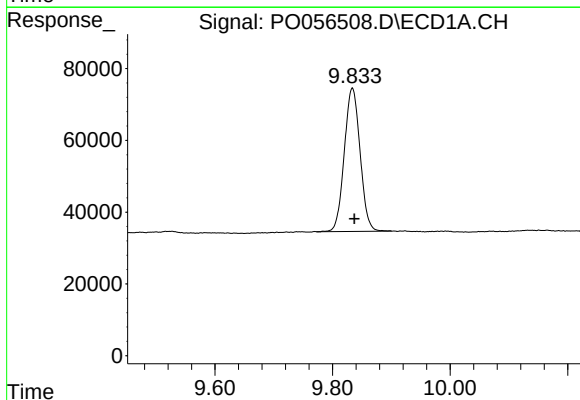

#2 Decachlorobiphenyl

R.T.: 9.834 min
Delta R.T.: -0.003 min
Response: 743760
Conc: 14.58 ng/ml

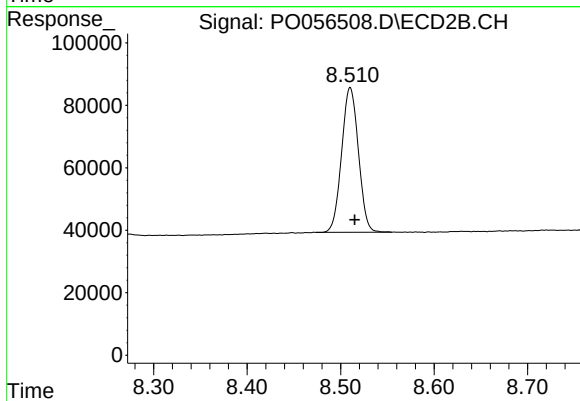

#2 Decachlorobiphenyl

R.T.: 8.510 min
Delta R.T.: -0.005 min
Response: 578113
Conc: 13.16 ng/ml