

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052219\
 Data File : P0056516.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 May 2019 3:21
 Operator : SM/SJ
 Sample : K2978-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CONCRETE-COMP

Manual Integrations
 APPROVED

Ankita
 5/24/2019 9:58:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 05:05:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.257	3.575	785335	798943	27.268m	29.624
2) SA Decachlor...	9.836	8.512	718956	620773	14.090m	14.131

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052219\
Data File : P0056516.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2019 3:21
Operator : SM/SJ
Sample : K2978-04
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONCRETE-COMP


Manual Integrations
APPROVED

Ankita
5/24/2019 9:58:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 05:05:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

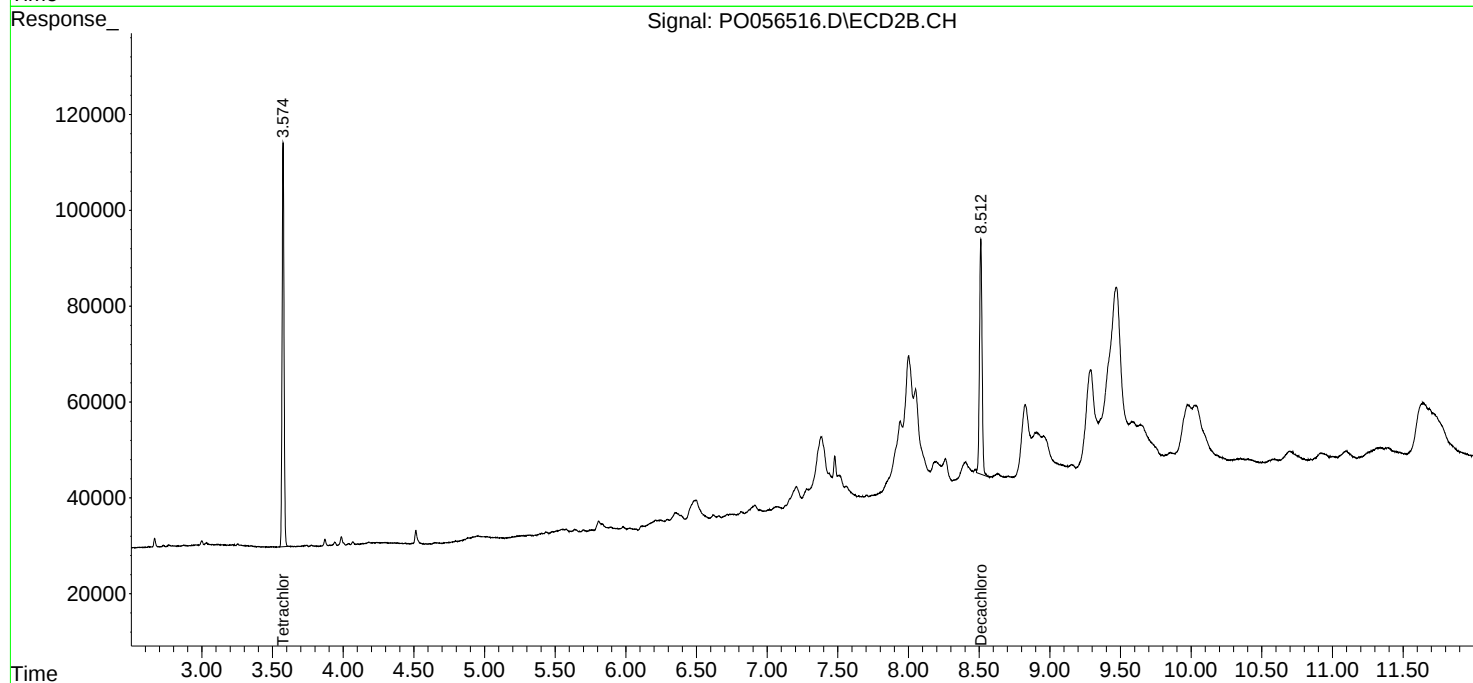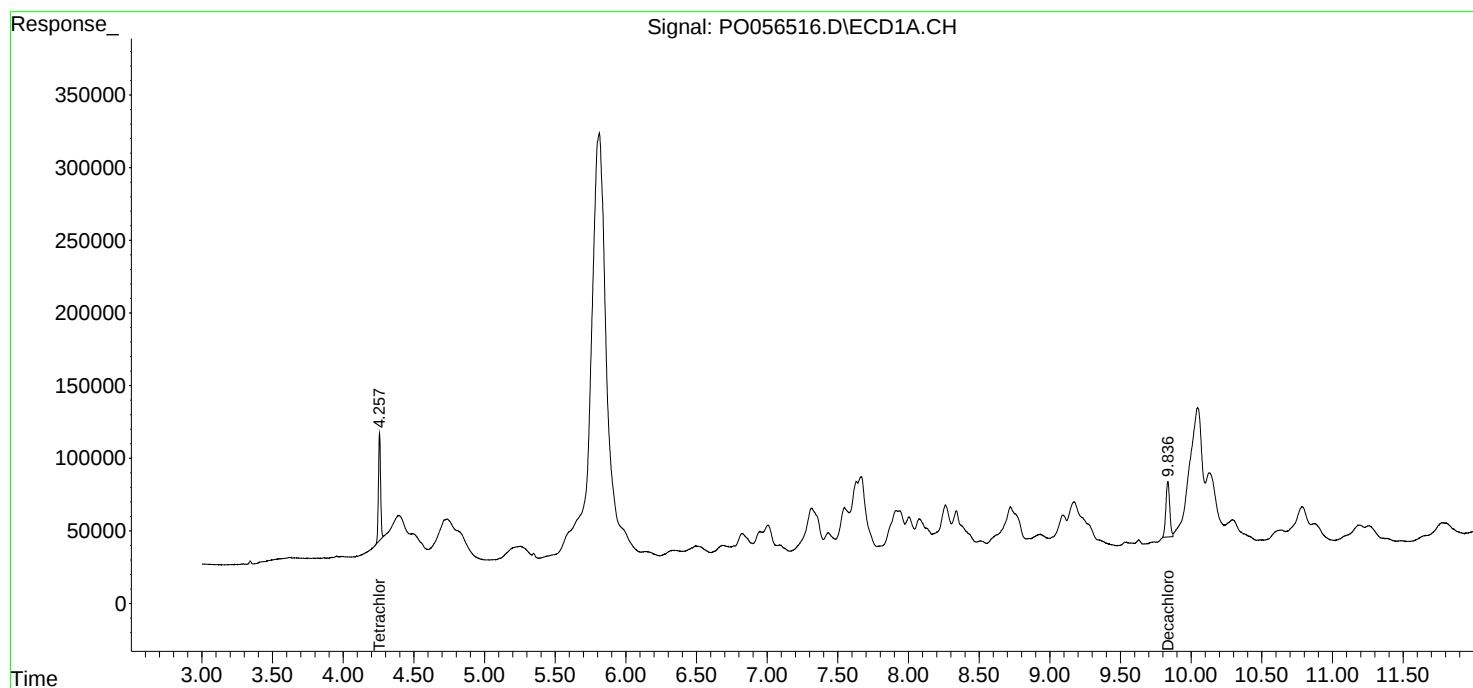

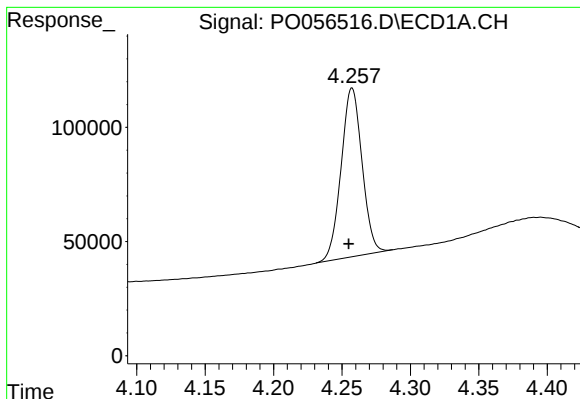


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: 0.002 min
Response: 785335
Conc: 27.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONCRETE-COMP


Manual Integrations
APPROVED

Ankita
5/24/2019 9:58:05 AM

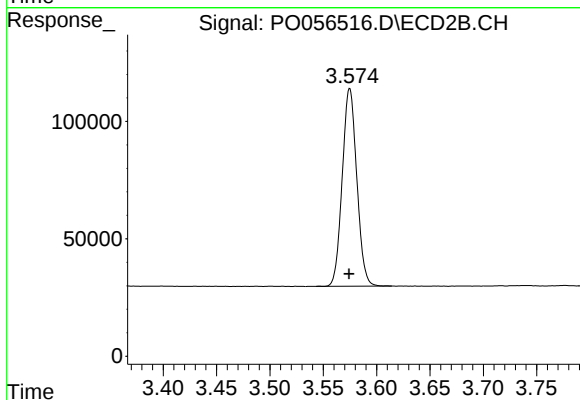


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.000 min
Response: 798943
Conc: 29.62 ng/ml

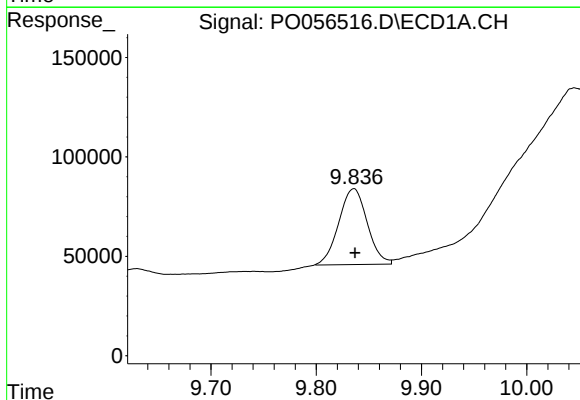

#2 Decachlorobiphenyl

R.T.: 9.836 min
Delta R.T.: -0.001 min
Response: 718956
Conc: 14.09 ng/ml m

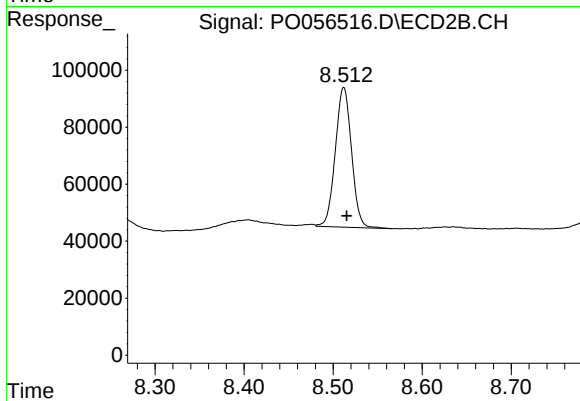

#2 Decachlorobiphenyl

R.T.: 8.512 min
Delta R.T.: -0.003 min
Response: 620773
Conc: 14.13 ng/ml