

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044956.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 17:05
Operator : SM/UA
Sample : J3008-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-D-S

Manual Integrations
APPROVED

ugo
5/24/2018 9:14:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:14:09 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.024	3.288	4865259	6062781	31.749	25.291
2) SA Decachlor...	9.327	8.022	4245847	5396986	20.650m	19.180m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044956.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 17:05
Operator : SM/UA
Sample : J3008-11
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-D-S


Manual Integrations
APPROVED

ugo
5/24/2018 9:14:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:14:09 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

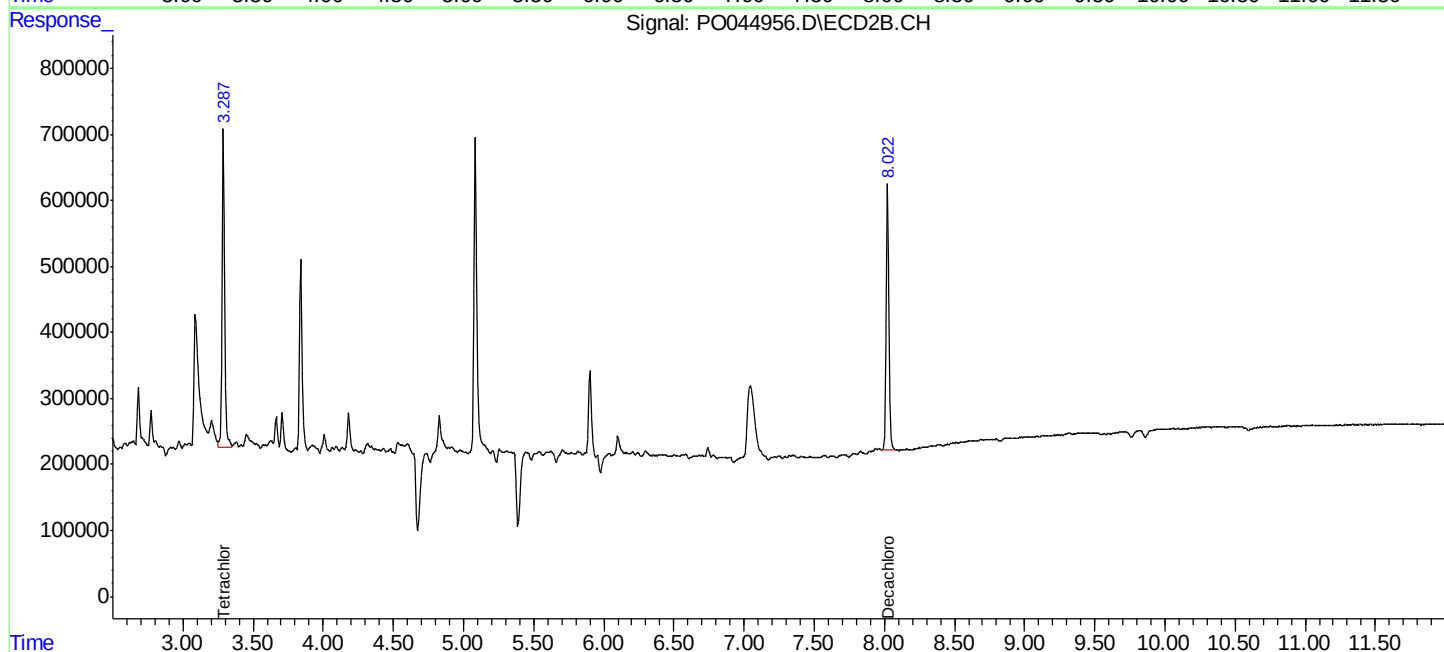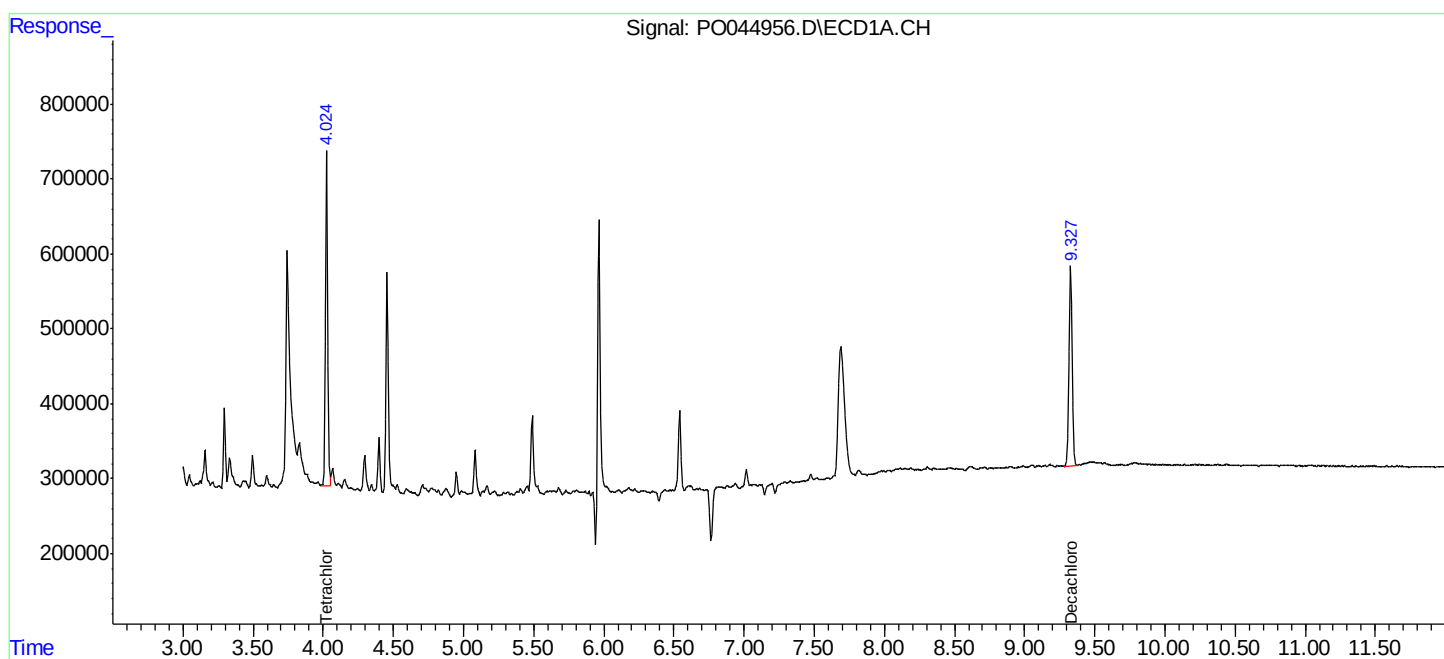

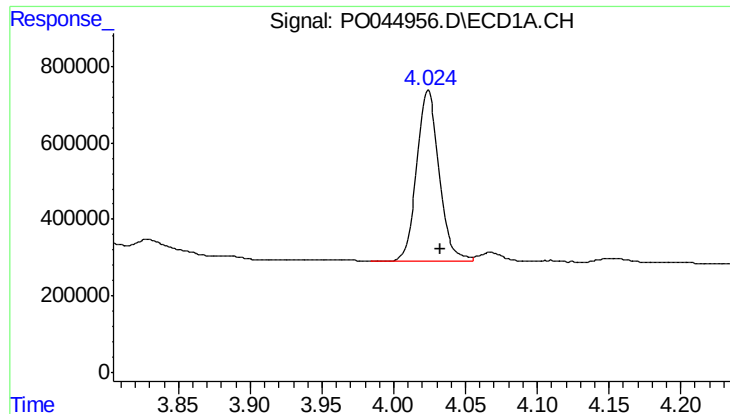


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: -0.009 min
Response: 4865259
Conc: 31.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-D-S


Manual Integrations
APPROVED

ugo
5/24/2018 9:14:17 PM

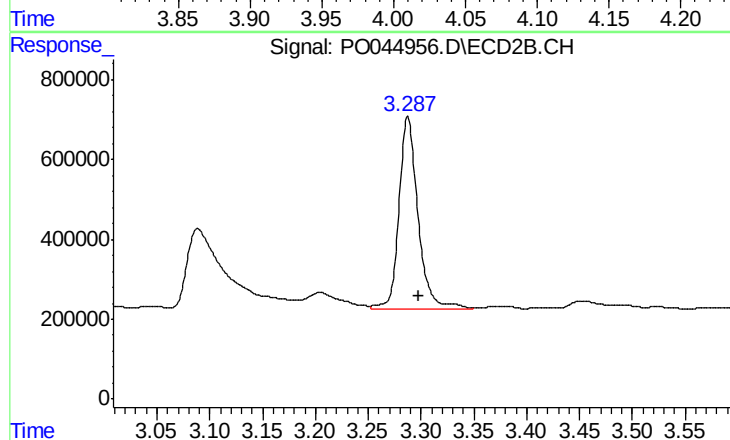


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: -0.010 min
Response: 6062781
Conc: 25.29 ng/ml

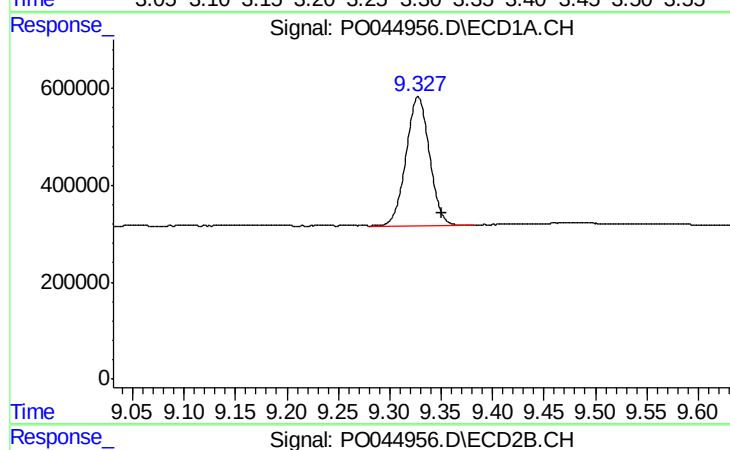

#2 Decachlorobiphenyl

R.T.: 9.327 min
Delta R.T.: -0.023 min
Response: 4245847
Conc: 20.65 ng/ml m

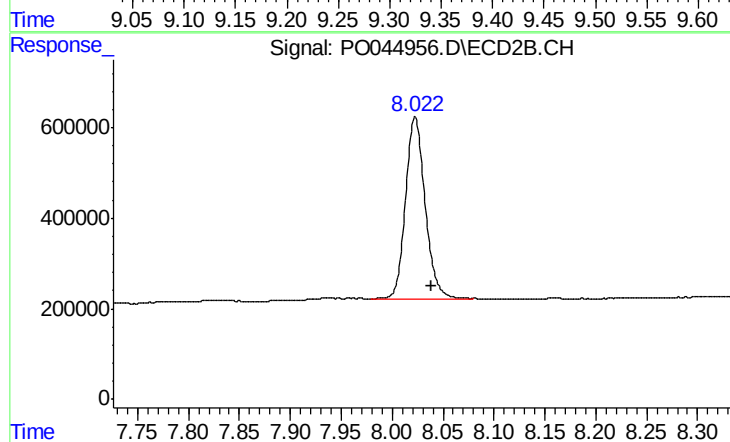

#2 Decachlorobiphenyl

R.T.: 8.022 min
Delta R.T.: -0.016 min
Response: 5396986
Conc: 19.18 ng/ml m