

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044957.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 17:20
Operator : SM/UA
Sample : J3008-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-U-B

Manual Integrations
APPROVED

ugo
5/24/2018 9:13:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:15:24 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.018	3.289	3908678	4951852	25.507	20.657
2) SA Decachlor...	9.318	8.019	3945152	5108427	19.187m	18.155m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044957.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 17:20
Operator : SM/UA
Sample : J3008-12
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-U-B


Manual Integrations
APPROVED

ugo
5/24/2018 9:13:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:15:24 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

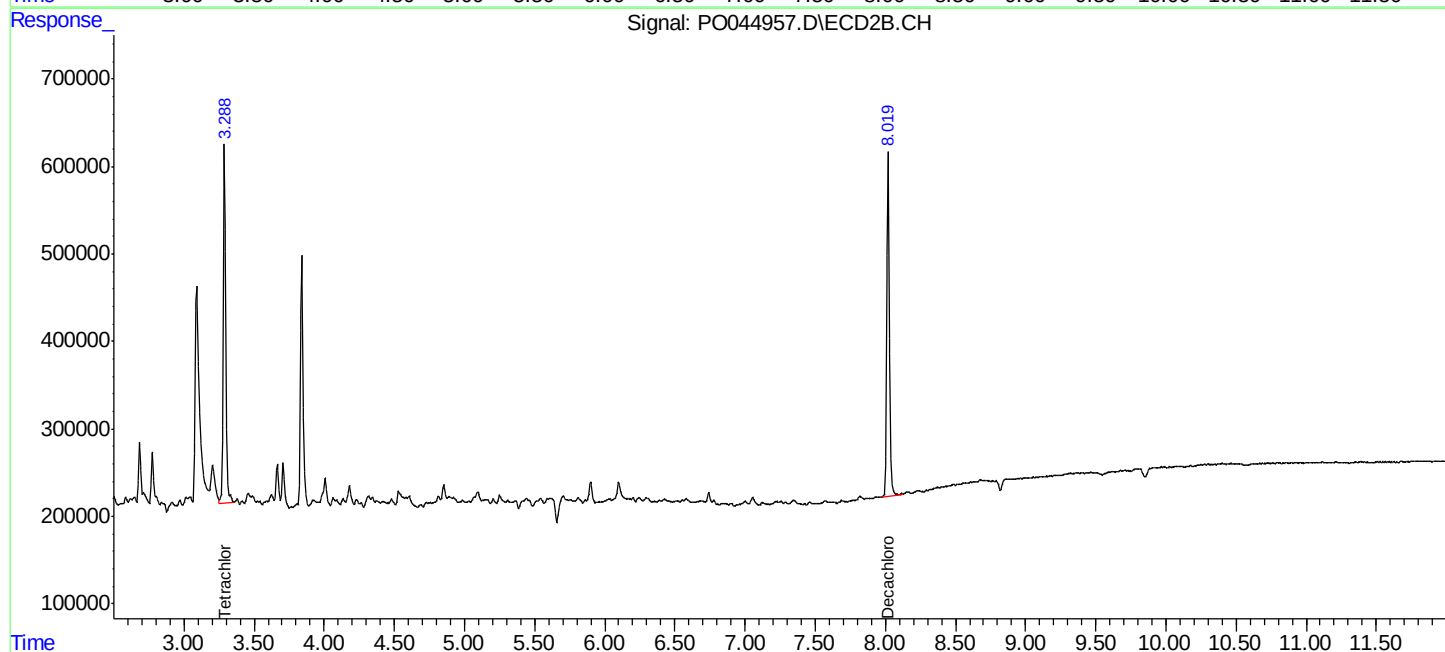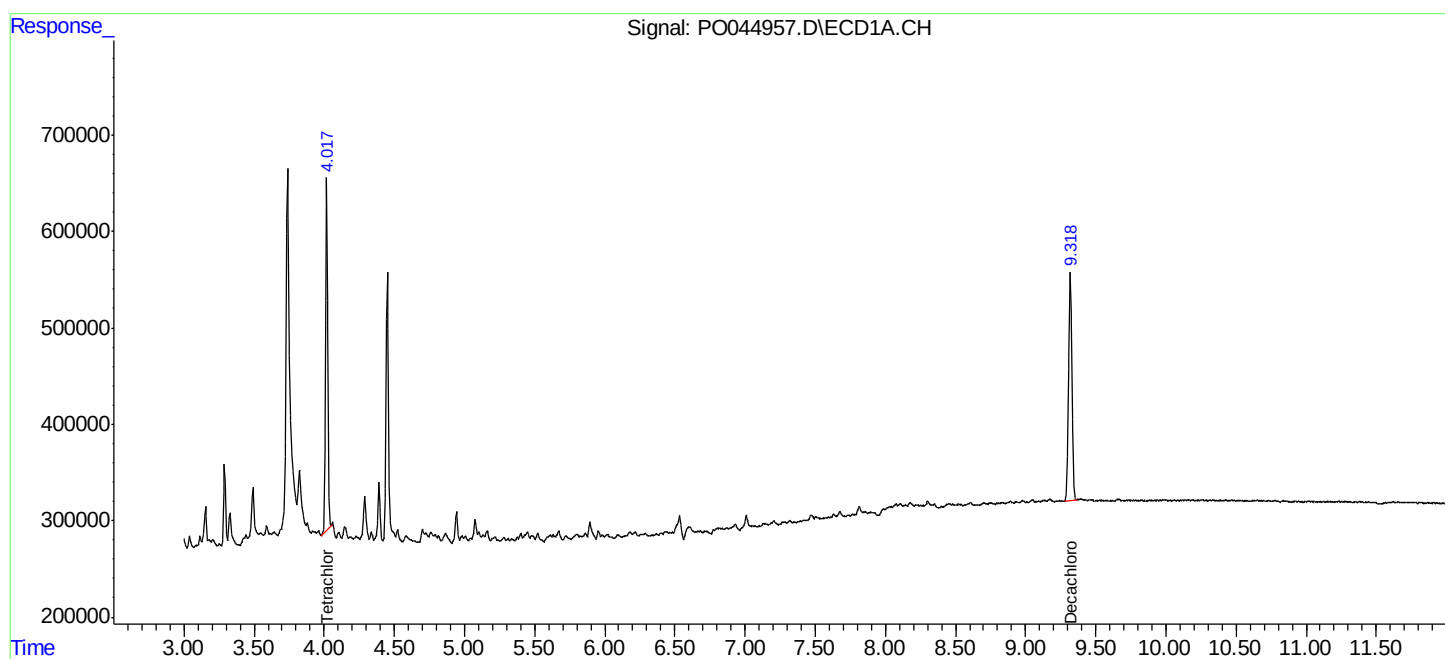

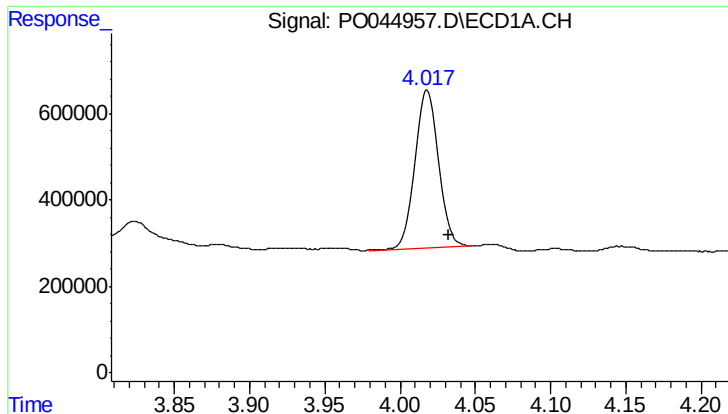


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: -0.015 min
Response: 3908678
Conc: 25.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
051618-SIDI-F-U-B


Manual Integrations
APPROVED

ugo
5/24/2018 9:13:06 PM

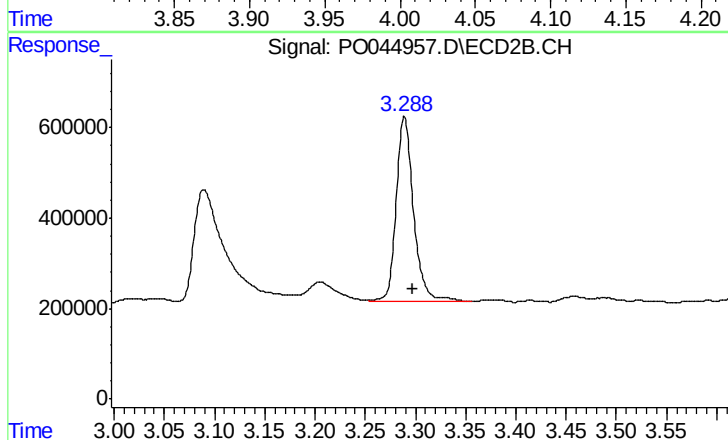


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: -0.009 min
Response: 4951852
Conc: 20.66 ng/ml

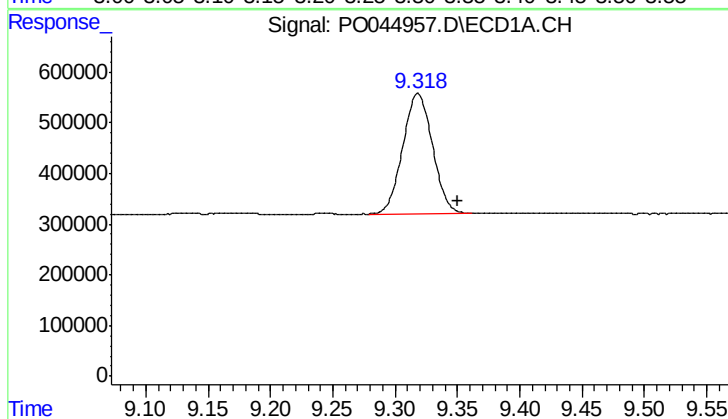

#2 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: -0.033 min
Response: 3945152
Conc: 19.19 ng/ml m

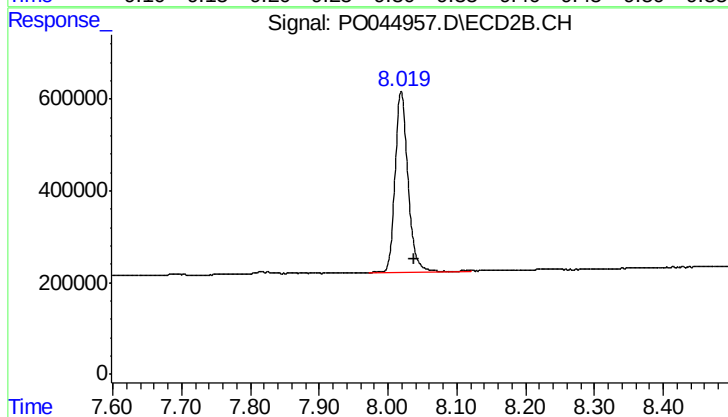

#2 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.020 min
Response: 5108427
Conc: 18.15 ng/ml m