

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 20:51
Operator : SM/UA
Sample : J3009-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
051718-SIDI-E-D-B

Manual Integrations
APPROVED

ugo
5/24/2018 9:11:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 04:09:05 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.017	3.289	4768553	5722585	31.118	23.872
2) SA Decachlor...	9.315	8.019	4275063	5690751	20.792	20.224m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0044971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2018 20:51
Operator : SM/UA
Sample : J3009-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
051718-SIDI-E-D-B


Manual Integrations
APPROVED

ugo
5/24/2018 9:11:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 04:09:05 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

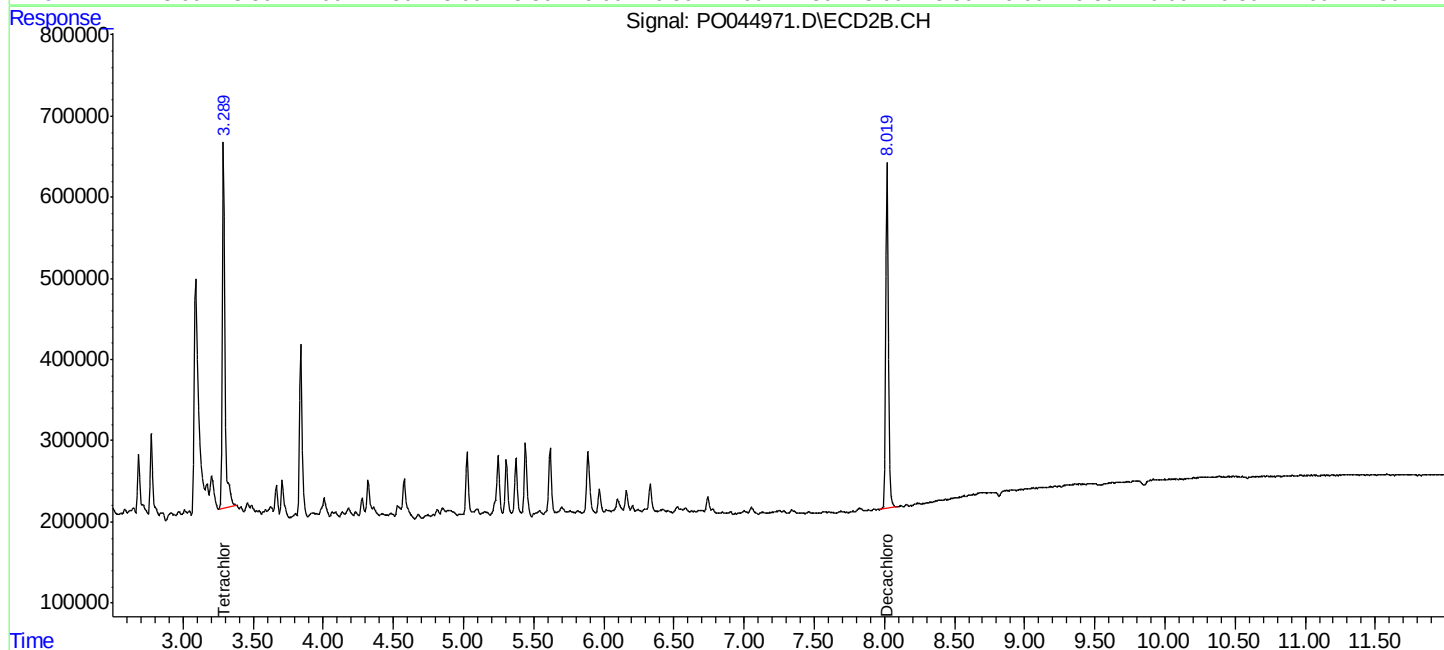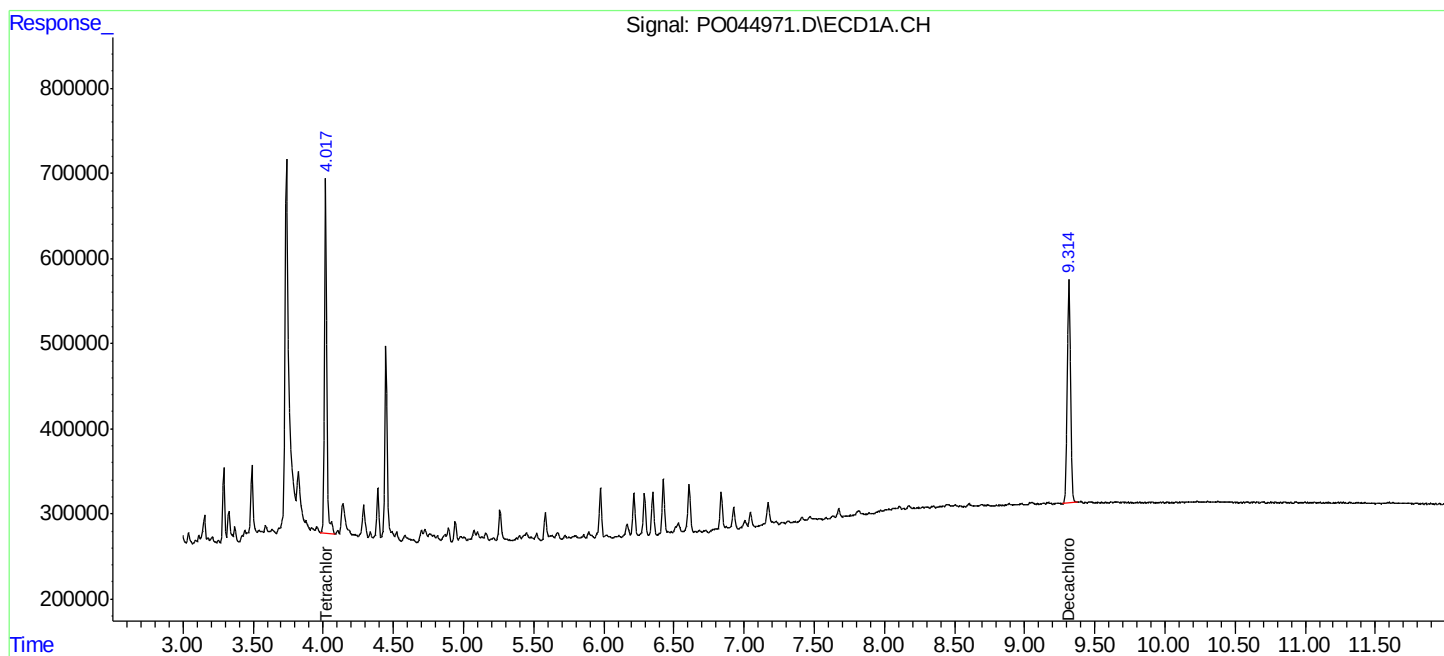

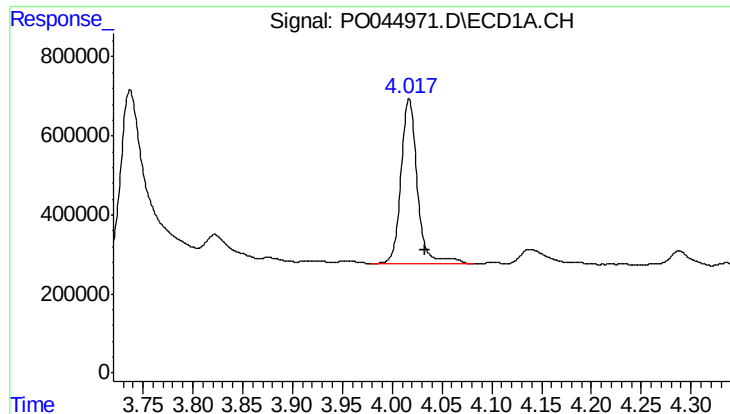


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: -0.016 min
Response: 4768553
Conc: 31.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
051718-SIDI-E-D-B


Manual Integrations
APPROVED

ugo
5/24/2018 9:11:49 PM

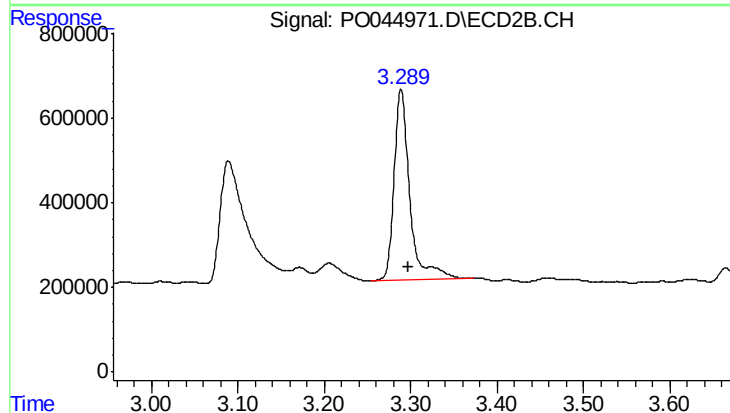


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: -0.009 min
Response: 5722585
Conc: 23.87 ng/ml

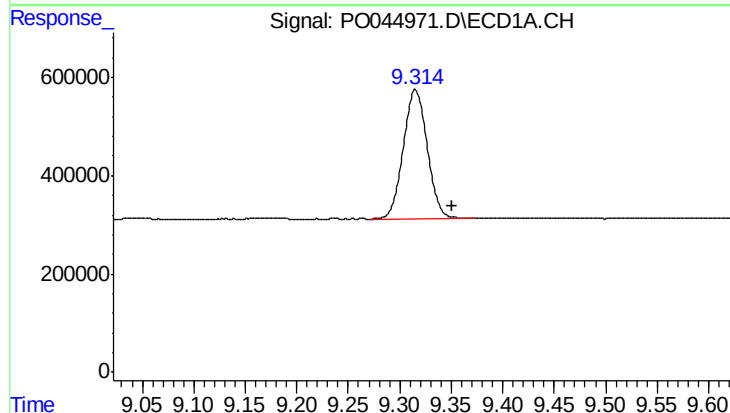

#2 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: -0.035 min
Response: 4275063
Conc: 20.79 ng/ml

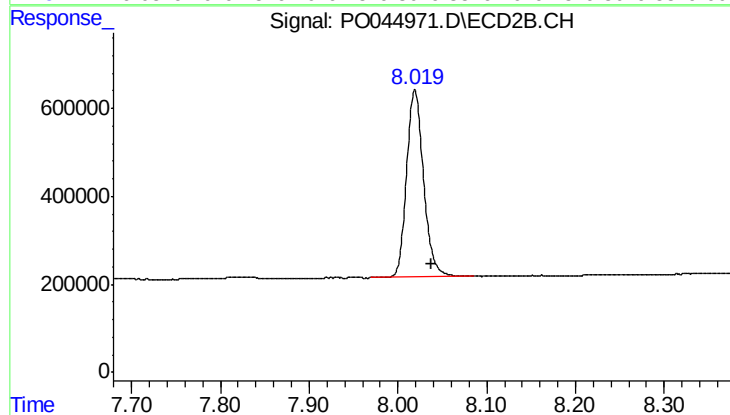

#2 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.020 min
Response: 5690751
Conc: 20.22 ng/ml m