

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
 Data File : P0045002.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2018 4:37
 Operator : SM/UA
 Sample : J3047-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 051818-SIDI-E-U-M

Manual Integrations
 APPROVED

ugo
 5/24/2018 9:11:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 06:20:20 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 15 15:44:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.016	3.288	5091355	5954610	33.225	24.840 #
2) SA Decachlor...	9.313	8.017	4194695	5505135	20.401	19.565m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0045002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2018 4:37
Operator : SM/UA
Sample : J3047-05
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
051818-SIDI-E-U-M


Manual Integrations
APPROVED

ugo
5/24/2018 9:11:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 06:20:20 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

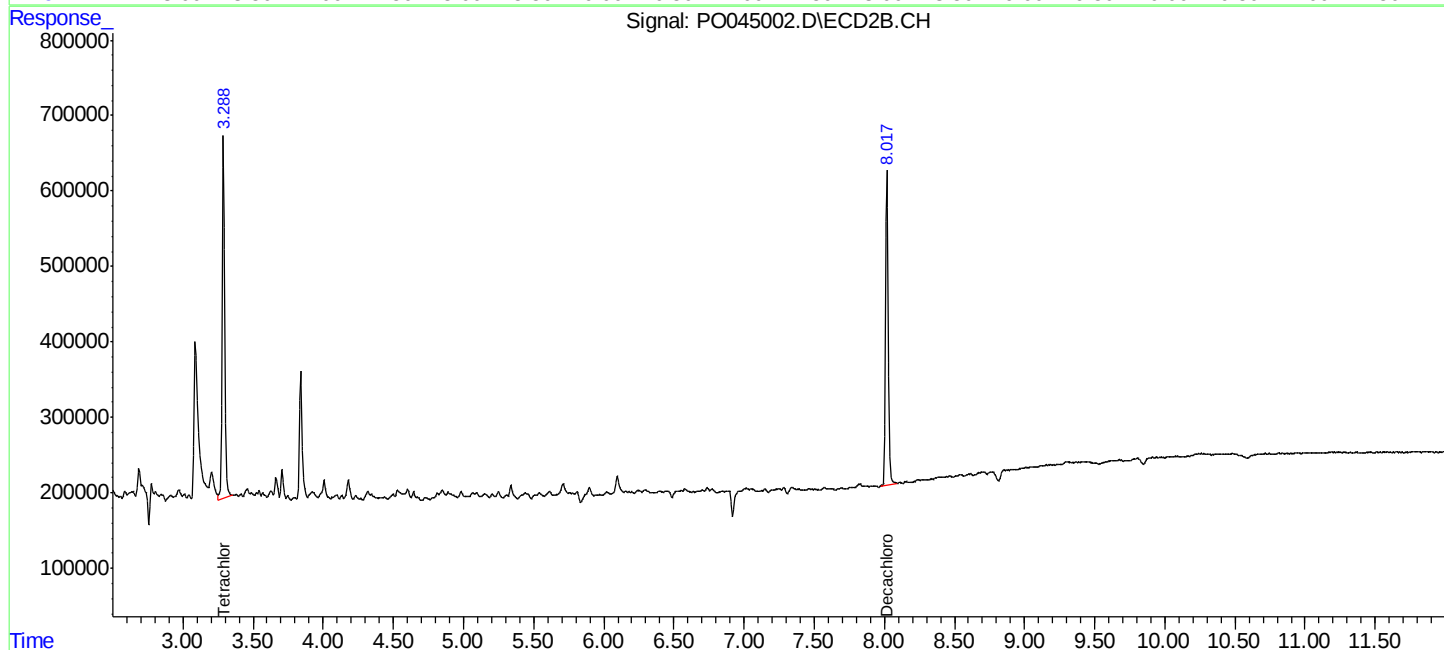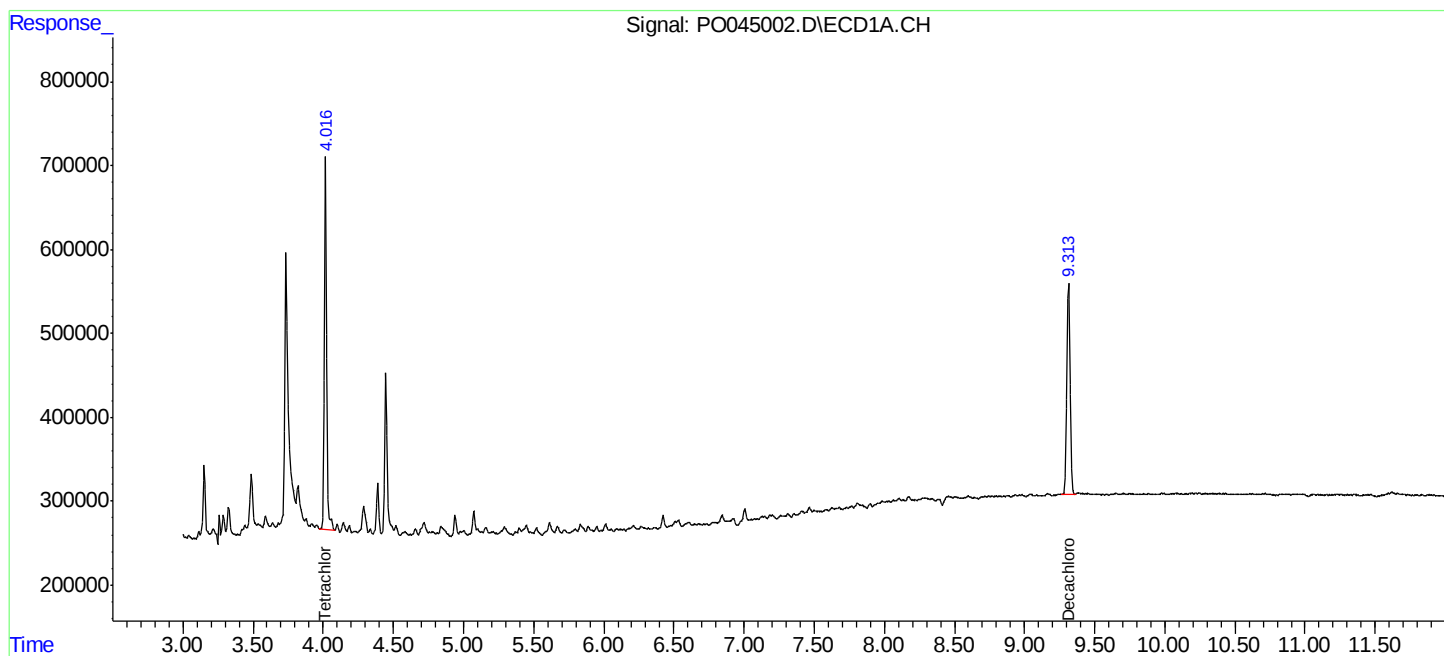

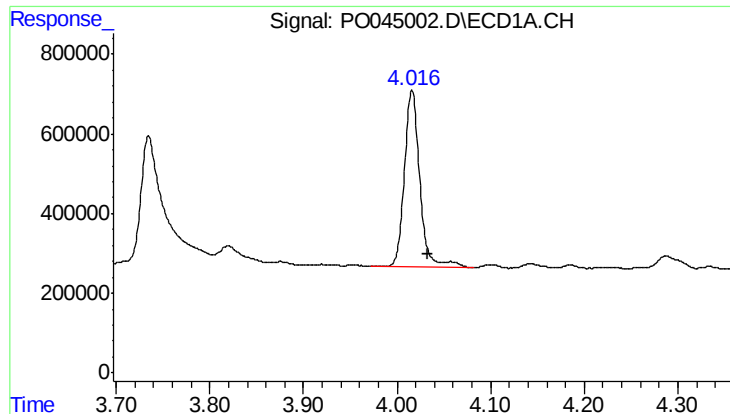


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: -0.017 min
Response: 5091355
Conc: 33.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
051818-SIDI-E-U-M


Manual Integrations
APPROVED

ugo
5/24/2018 9:11:02 PM

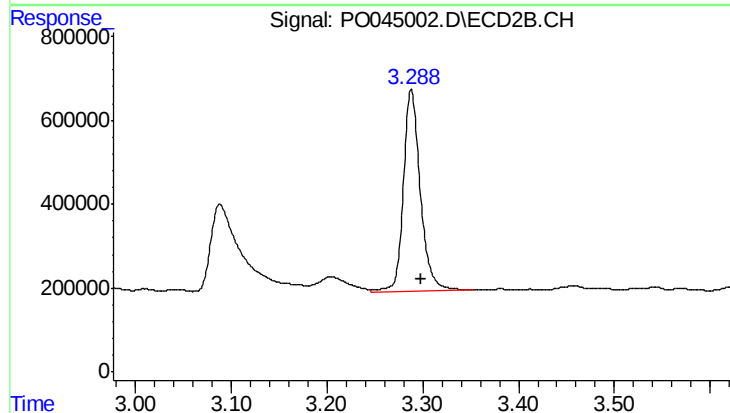


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: -0.010 min
Response: 5954610
Conc: 24.84 ng/ml

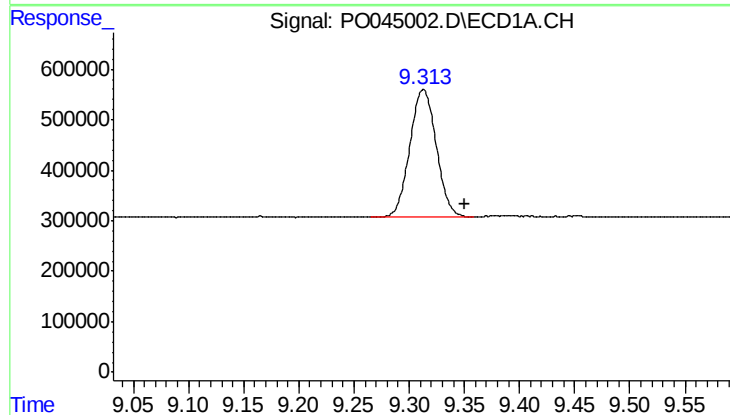

#2 Decachlorobiphenyl

R.T.: 9.313 min
Delta R.T.: -0.038 min
Response: 4194695
Conc: 20.40 ng/ml

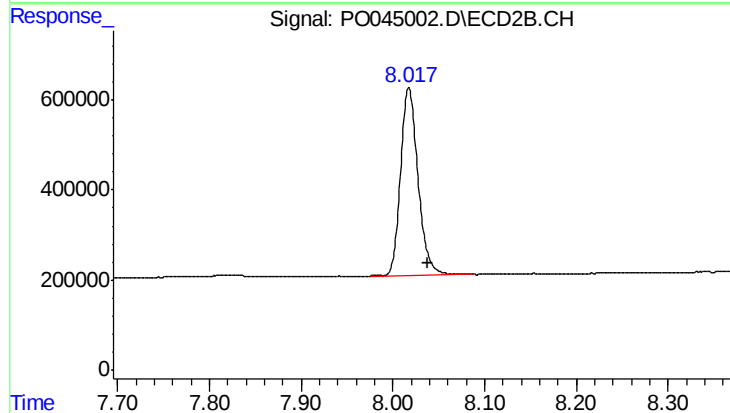

#2 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.022 min
Response: 5505135
Conc: 19.56 ng/ml m