

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
 Data File : P0045003.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2018 4:52
 Operator : SM/UA
 Sample : J3047-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 051818-SIDI-E-U-S

Manual Integrations
 APPROVED

ugo
 5/24/2018 9:10:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 06:22:24 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 15 15:44:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.016	3.288	5049828	5535800	32.954	23.093 #
2)	SA Decachlor...	9.313	8.017	4036624	5364739	19.632	19.066m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052318\
Data File : P0045003.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2018 4:52
Operator : SM/UA
Sample : J3047-06
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
051818-SIDI-E-U-S


Manual Integrations
APPROVED

ugo
5/24/2018 9:10:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 06:22:24 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0051518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 15 15:44:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

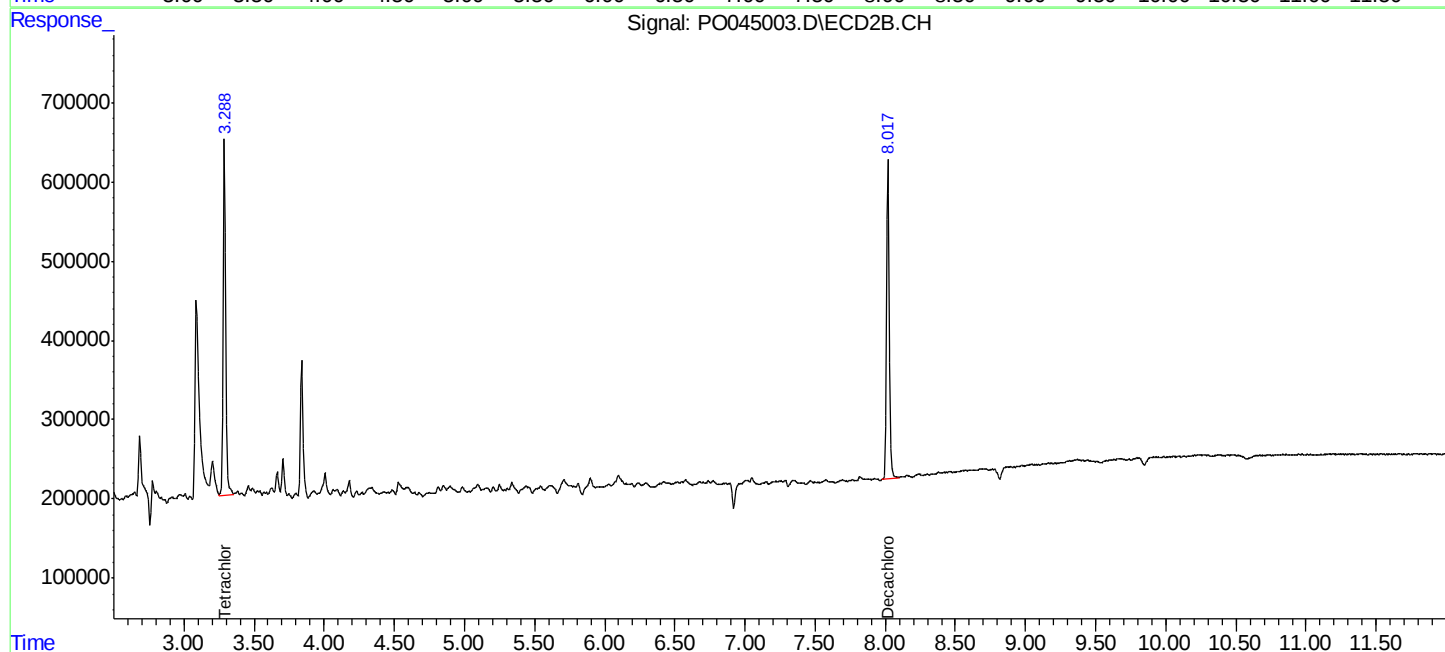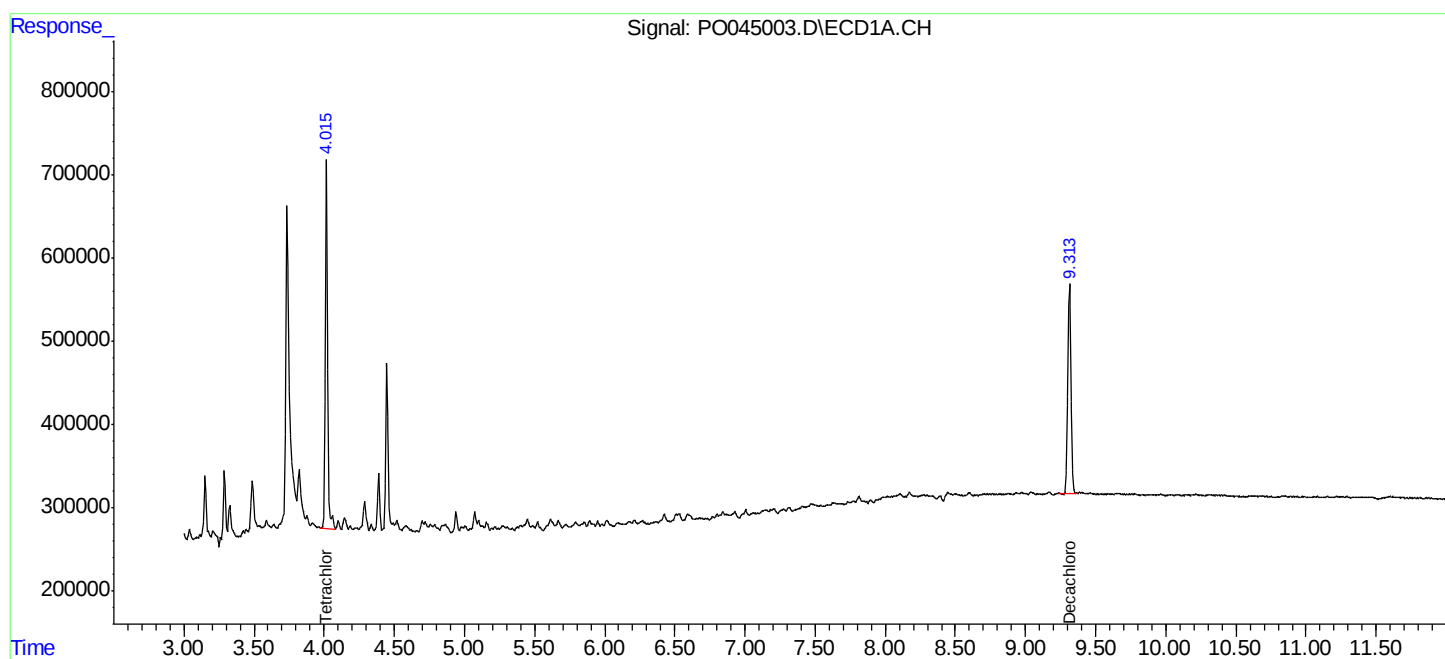

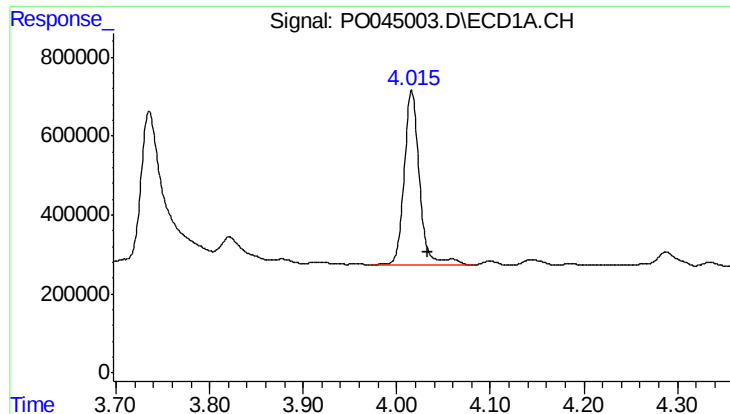


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: -0.017 min
Response: 5049828
Conc: 32.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
051818-SIDI-E-U-S


Manual Integrations
APPROVED

ugo
5/24/2018 9:10:12 PM

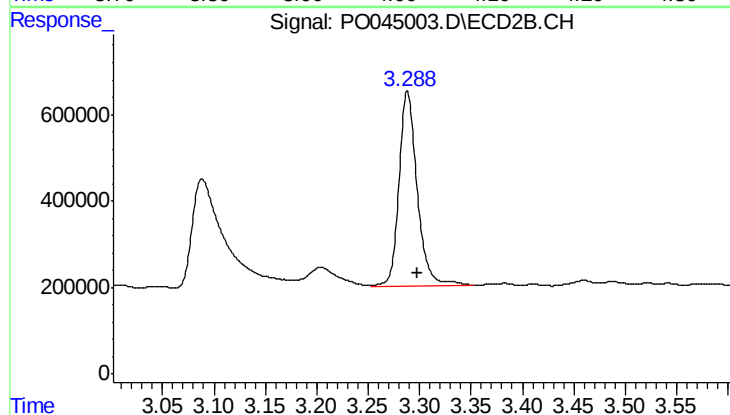


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: -0.010 min
Response: 5535800
Conc: 23.09 ng/ml

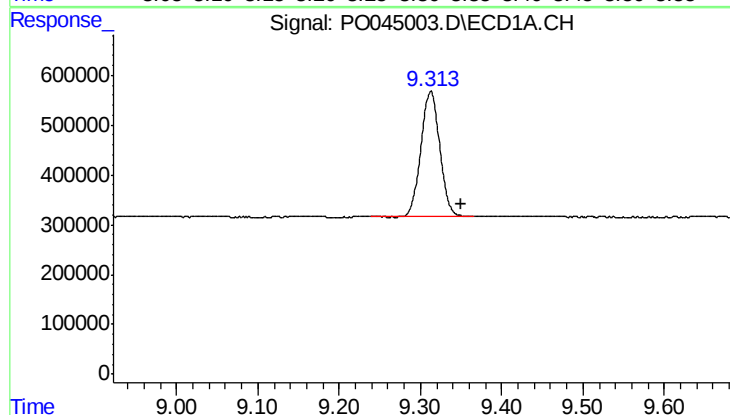

#2 Decachlorobiphenyl

R.T.: 9.313 min
Delta R.T.: -0.038 min
Response: 4036624
Conc: 19.63 ng/ml

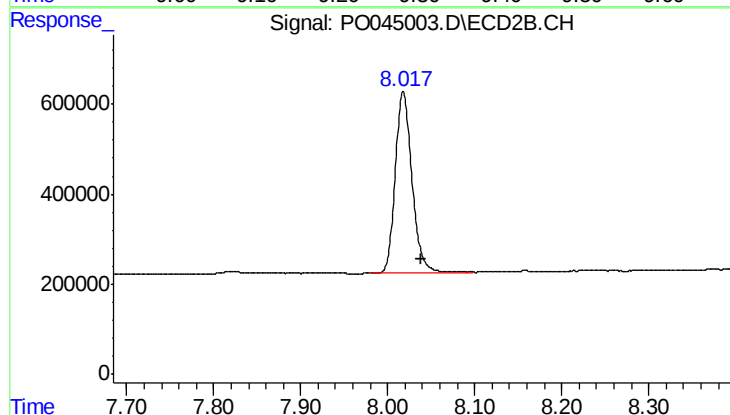

#2 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.021 min
Response: 5364739
Conc: 19.07 ng/ml m