

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052319\
Data File : P0056524.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2019 10:57
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Ankita
5/24/2019 3:11:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 00:12:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.271	3.573	672230	572300	17.559m	17.354
2) SA Decachlor...	9.859	8.517	825078	552356	16.810m	15.491

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052319\
Data File : P0056524.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 May 2019 10:57
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/24/2019 3:11:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 00:12:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

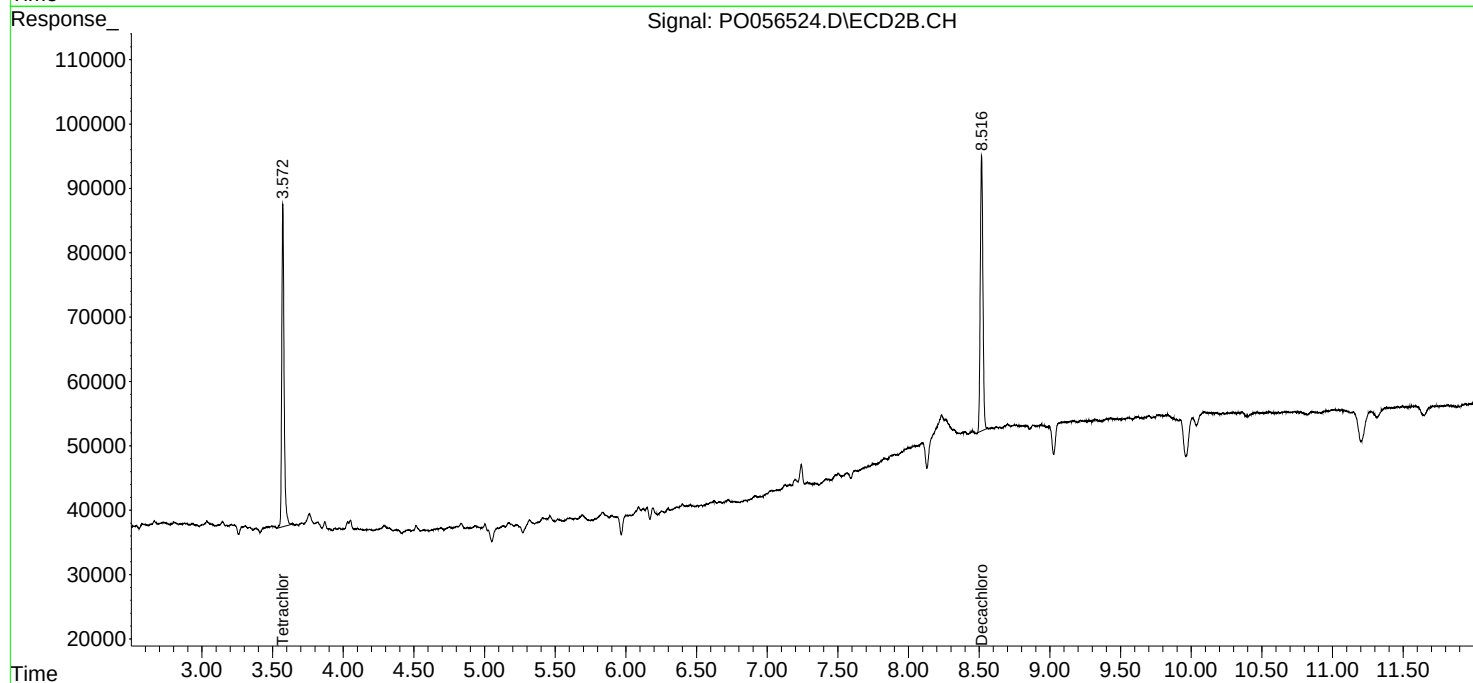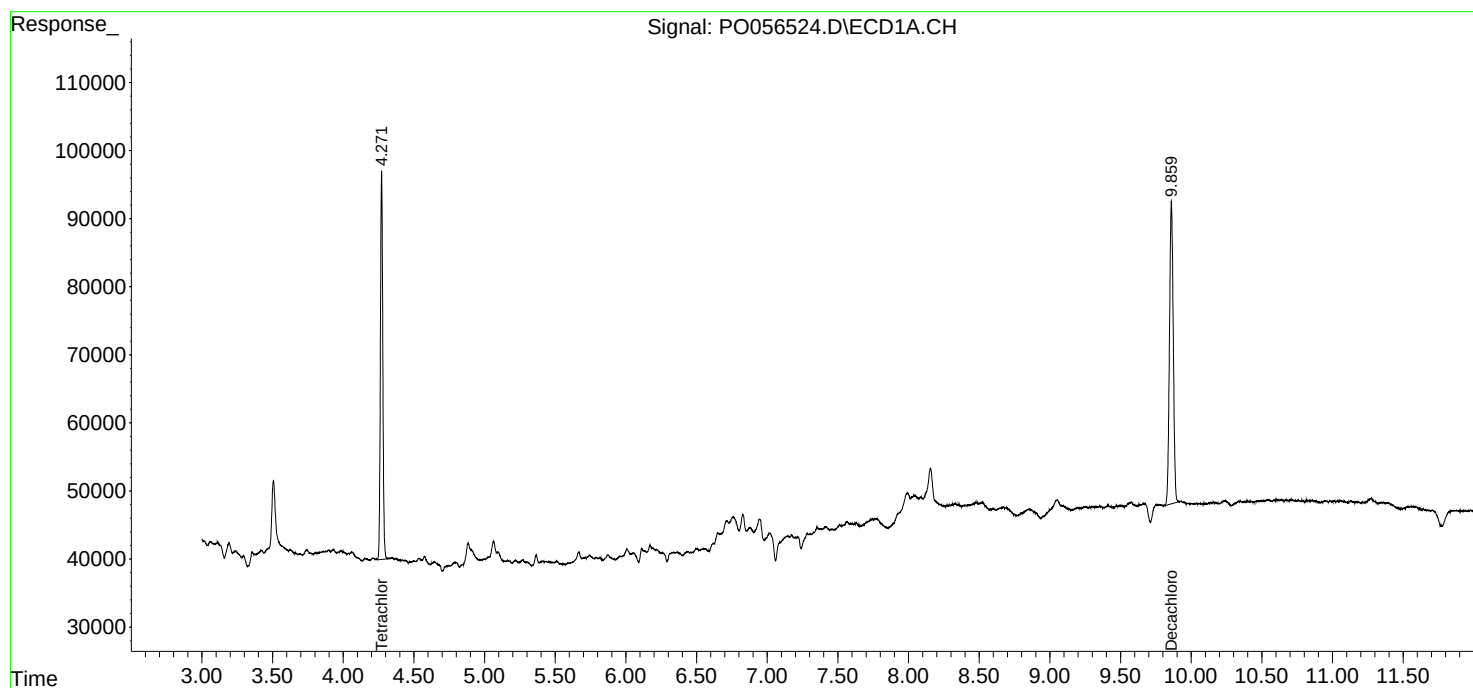

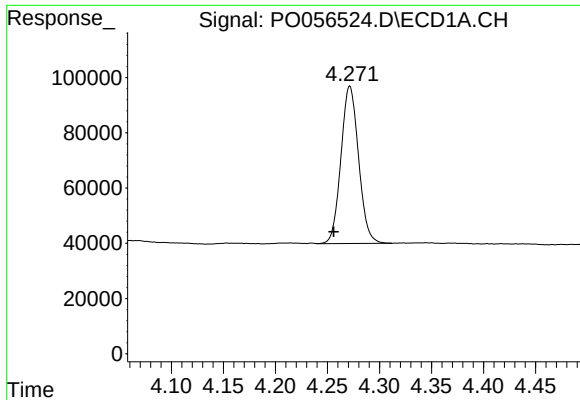


#1 Tetrachloro-m-xylene

R.T.: 4.271 min
Delta R.T.: 0.015 min
Response: 672230
Conc: 17.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/24/2019 3:11:37 PM

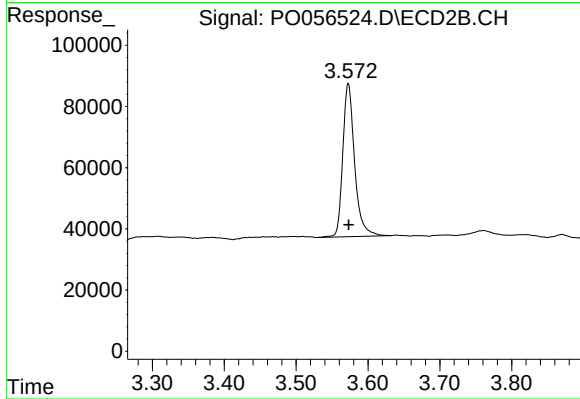


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 572300
Conc: 17.35 ng/ml

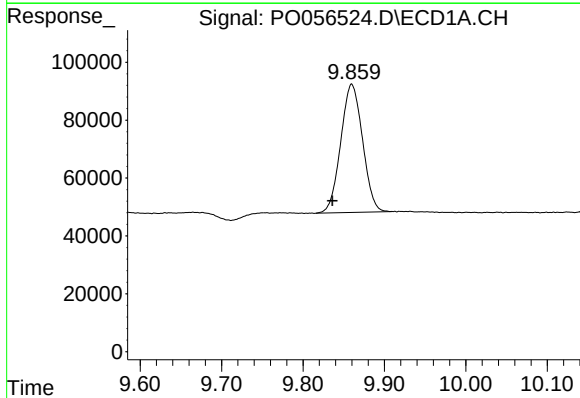

#2 Decachlorobiphenyl

R.T.: 9.859 min
Delta R.T.: 0.023 min
Response: 825078
Conc: 16.81 ng/ml m

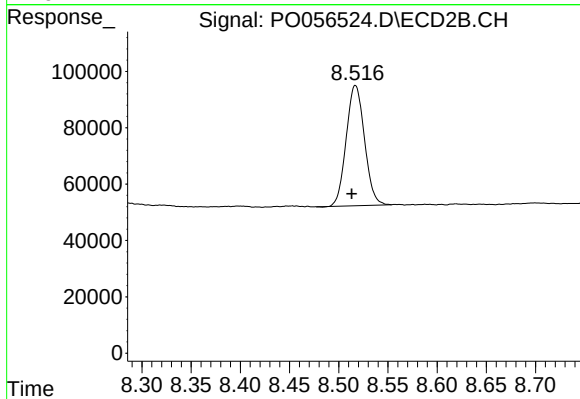

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: 0.004 min
Response: 552356
Conc: 15.49 ng/ml