

Data Path : P:\HPCHEM1\ECD_D\Data\PD052418\
 Data File : PD047904.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2018 3:42
 Operator : UA/AJ
 Sample : BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOQ-SCM-Precision-Bias-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:11:44 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD052418.M
 Quant Title : GC Extractables
 QLast Update : Thu May 24 12:13:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.424	4.039	23379867	397.3E6	20.361	22.095
28) SA Decachlor...	8.145	9.116	27447234	398.9E6	19.431	23.410
Target Compounds						
2) A alpha-BHC	0.000	4.440	0	8478512	N.D.	0.296 #
7) B delta-BHC	0.000	5.077	0	17712872	N.D.	0.682 #
23) Chlordane-1	0.000	5.077	0	17712872	N.D.	17.399 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD052418\
Data File : PD047904.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2018 3:42
Operator : UA/AJ
Sample : BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOQ-SCM-Precision-Bias-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:11:44 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD052418.M
Quant Title : GC Extractables
QLast Update : Thu May 24 12:13:46 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

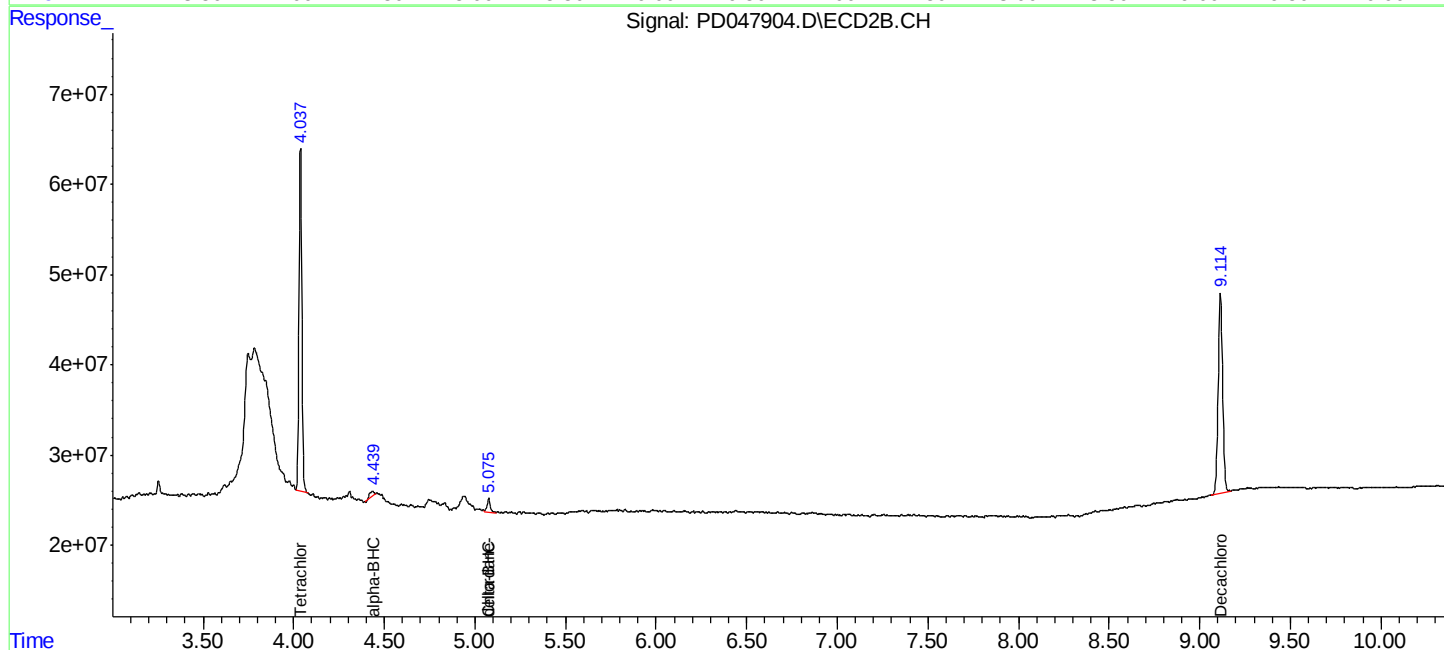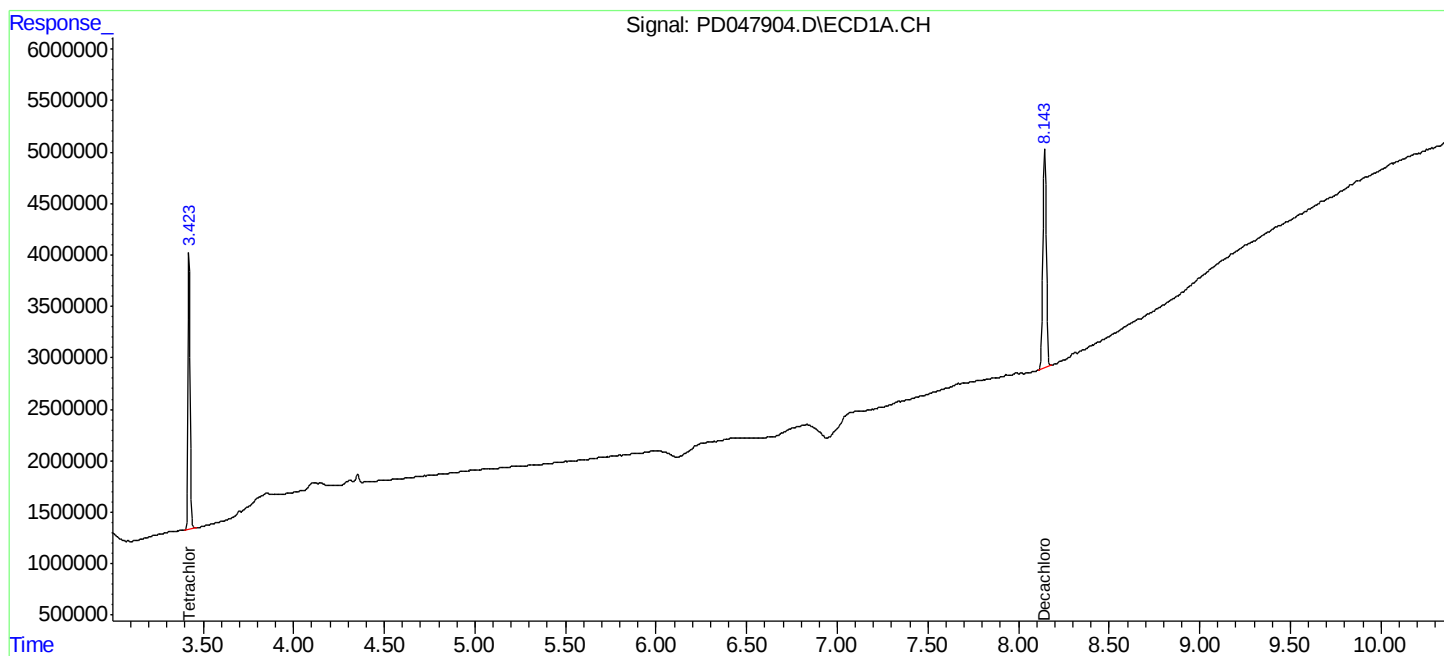


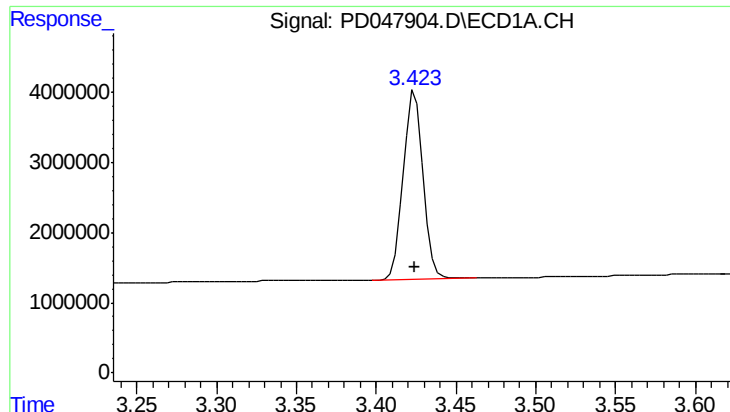

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: 0.000 min
Response: 23379867
Conc: 20.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-SCM-Precision-Bias-3

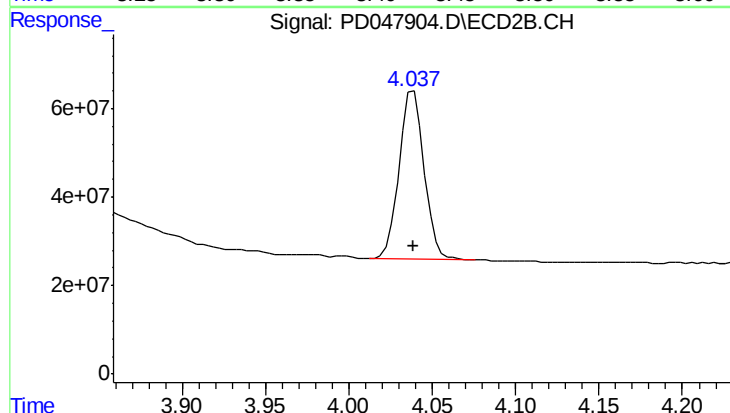


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: 0.000 min
Response: 397297815
Conc: 22.10 ng/ml

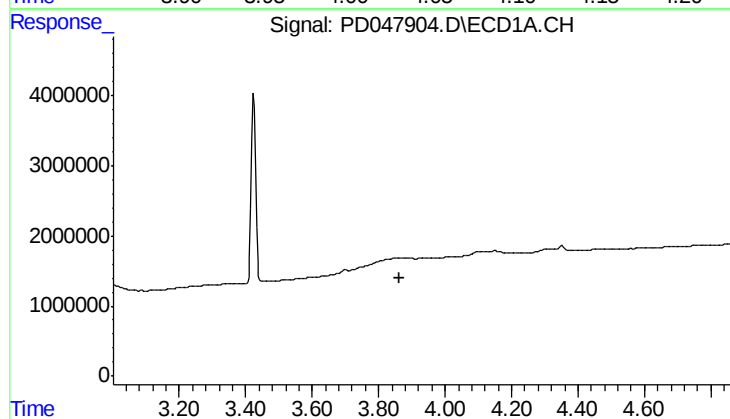


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 3.861 min
Response: 0
Conc: N.D.

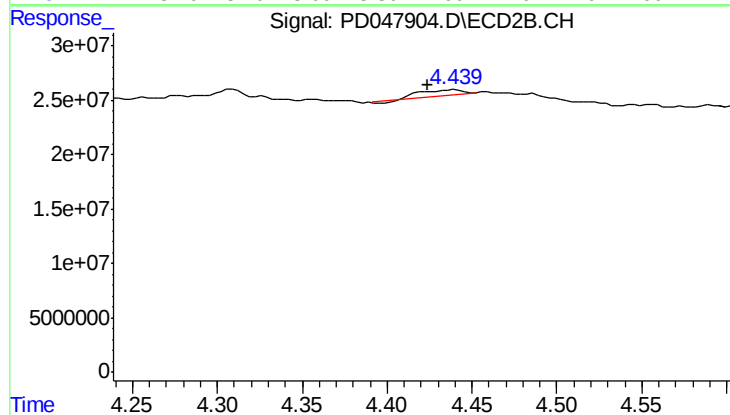

#2 alpha-BHC


R.T.: 4.440 min
Delta R.T.: 0.016 min
Response: 8478512
Conc: 0.30 ng/ml

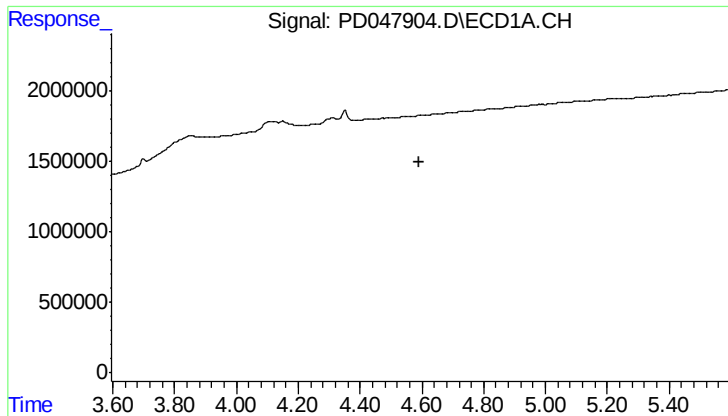

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOQ-SCM-Precision-Bias-3

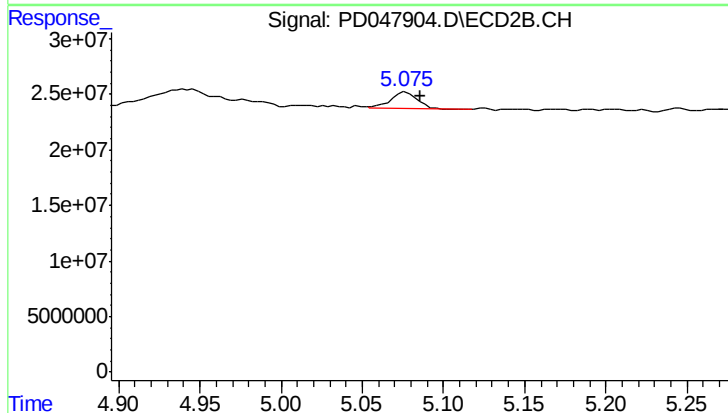


#7 delta-BHC

R.T.: 5.077 min
Delta R.T.: -0.009 min
Response: 17712872
Conc: 0.68 ng/ml

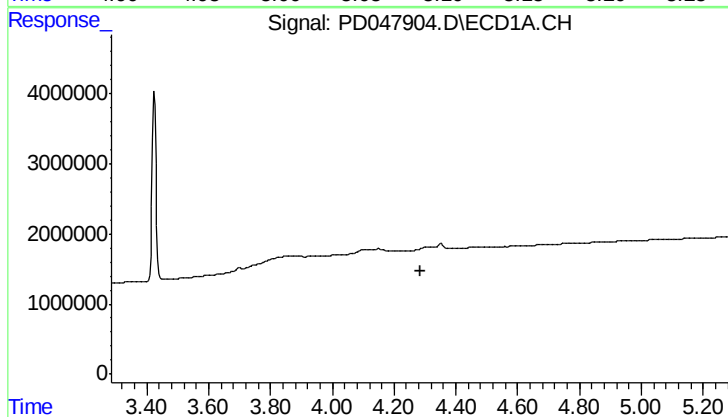


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.285 min
Response: 0
Conc: N.D.

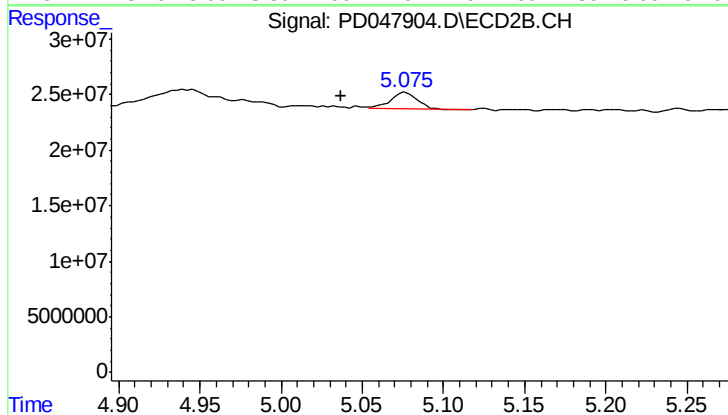

#23 Chlordane-1


R.T.: 5.077 min
Delta R.T.: 0.040 min
Response: 17712872
Conc: 17.40 ng/ml

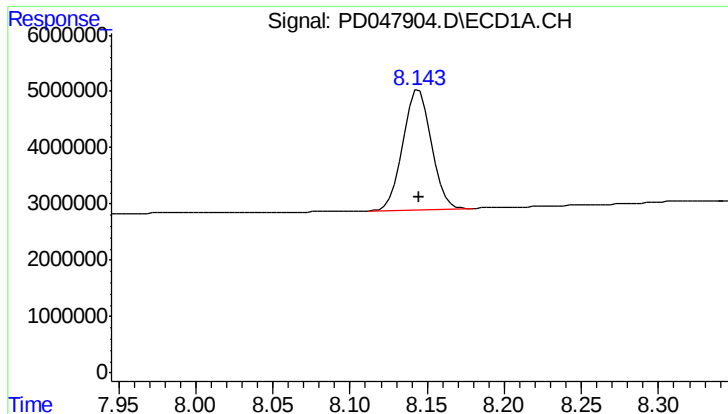

#28 Decachlorobiphenyl

R.T.: 8.145 min
Delta R.T.: 0.000 min
Response: 27447234
Conc: 19.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-SCM-Precision-Bias-3

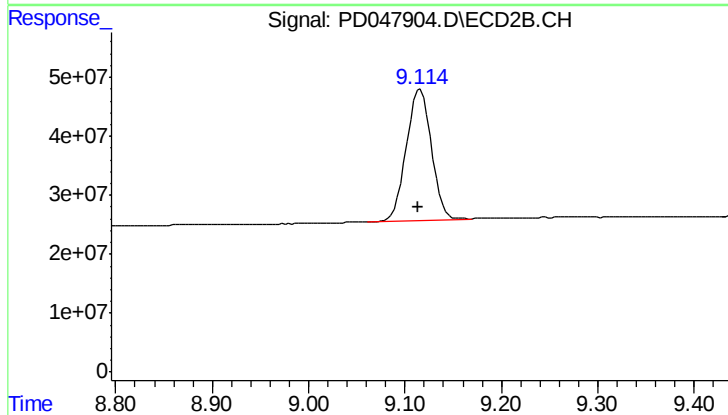

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.002 min
Response: 398862997
Conc: 23.41 ng/ml