

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052720\
 Data File : P0068580.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2020 8:31
 Operator : DD\AJ
 Sample : L2745-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NM76-COMP-2020-0-6

Manual Integrations
 APPROVED

Sohil
 5/28/2020 4:09:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 12:33:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.901	3.931	598173	875279	21.328m	25.508
2) SA Decachlor...	10.842	9.201	505281	617902	12.698m	16.050m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052720\
Data File : P0068580.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2020 8:31
Operator : DD\AJ
Sample : L2745-10
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NM76-COMP-2020-0-6


Manual Integrations
APPROVED

Sohil
5/28/2020 4:09:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 12:33:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

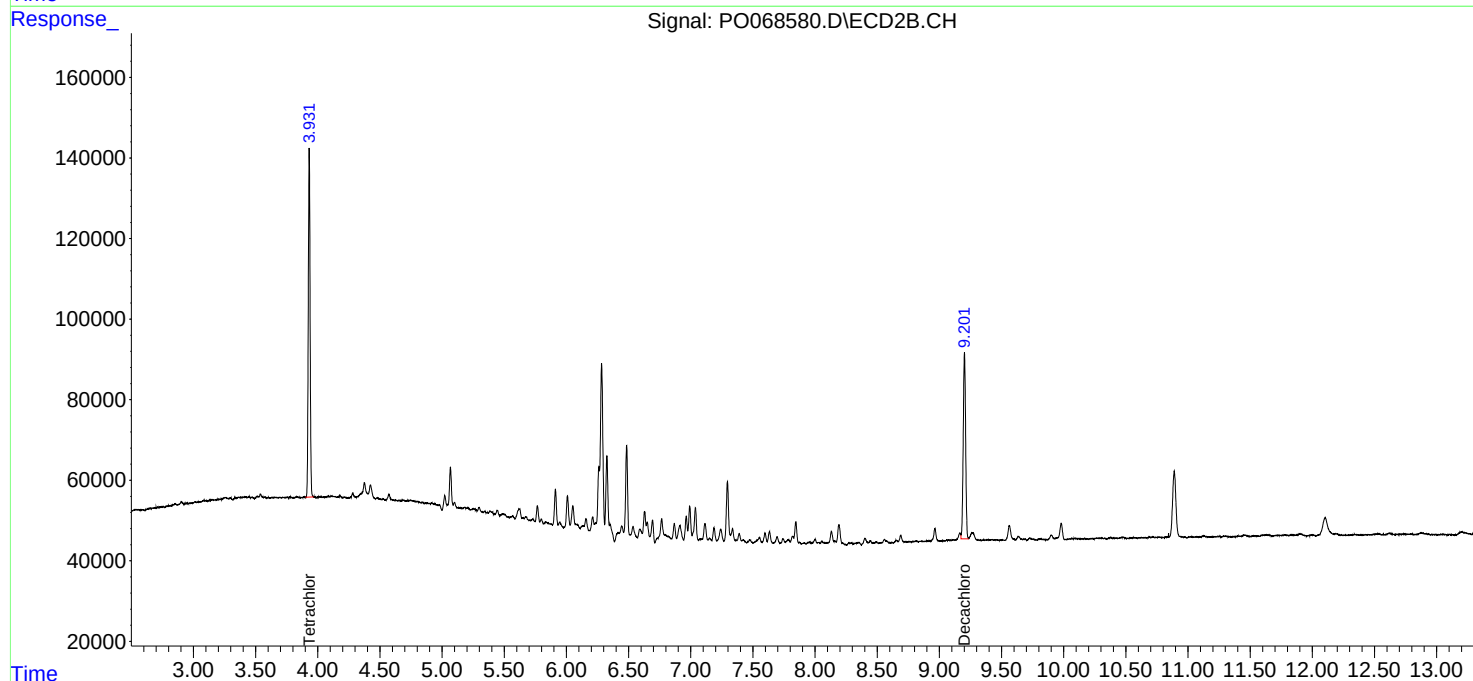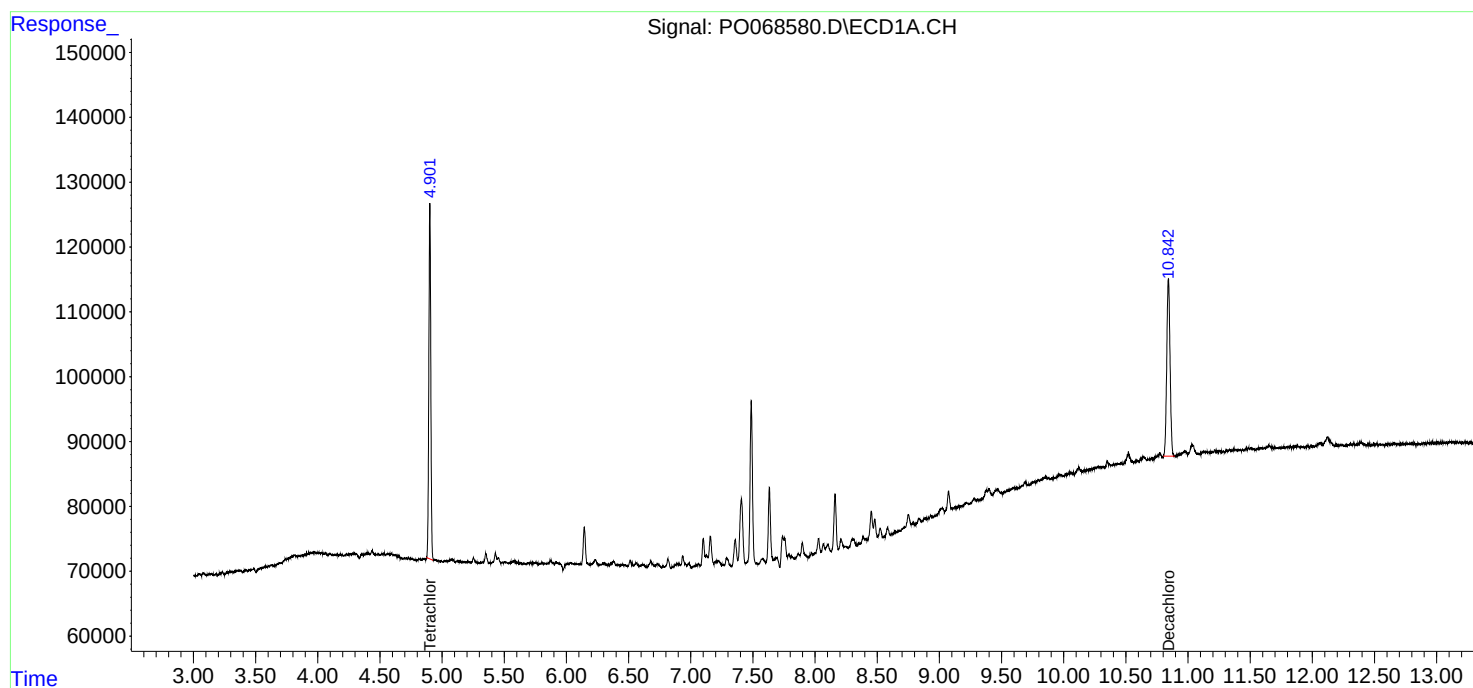

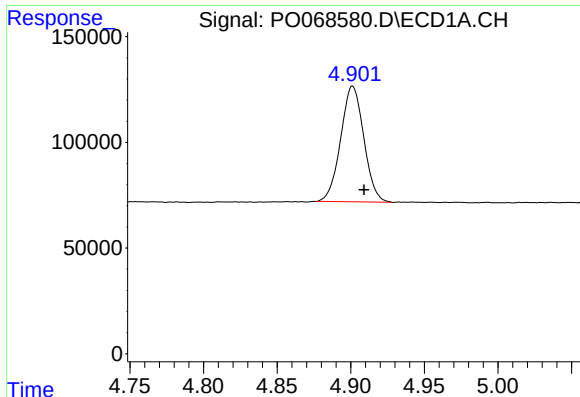


#1 Tetrachloro-m-xylene

R.T.: 4.901 min
Delta R.T.: -0.008 min
Response: 598173
Conc: 21.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NM76-COMP-2020-0-6


Manual Integrations
APPROVED

Sohil
5/28/2020 4:09:02 PM

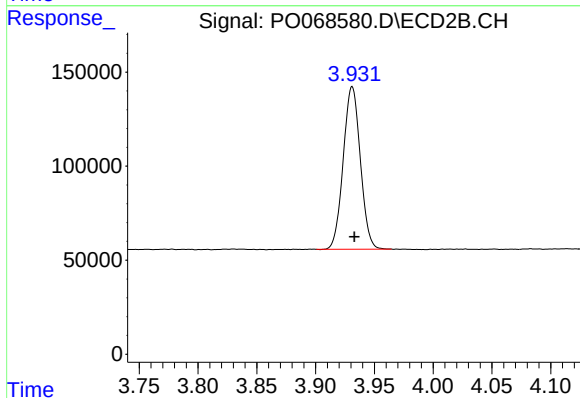


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 875279
Conc: 25.51 ng/ml

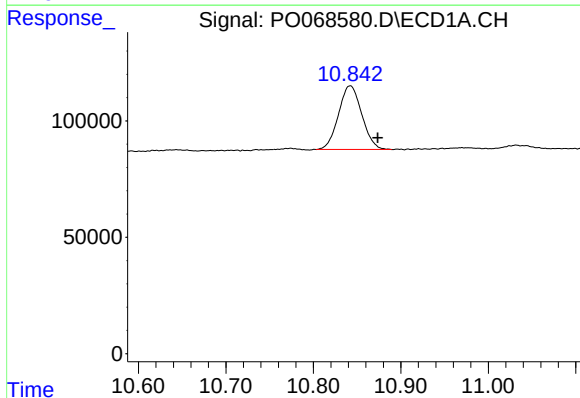

#2 Decachlorobiphenyl

R.T.: 10.842 min
Delta R.T.: -0.031 min
Response: 505281
Conc: 12.70 ng/ml m

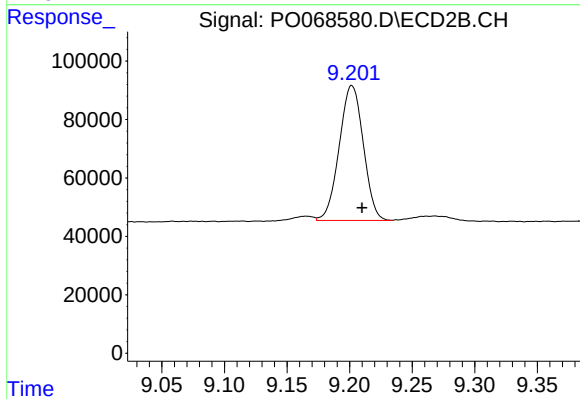

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.009 min
Response: 617902
Conc: 16.05 ng/ml m