

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052720\
 Data File : P0068595.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2020 12:47
 Operator : DD\AJ
 Sample : L2744-20RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NM50-COMP-2020-0-6RE

Manual Integrations
 APPROVED

Sohil
 5/28/2020 4:09:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 13:37:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.928	434217	652249	15.482m	19.008
2) SA Decachlor...	10.835	9.198	338427	428027	8.505m	11.118 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052720\
Data File : P0068595.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2020 12:47
Operator : DD\AJ
Sample : L2744-20RE
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NM50-COMP-2020-0-6RE


Manual Integrations
APPROVED

Sohil
5/28/2020 4:09:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 13:37:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

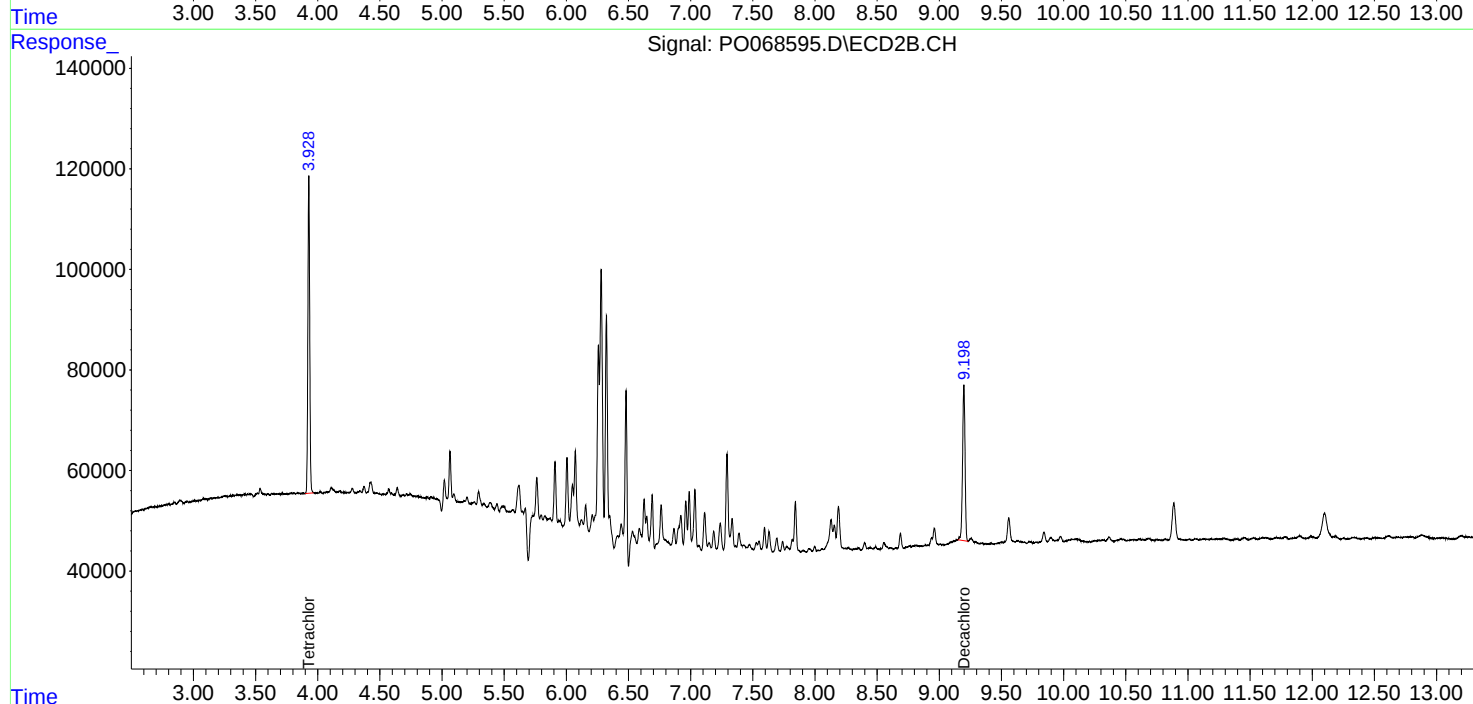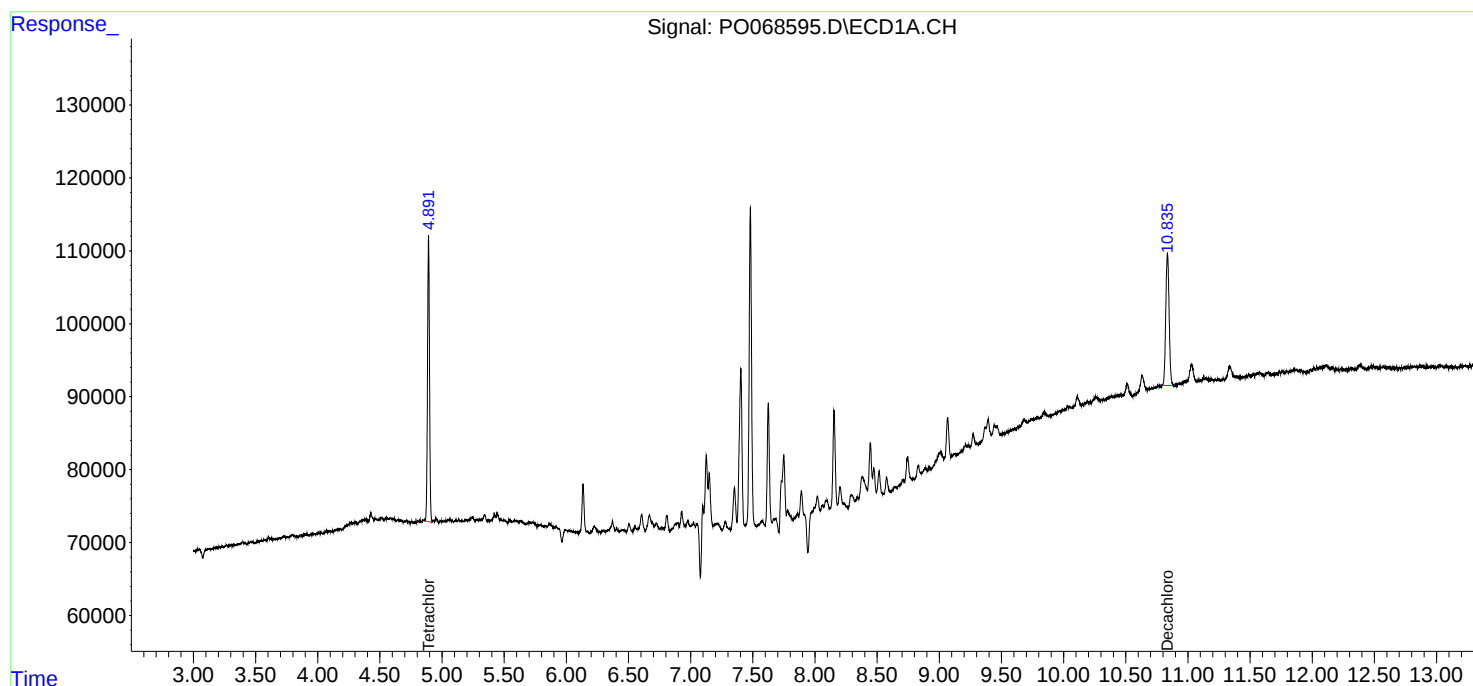

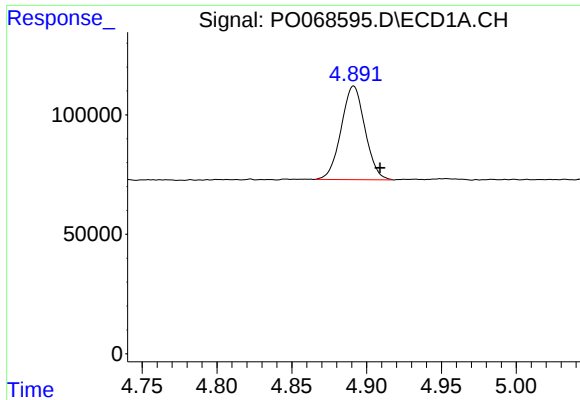


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.018 min
Response: 434217
Conc: 15.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NM50-COMP-2020-0-6RE


Manual Integrations
APPROVED

Sohil
5/28/2020 4:09:14 PM

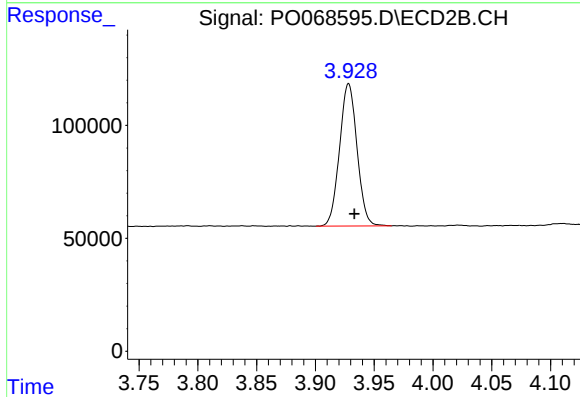


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.005 min
Response: 652249
Conc: 19.01 ng/ml

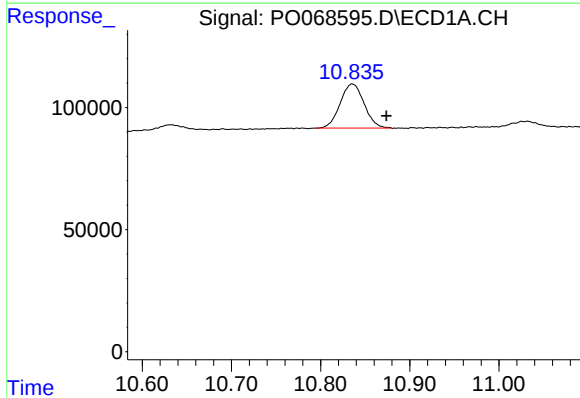

#2 Decachlorobiphenyl

R.T.: 10.835 min
Delta R.T.: -0.039 min
Response: 338427
Conc: 8.50 ng/ml m

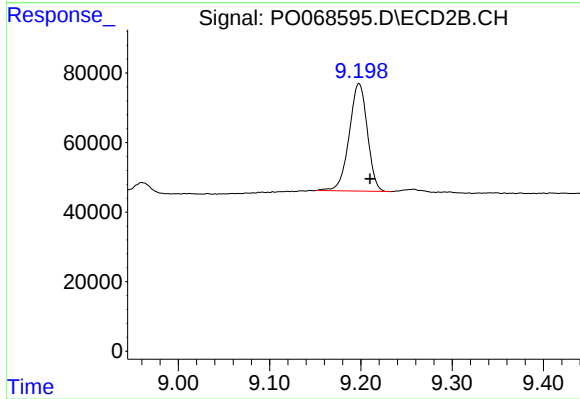

#2 Decachlorobiphenyl

R.T.: 9.198 min
Delta R.T.: -0.012 min
Response: 428027
Conc: 11.12 ng/ml