

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052819\
 Data File : P0056634.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 May 2019 11:08
 Operator : SM/SJ
 Sample : K2643-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-052319-A

Manual Integrations
 APPROVED

Ankita
 5/29/2019 2:12:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 11:29:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.255	3.572	989868	777201	25.856m	23.567m
2)	SA Decachlor...	9.835	8.510	683958	487597	13.934	13.675m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052819\
Data File : PO056634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 May 2019 11:08
Operator : SM/SJ
Sample : K2643-09
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-052319-A


Manual Integrations
APPROVED

Ankita
5/29/2019 2:12:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 11:29:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

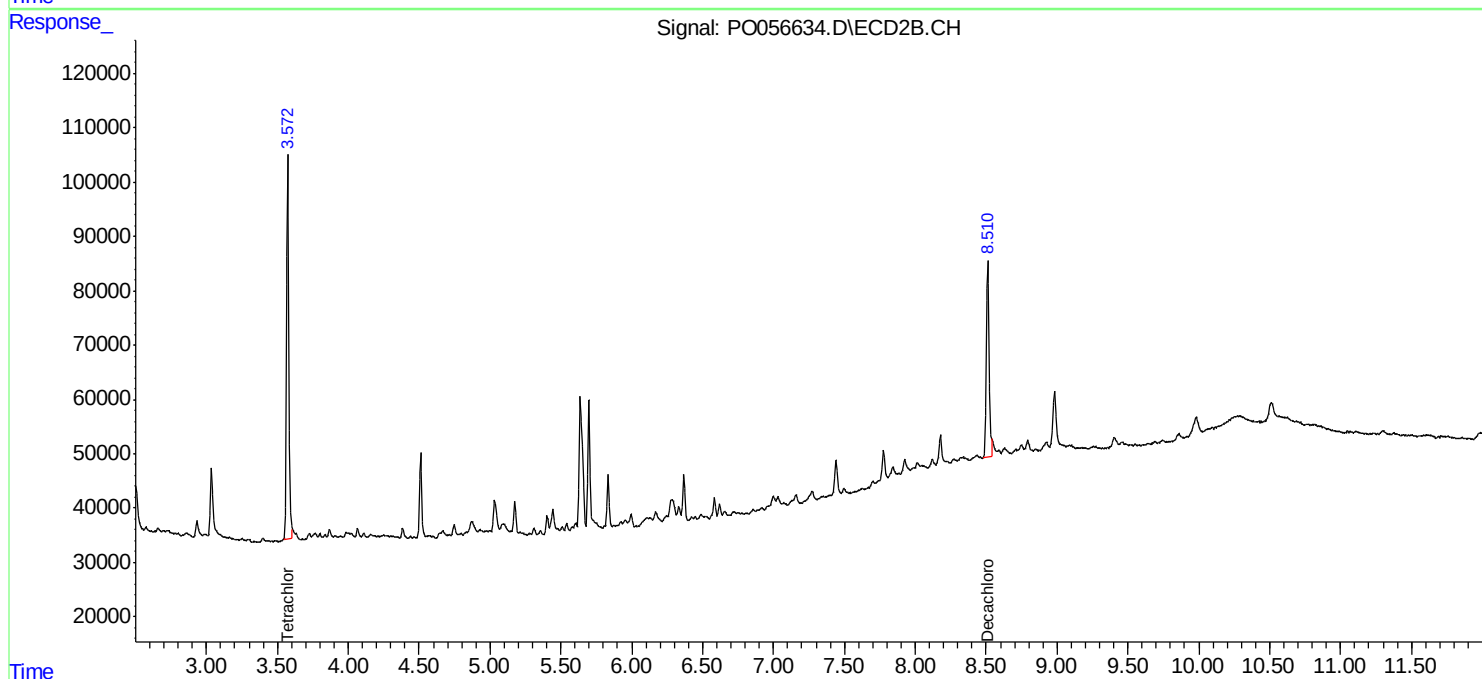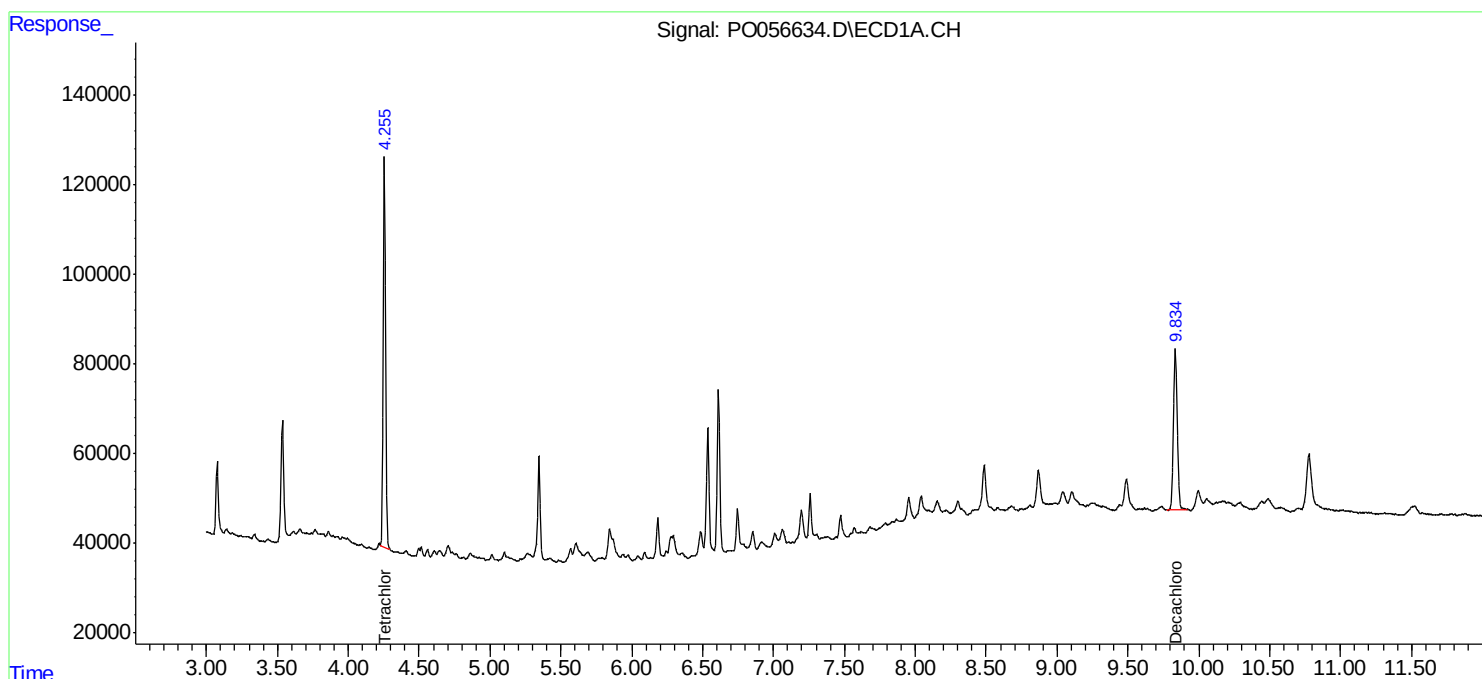

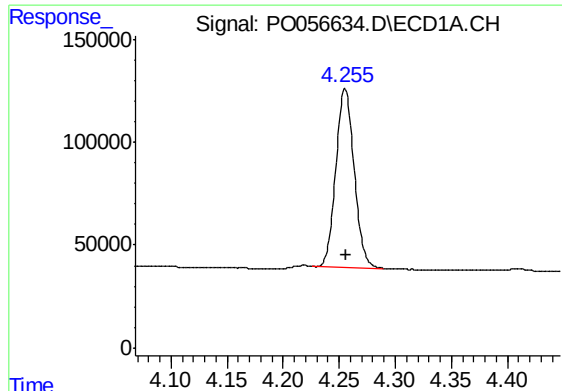


#1 Tetrachloro-m-xylene

R.T.: 4.255 min
Delta R.T.: -0.001 min
Response: 989868
Conc: 25.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-03-052319-A


Manual Integrations
APPROVED

Ankita
5/29/2019 2:12:44 PM

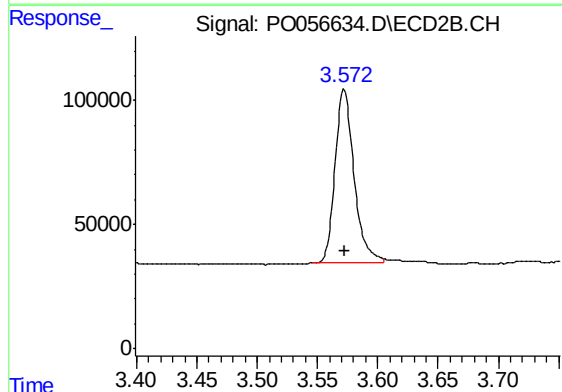


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: -0.001 min
Response: 777201
Conc: 23.57 ng/ml m

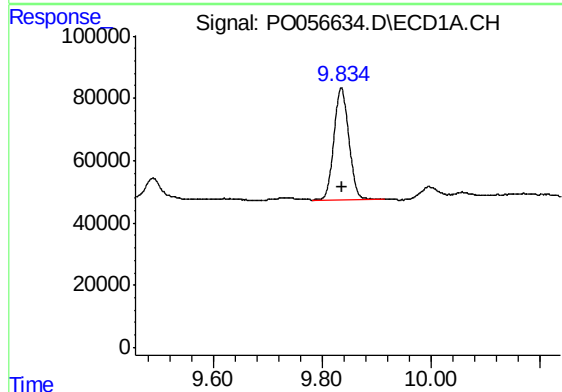

#2 Decachlorobiphenyl

R.T.: 9.835 min
Delta R.T.: -0.001 min
Response: 683958
Conc: 13.93 ng/ml

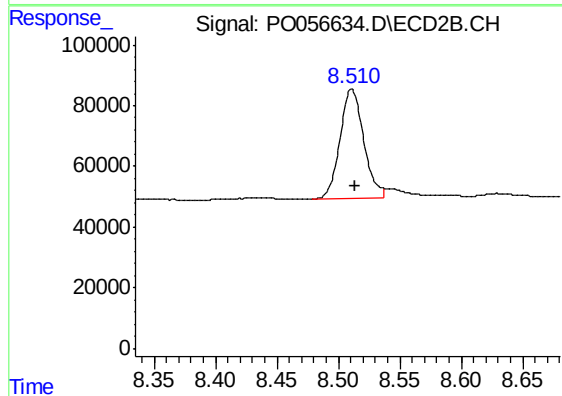

#2 Decachlorobiphenyl

R.T.: 8.510 min
Delta R.T.: -0.003 min
Response: 487597
Conc: 13.67 ng/ml m