

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052820\
 Data File : P0068669.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2020 1:42
 Operator : DD\AJ
 Sample : L2776-02MSD
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 351MSD

Manual Integrations
 APPROVED

Sohil
 5/29/2020 12:32:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:41:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 29 02:25:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.929	409105	704375	13.197m	19.067m#
2) SA Decachlor...	10.838	9.200	432703	514933	10.034	12.127

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052820\
Data File : P0068669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2020 1:42
Operator : DD\AJ
Sample : L2776-02MSD
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
351MSD


Manual Integrations
APPROVED

Sohil
5/29/2020 12:32:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:41:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 29 02:25:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

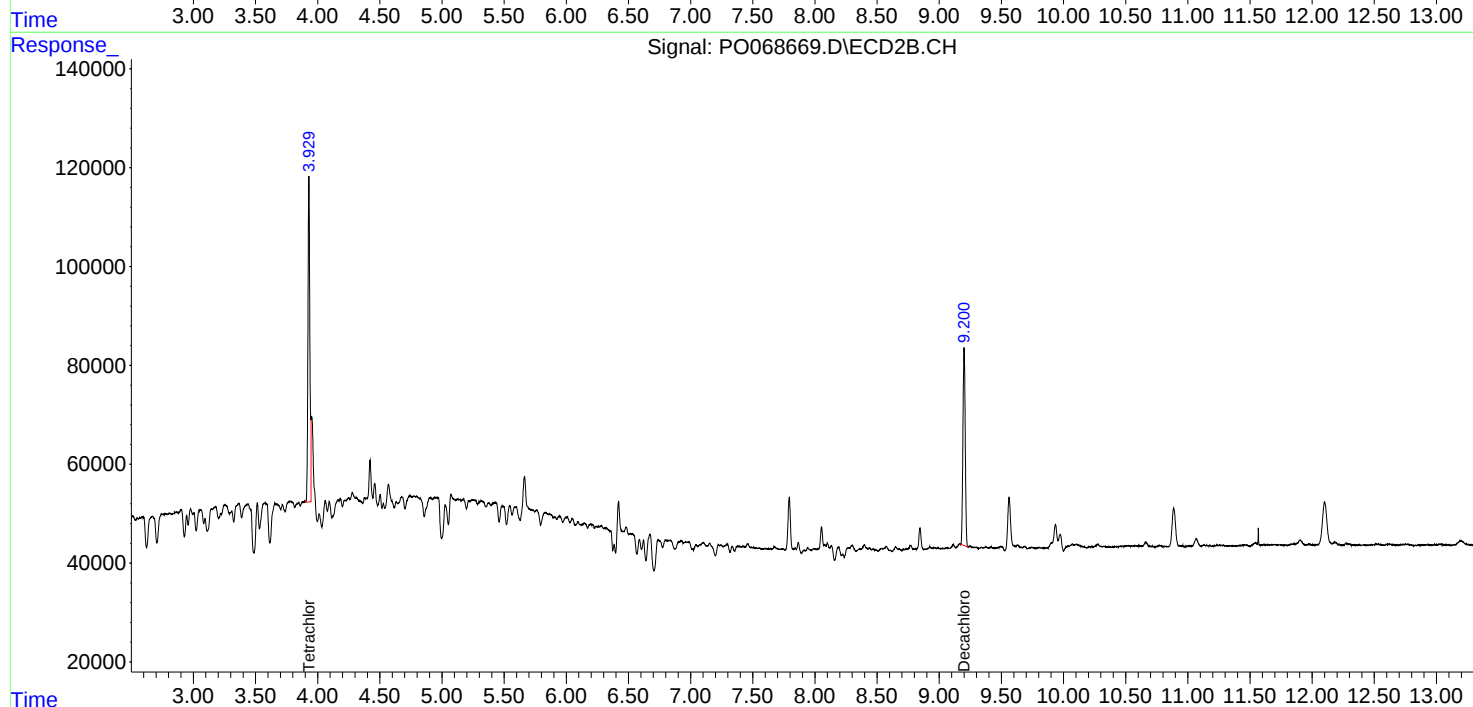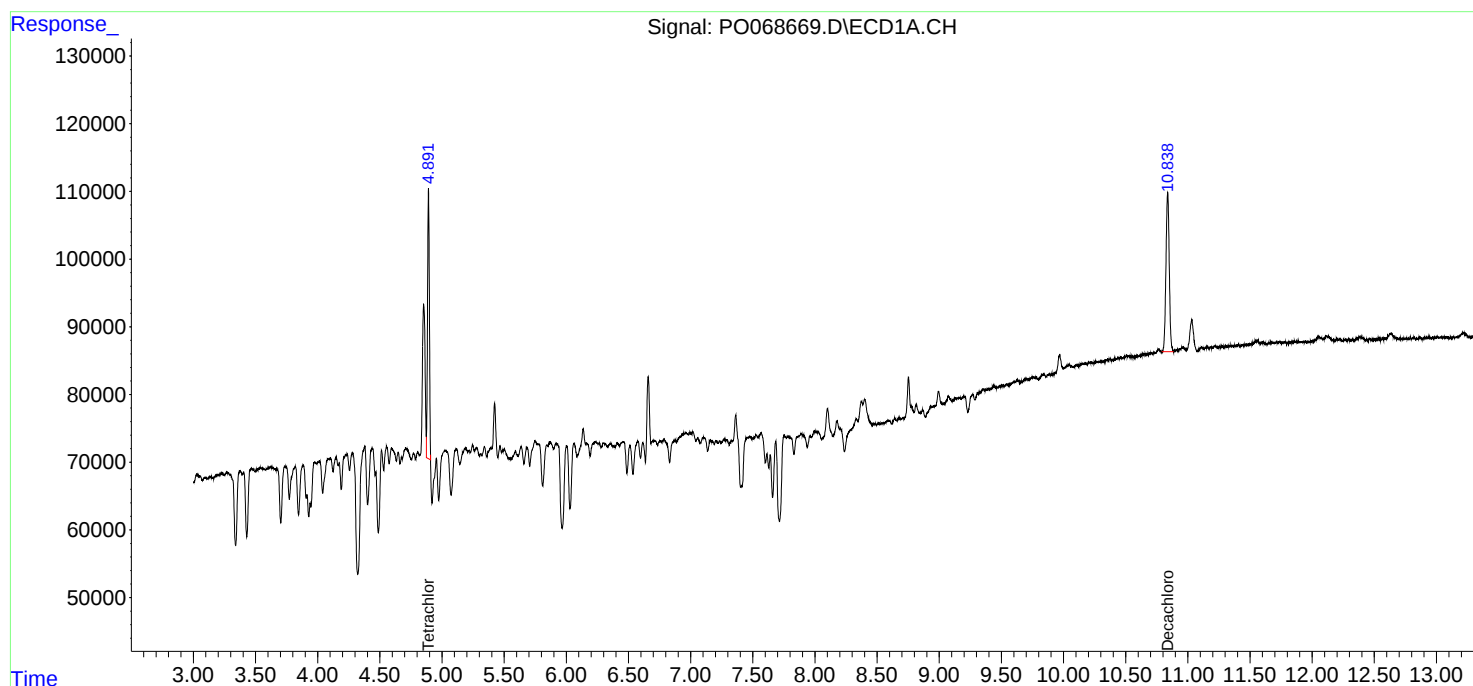

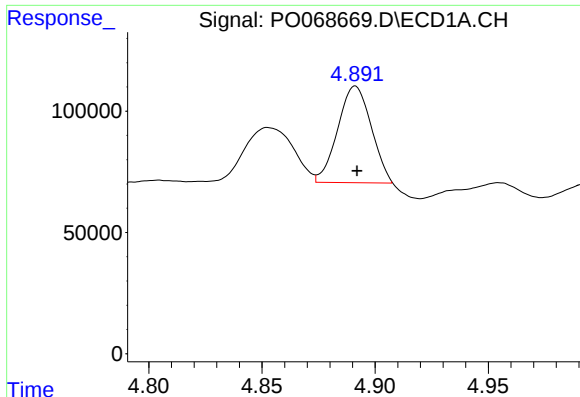


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.001 min
Response: 409105
Conc: 13.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
351MSD


Manual Integrations
APPROVED

Sohil
5/29/2020 12:32:16 PM

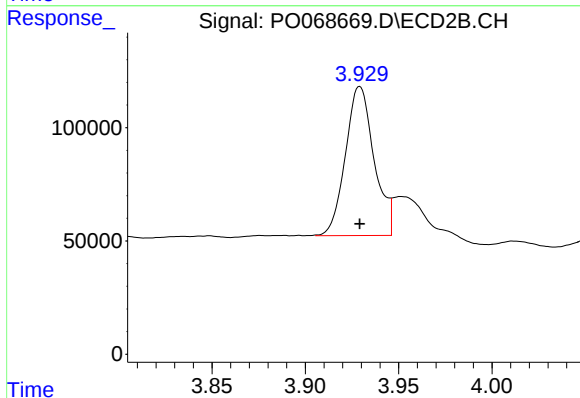


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: 0.000 min
Response: 704375
Conc: 19.07 ng/ml m

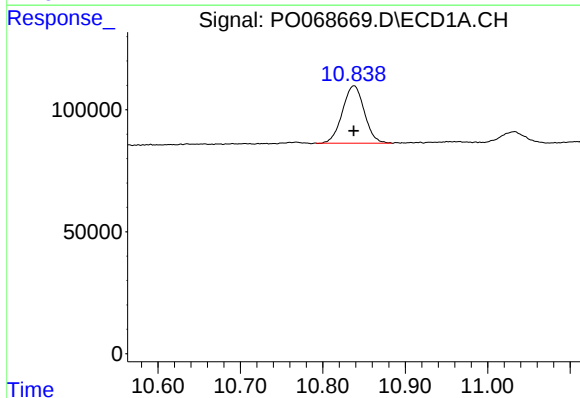

#2 Decachlorobiphenyl

R.T.: 10.838 min
Delta R.T.: 0.000 min
Response: 432703
Conc: 10.03 ng/ml

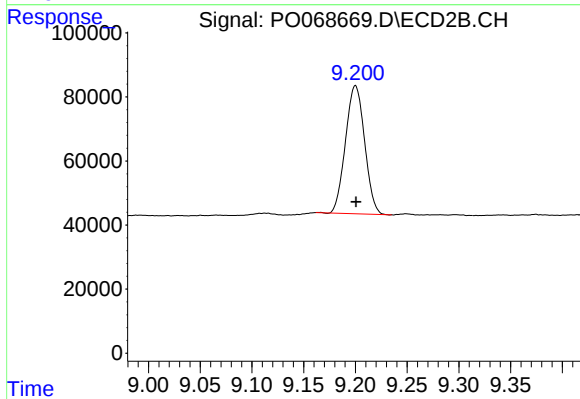

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: 0.000 min
Response: 514933
Conc: 12.13 ng/ml