

Data Path : P:\HPCHEM1\ECD_0\Data\P0052918\
 Data File : P0045182.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2018 16:33
 Operator : SM/UA
 Sample : J3094-04RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HS-BASELINE-WATERRE

Manual Integrations
 APPROVED

Sohil
 5/30/2018 7:47:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 17:12:45 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0052518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 26 01:36:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.001	3.271	5087064	5027336	8.747	7.852m
2) SA Decachlor...	9.291	8.001	3311710	3671855	6.291m	6.405m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0052918\
Data File : P0045182.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2018 16:33
Operator : SM/UA
Sample : J3094-04RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HS-BASELINE-WATERRE


Manual Integrations
APPROVED

Sohil
5/30/2018 7:47:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 17:12:45 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0052518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 26 01:36:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

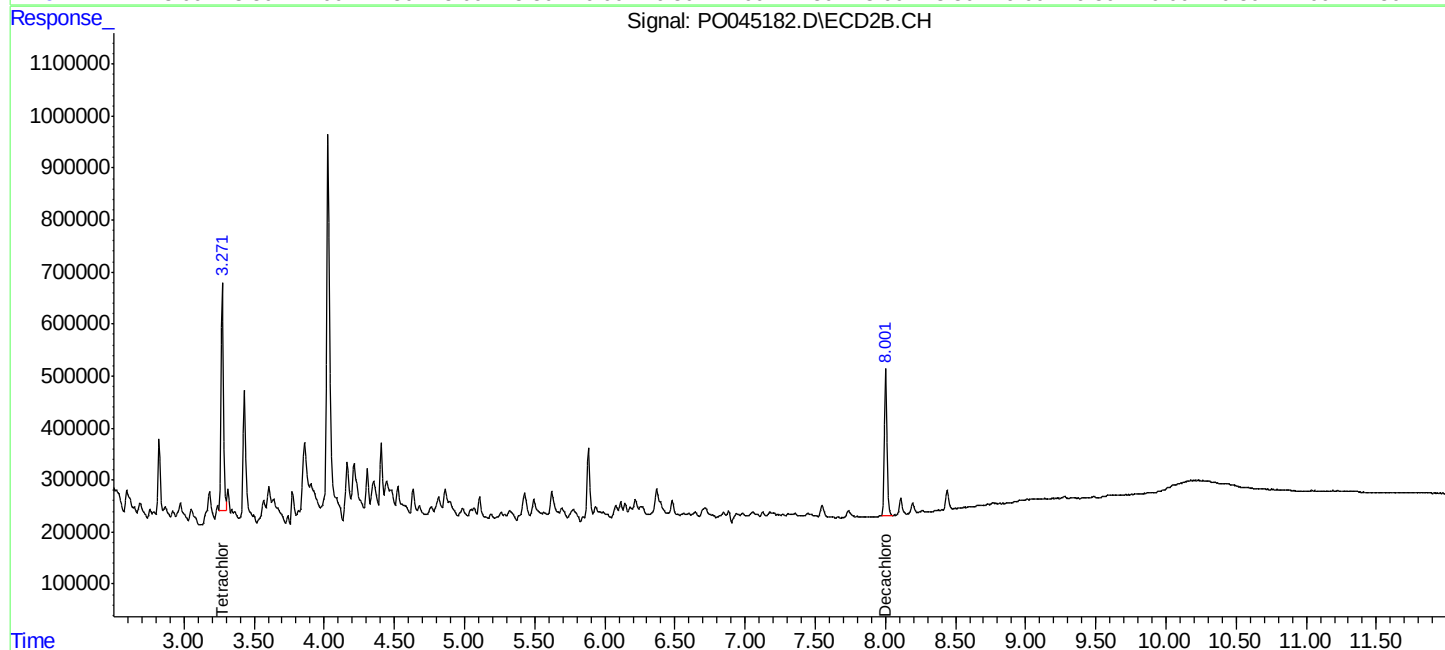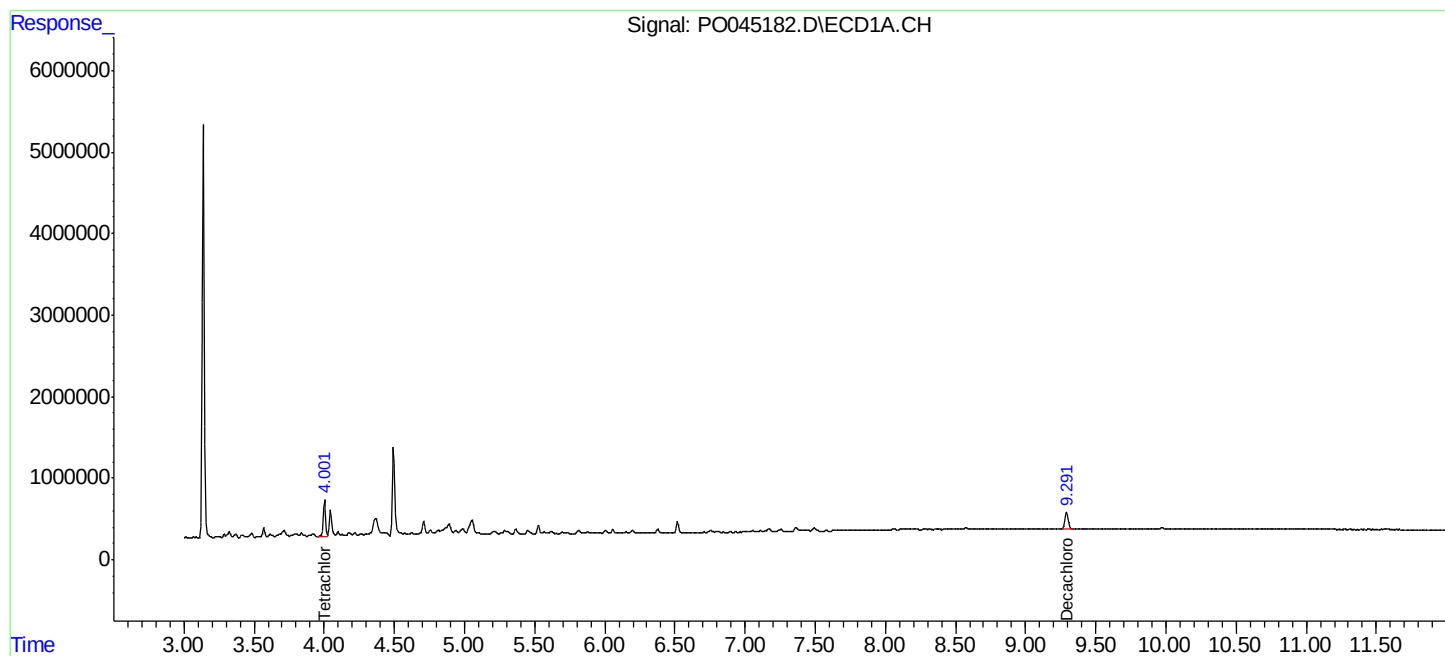

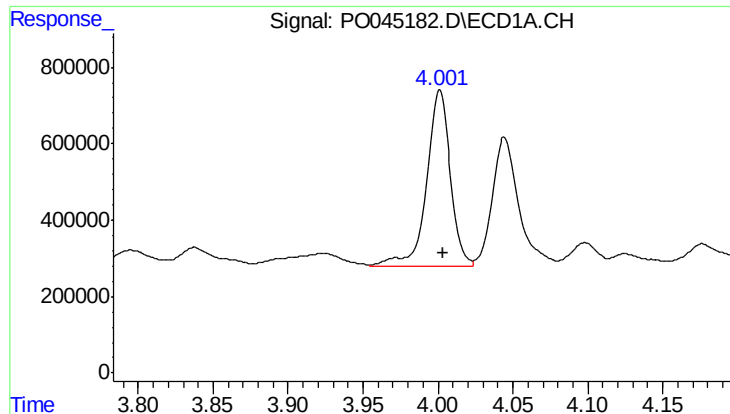


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.002 min
Response: 5087064
Conc: 8.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
HS-BASELINE-WATERRE


Manual Integrations
APPROVED

Sohil
5/30/2018 7:47:14 AM

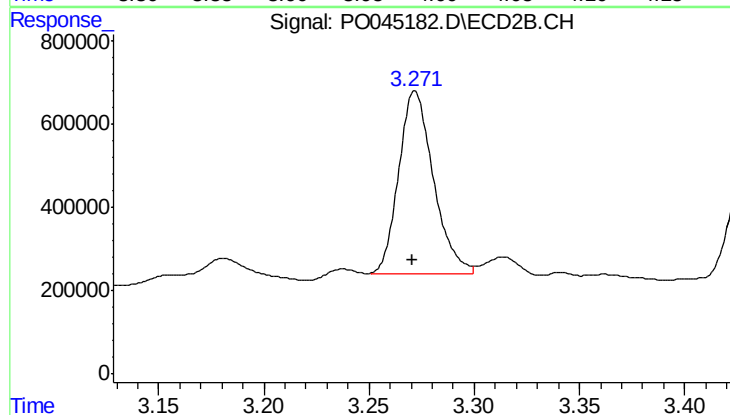


#1 Tetrachloro-m-xylene

R.T.: 3.271 min
Delta R.T.: 0.000 min
Response: 5027336
Conc: 7.85 ng/ml m

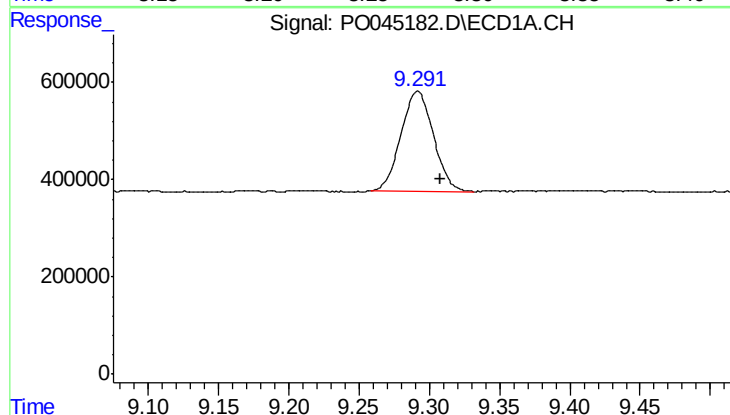

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.016 min
Response: 3311710
Conc: 6.29 ng/ml m

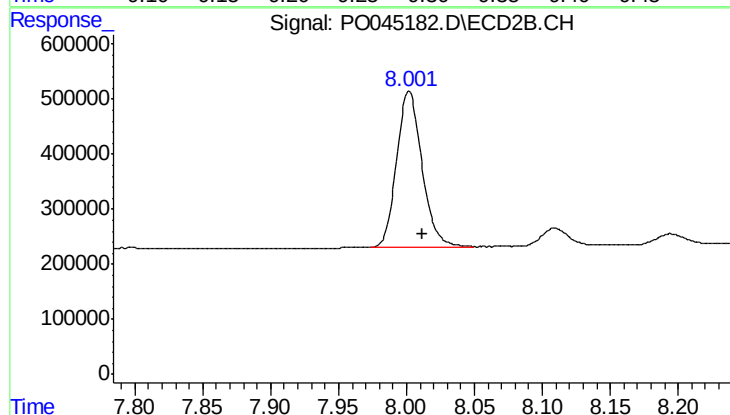

#2 Decachlorobiphenyl

R.T.: 8.001 min
Delta R.T.: -0.011 min
Response: 3671855
Conc: 6.40 ng/ml m