

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
 Data File : P0056708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2019 23:08
 Operator : SM/SJ
 Sample : K3075-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:20:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.250	3.568	735898	584721	19.222	17.730
2)	SA Decachlor...	9.826	8.504	697021	453329	14.201	12.714
Target Compounds							
10)	L2 AR-1221-3	0.000	3.982	0	21484	N.D.	17.948 #
11)	L3 AR-1232-1	0.000	3.982	0	21484	N.D.	23.915 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
Data File : P0056708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 23:08
Operator : SM/SJ
Sample : K3075-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:20:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

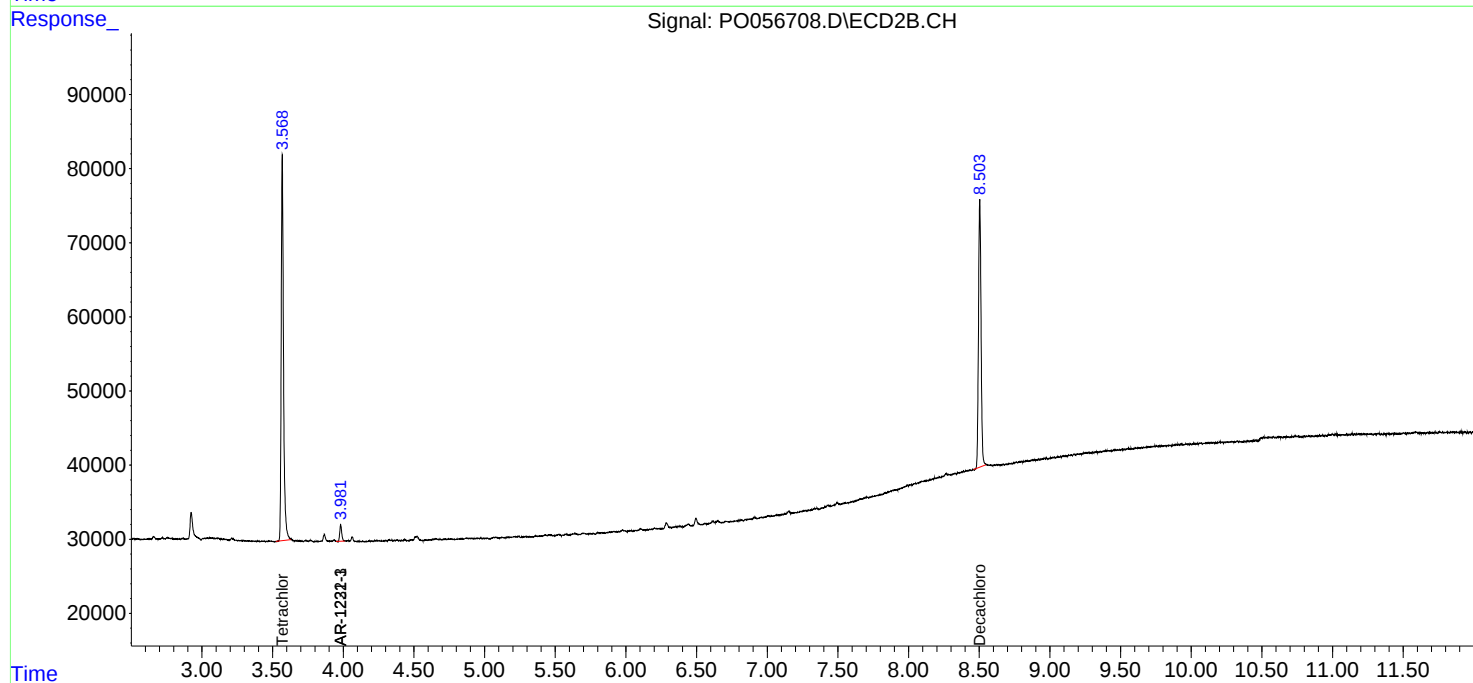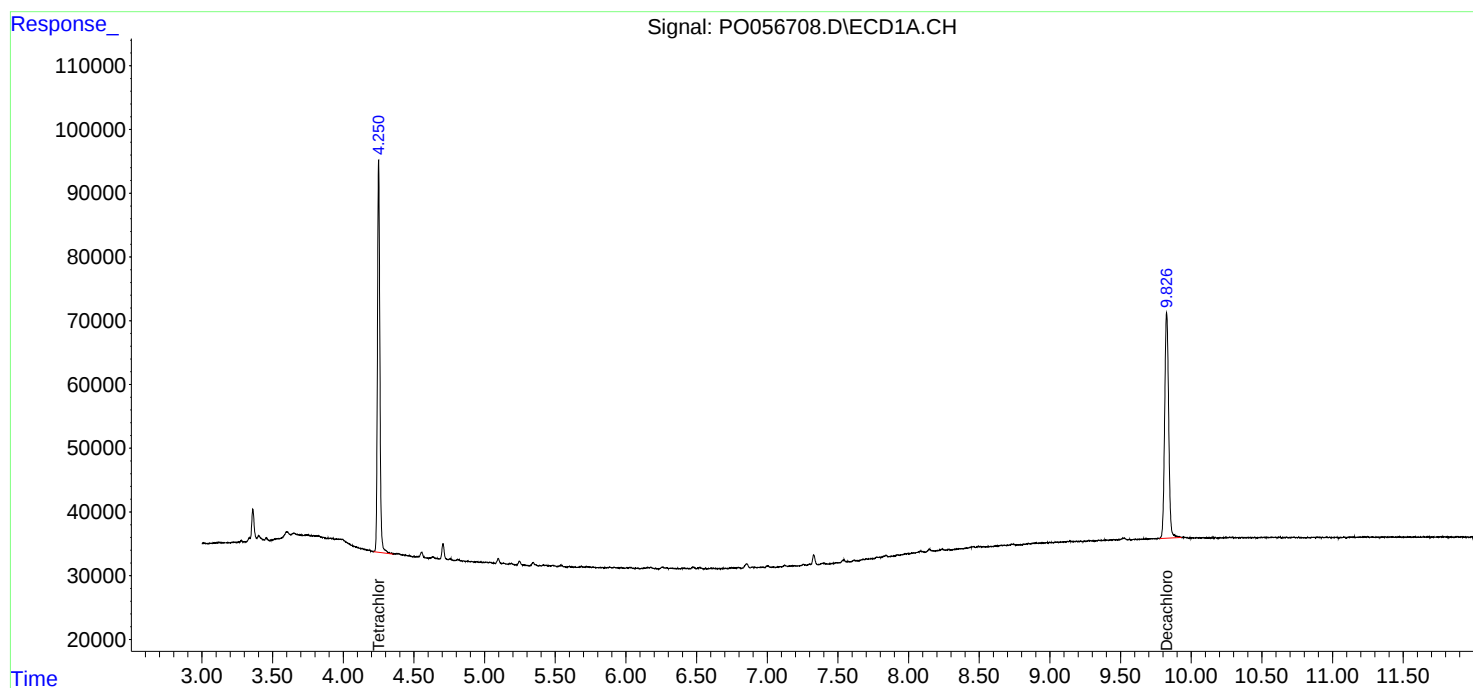


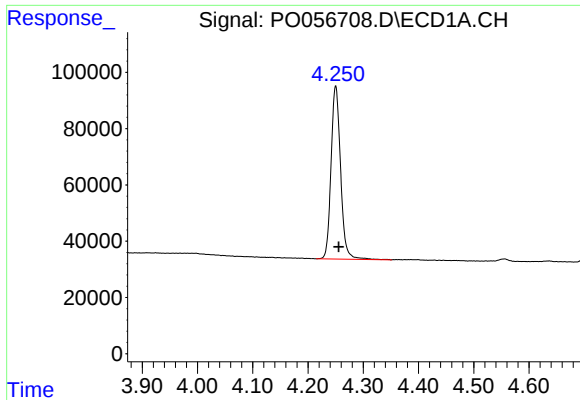

#1 Tetrachloro-m-xylene


R.T.: 4.250 min
Delta R.T.: -0.006 min
Response: 735898
Conc: 19.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

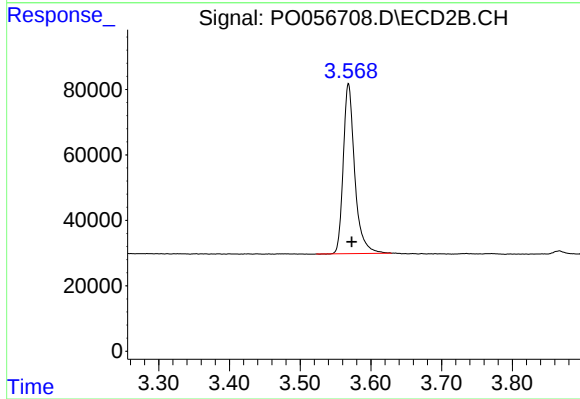


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.005 min
Response: 584721
Conc: 17.73 ng/ml

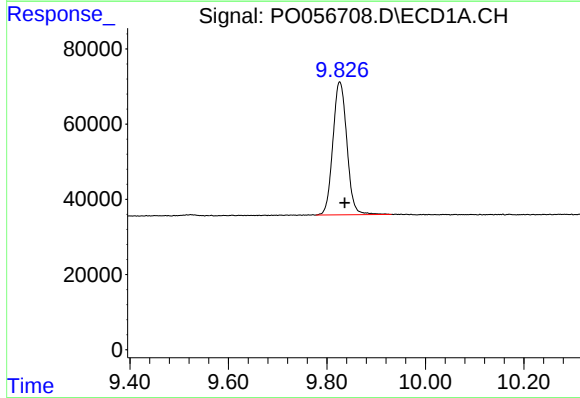


#2 Decachlorobiphenyl

R.T.: 9.826 min
Delta R.T.: -0.010 min
Response: 697021
Conc: 14.20 ng/ml

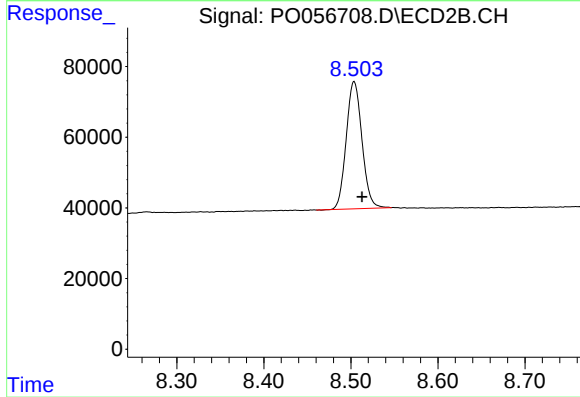

#2 Decachlorobiphenyl


R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 453329
Conc: 12.71 ng/ml

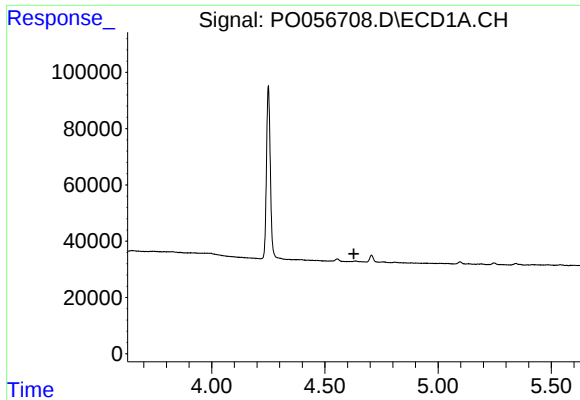

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

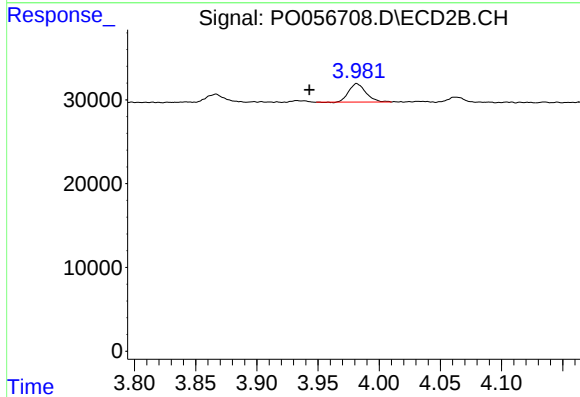


#10 AR-1221-3

R.T.: 3.982 min
Delta R.T.: 0.038 min
Response: 21484
Conc: 17.95 ng/ml

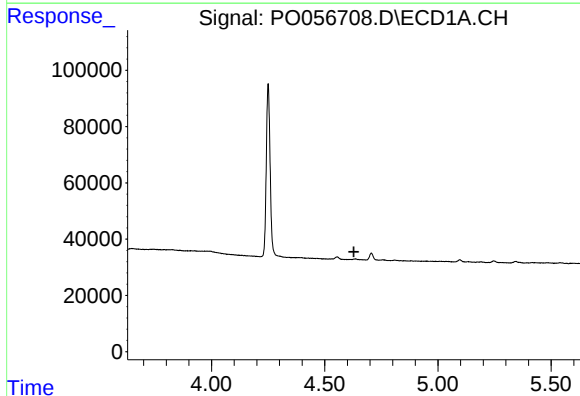

#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

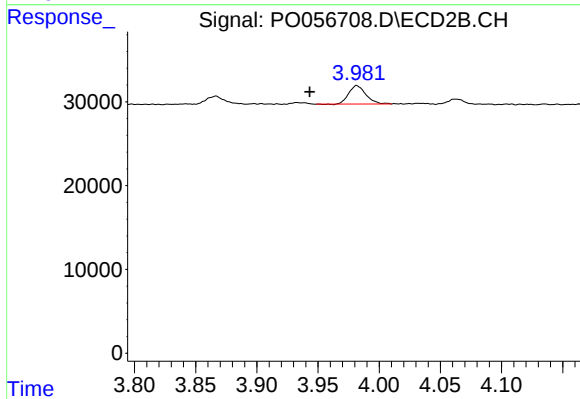

#11 AR-1232-1

R.T.: 3.982 min
Delta R.T.: 0.038 min
Response: 21484
Conc: 23.91 ng/ml