

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
 Data File : P0056666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2019 9:08 (#1); 29 May 2019 9:07 (#2)
 Operator : SM/SJ
 Sample : K3026-15RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3-SRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 10:03:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.570	697409	576613	18.217	17.485
2) SA Decachlor...	9.839	8.509	500293	357199	10.193	10.018

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
Data File : P0056666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 9:08 (#1); 29 May 2019 9:07 (#2)
Operator : SM/SJ
Sample : K3026-15RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3-SRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 10:03:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

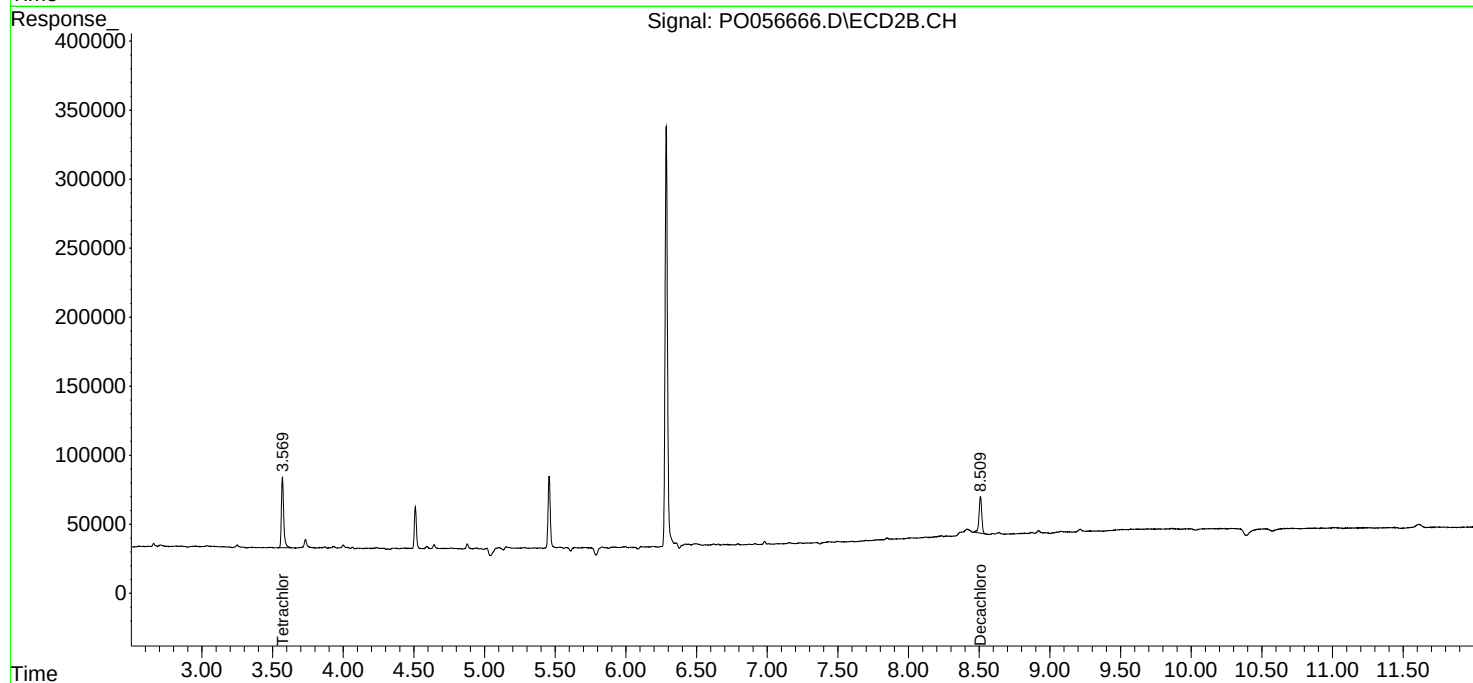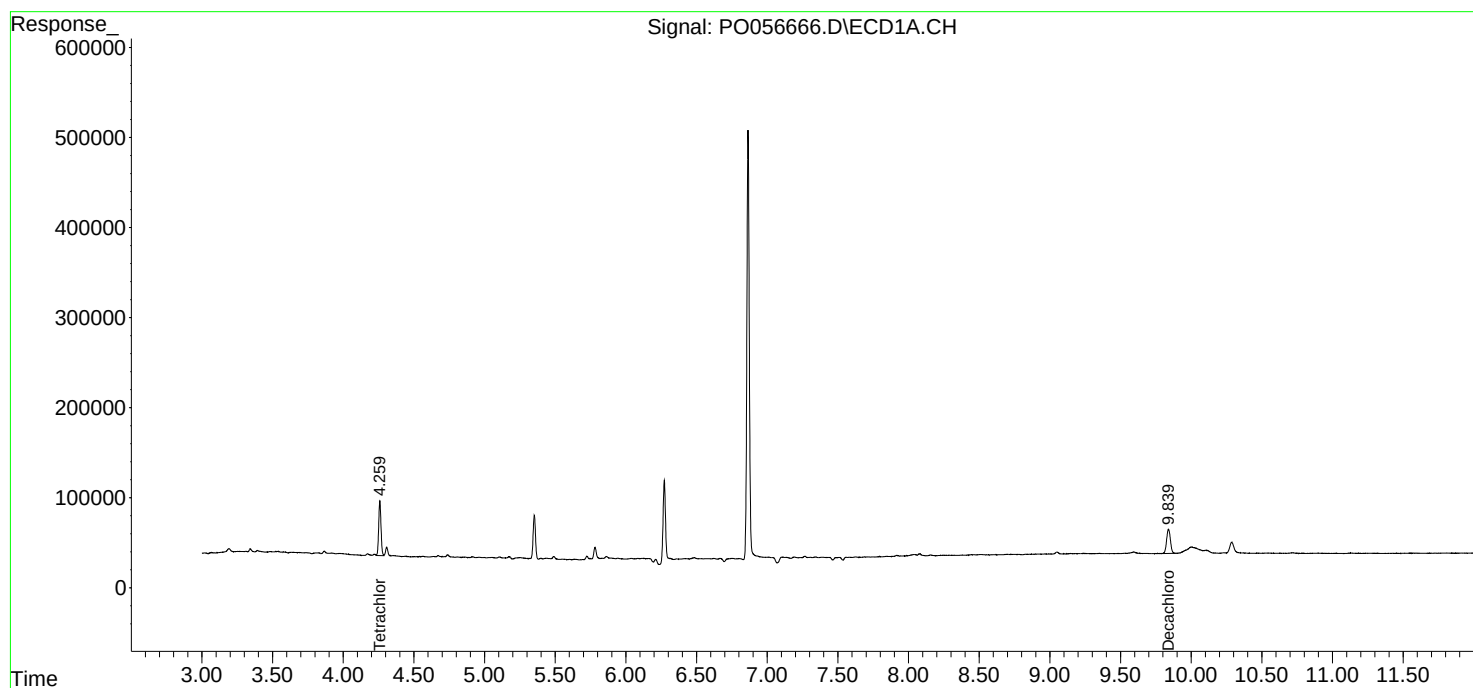


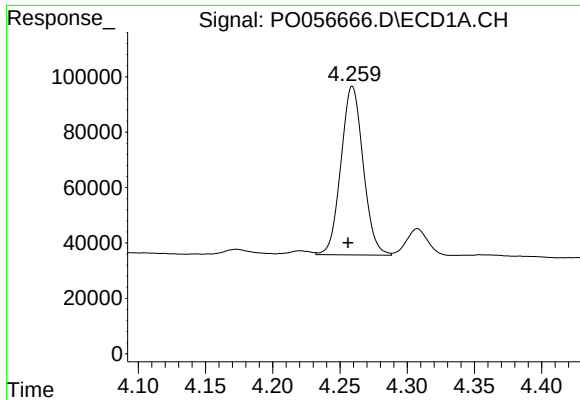

#1 Tetrachloro-m-xylene


R.T.: 4.259 min
Delta R.T.: 0.003 min
Response: 697409
Conc: 18.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-SRE

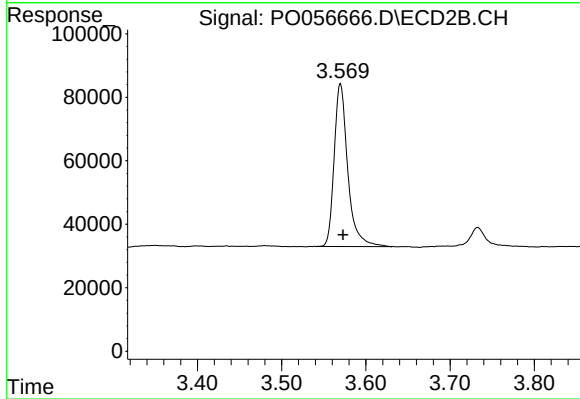


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: -0.003 min
Response: 576613
Conc: 17.48 ng/ml

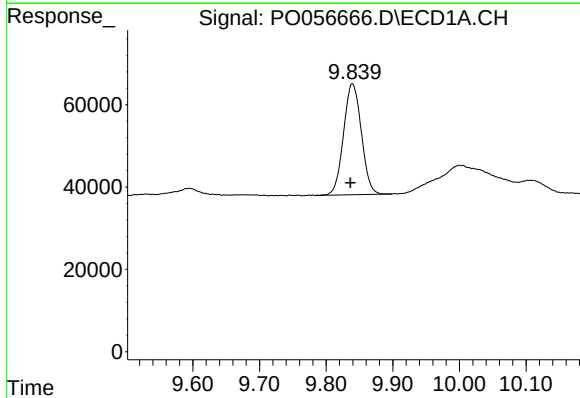

#2 Decachlorobiphenyl

R.T.: 9.839 min
Delta R.T.: 0.003 min
Response: 500293
Conc: 10.19 ng/ml

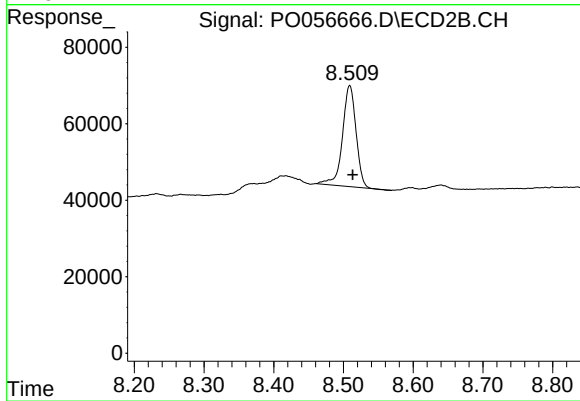

#2 Decachlorobiphenyl

R.T.: 8.509 min
Delta R.T.: -0.004 min
Response: 357199
Conc: 10.02 ng/ml