

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
 Data File : P0056694.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2019 19:10
 Operator : SM/SJ
 Sample : K3072-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Ankita
 5/30/2019 9:31:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:16:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.251	3.568	830075	670641	21.682	20.336
2) SA Decachlor...	9.829	8.504	944272	635311	19.238	17.817m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052919\
Data File : PO056694.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 19:10
Operator : SM/SJ
Sample : K3072-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
5/30/2019 9:31:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:16:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

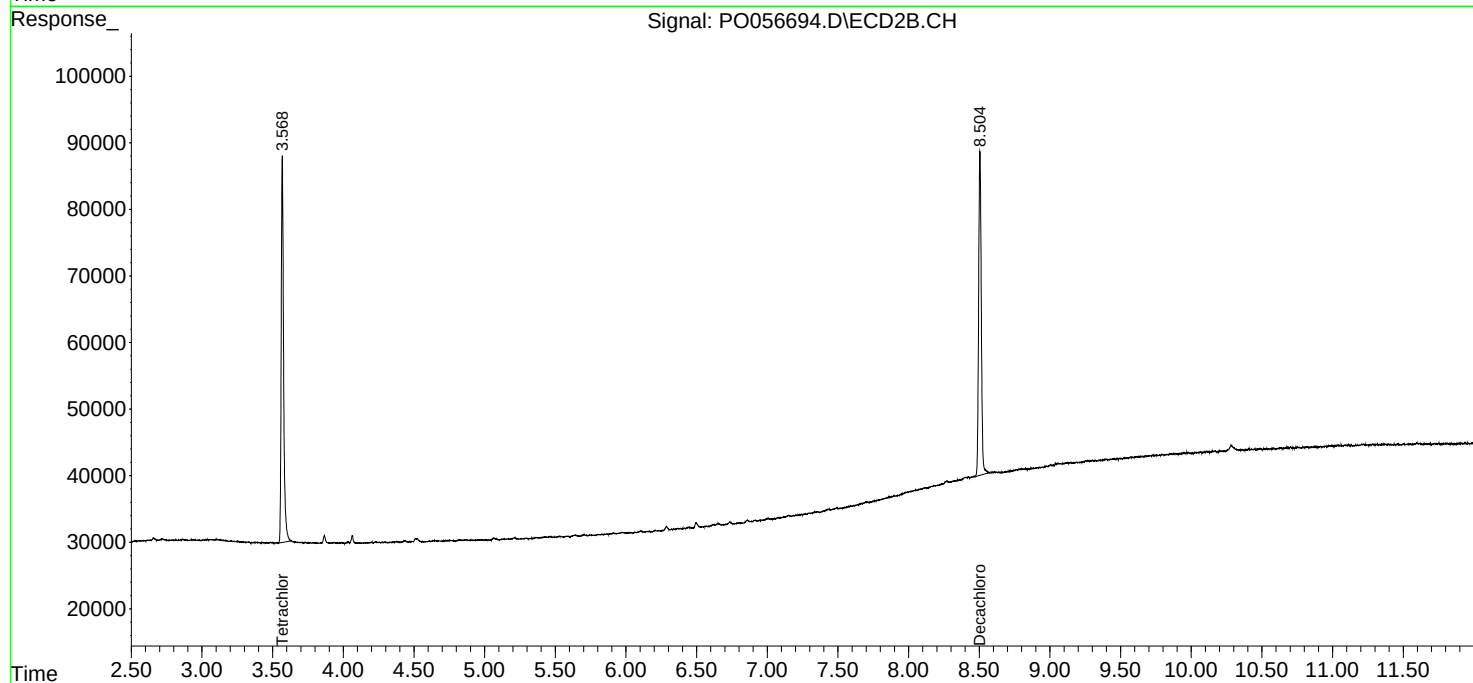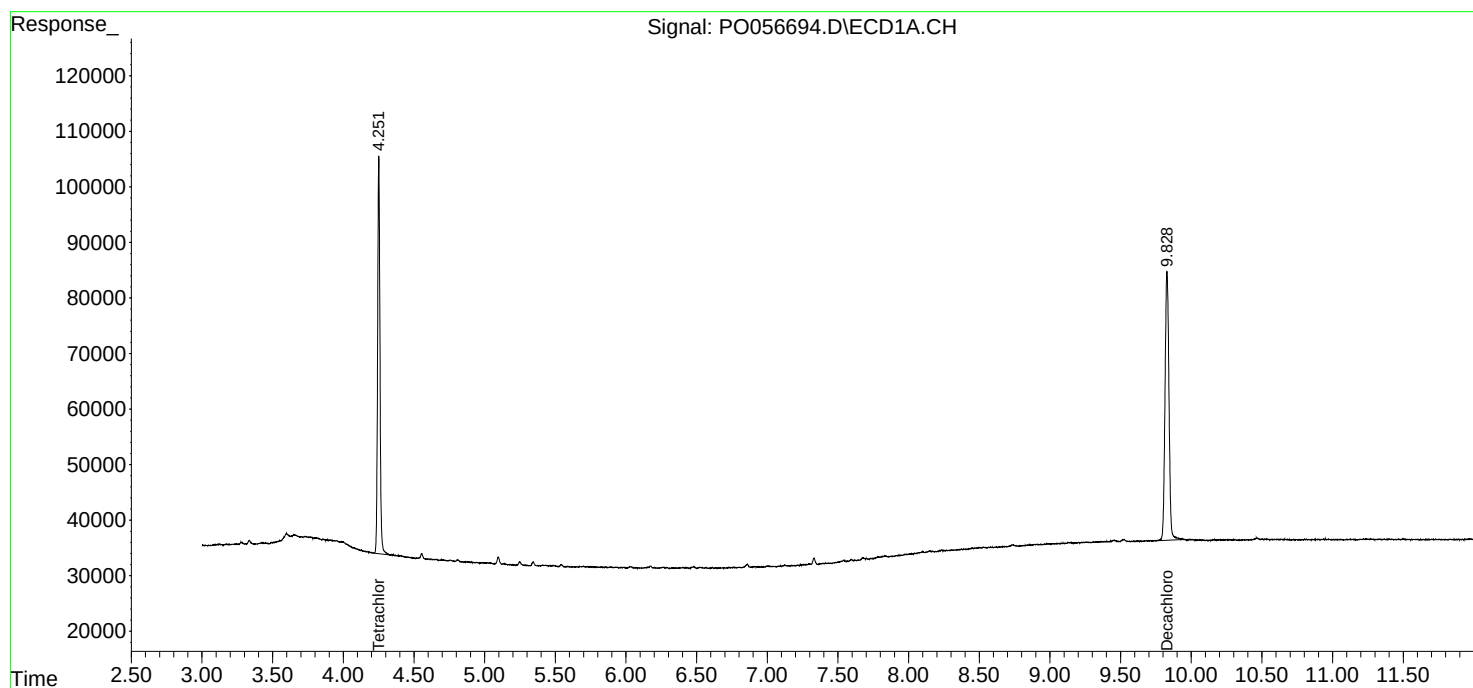

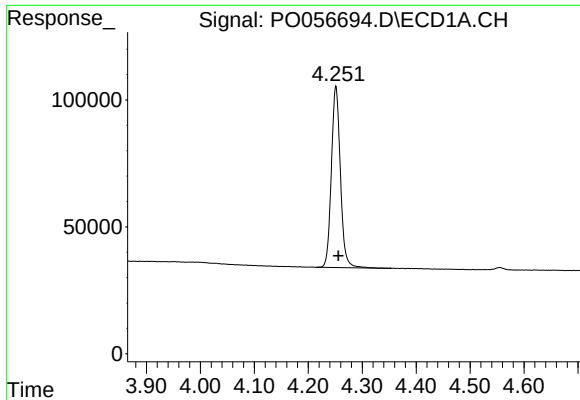


#1 Tetrachloro-m-xylene

R.T.: 4.251 min
Delta R.T.: -0.005 min
Response: 830075
Conc: 21.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
5/30/2019 9:31:50 AM

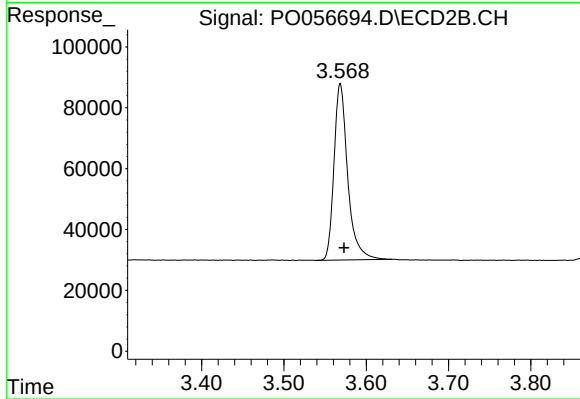


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.005 min
Response: 670641
Conc: 20.34 ng/ml

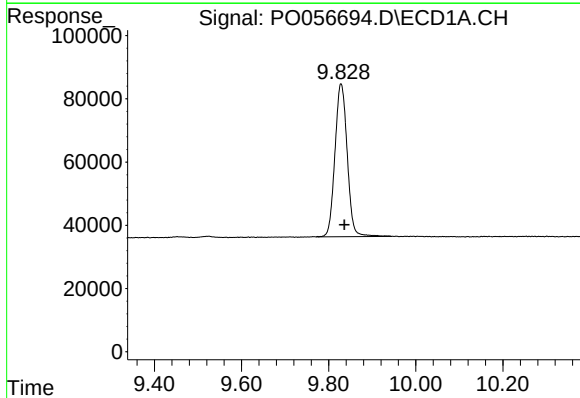

#2 Decachlorobiphenyl

R.T.: 9.829 min
Delta R.T.: -0.008 min
Response: 944272
Conc: 19.24 ng/ml

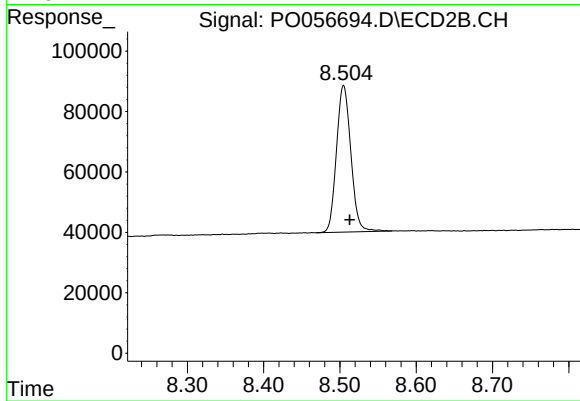

#2 Decachlorobiphenyl

R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 635311
Conc: 17.82 ng/ml m