

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
Data File : P0056695.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 19:27
Operator : SM/SJ
Sample : K3072-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Ankita
5/30/2019 9:31:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:17:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.252	3.569	789950	648415	20.634	19.662m
2) SA Decachlor...	9.831	8.505	891509	593056	18.163	16.632

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052919\
Data File : P0056695.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 19:27
Operator : SM/SJ
Sample : K3072-05
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
5/30/2019 9:31:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:17:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

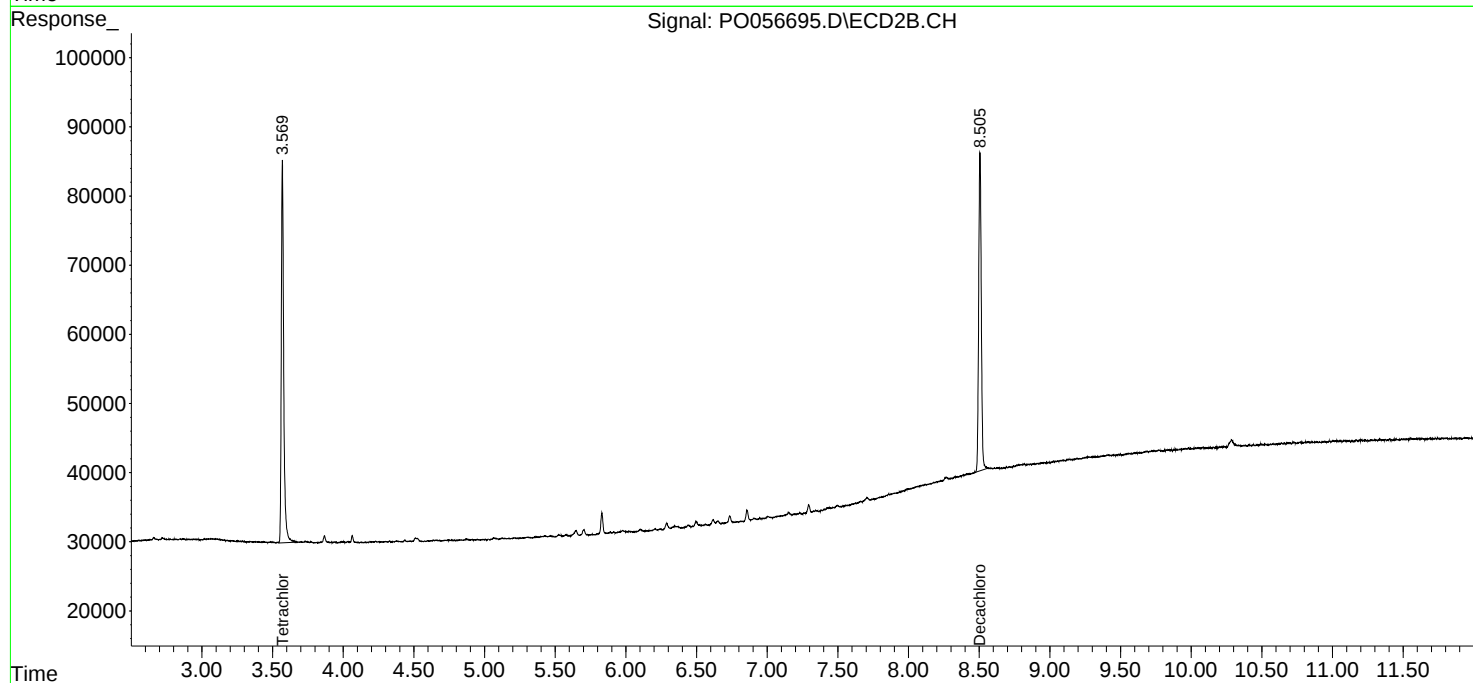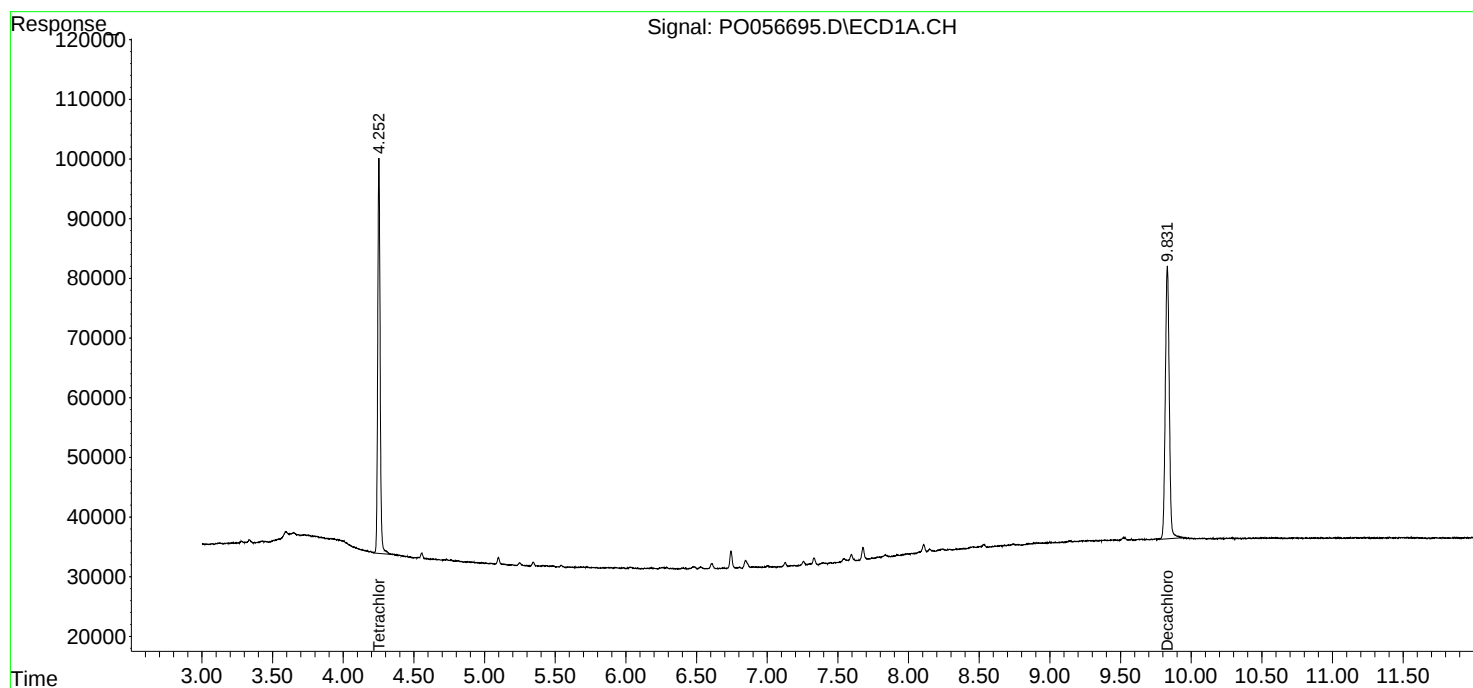

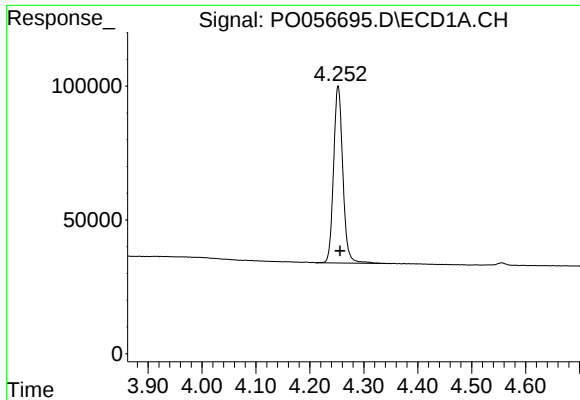


#1 Tetrachloro-m-xylene

R.T.: 4.252 min
Delta R.T.: -0.004 min
Response: 789950
Conc: 20.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
5/30/2019 9:31:52 AM

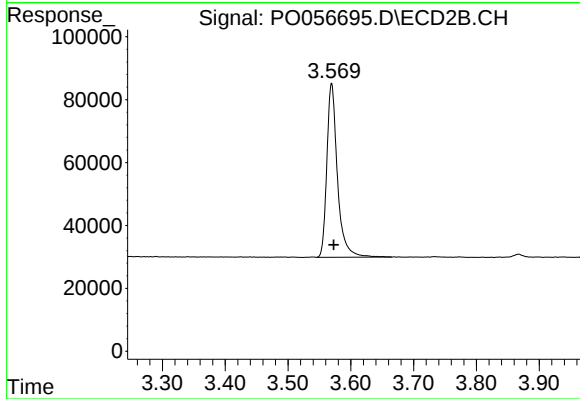


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.004 min
Response: 648415
Conc: 19.66 ng/ml m

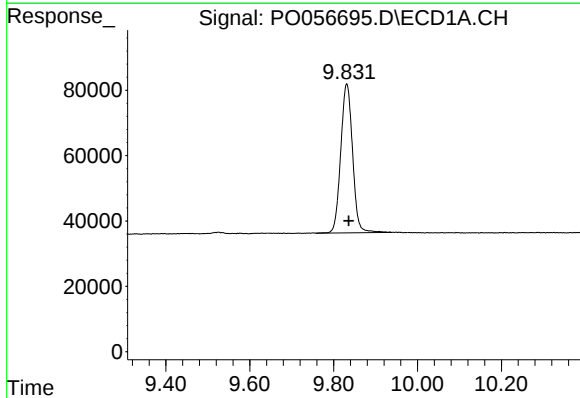

#2 Decachlorobiphenyl

R.T.: 9.831 min
Delta R.T.: -0.005 min
Response: 891509
Conc: 18.16 ng/ml

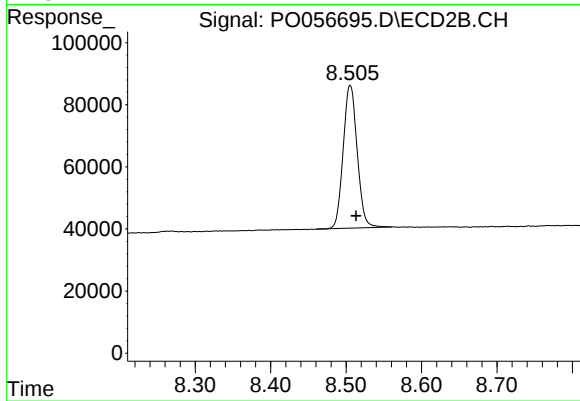

#2 Decachlorobiphenyl

R.T.: 8.505 min
Delta R.T.: -0.008 min
Response: 593056
Conc: 16.63 ng/ml