

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052920\
 Data File : P0068680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2020 9:43
 Operator : DD\AJ
 Sample : L2773-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NM4-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 10:37:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 29 02:25:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.927	603875	764671	19.344	20.679
2) SA Decachlor...	10.835	9.199	519643	625719	11.849	14.687

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052920\
Data File : P0068680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2020 9:43
Operator : DD\AJ
Sample : L2773-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NM4-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 10:37:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 29 02:25:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

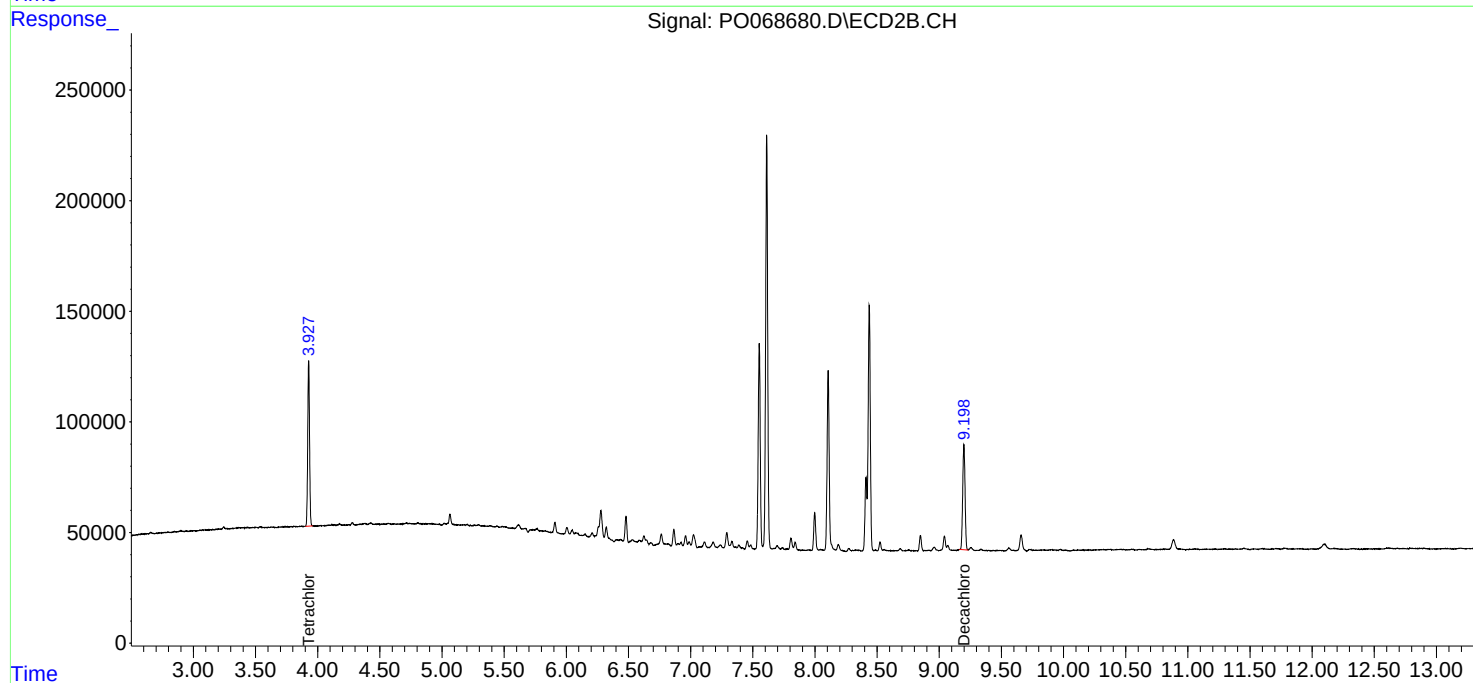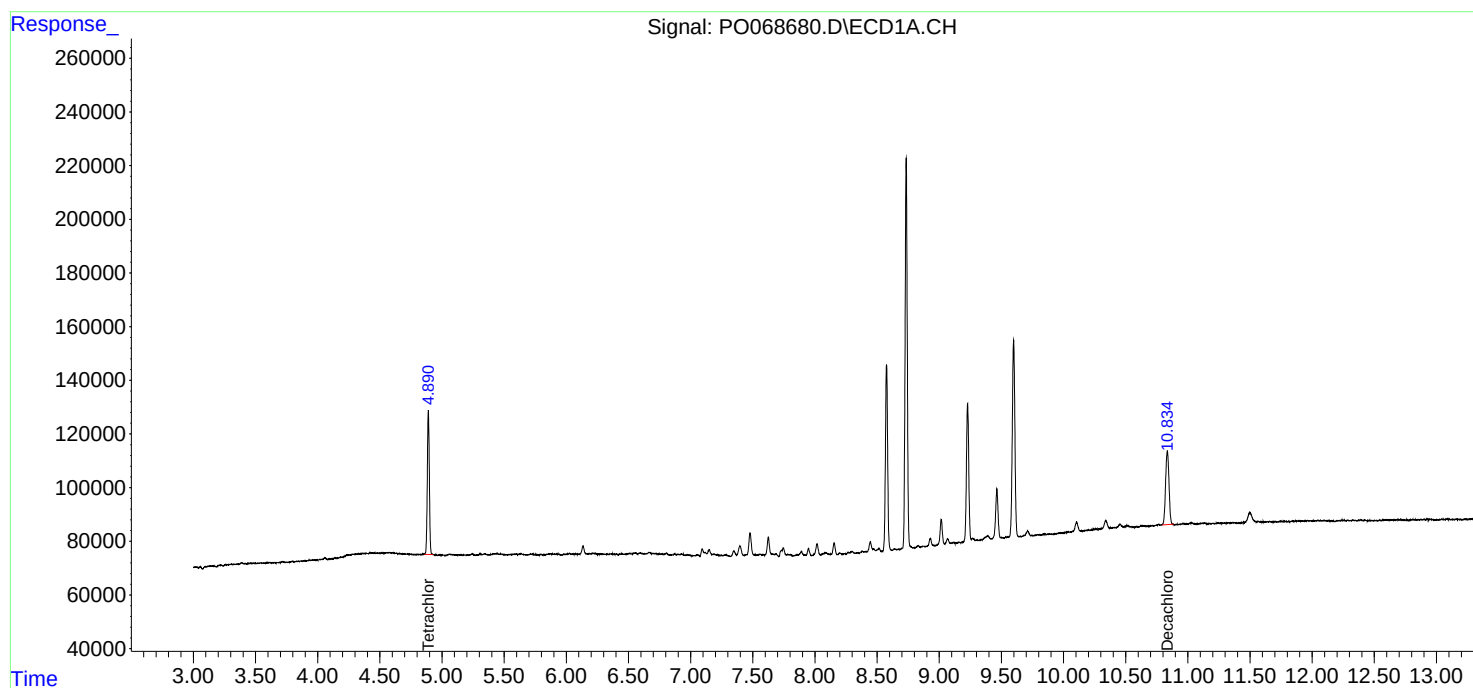


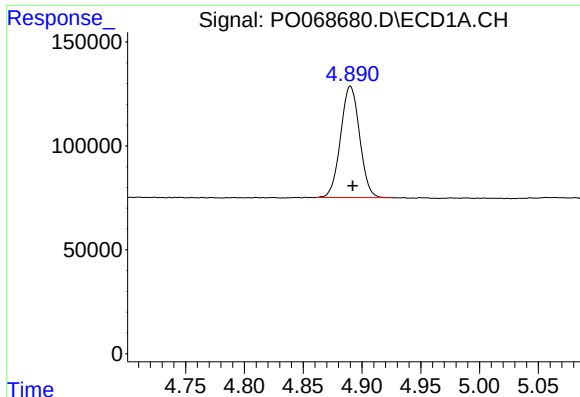

#1 Tetrachloro-m-xylene


R.T.: 4.890 min
Delta R.T.: -0.002 min
Response: 603875
Conc: 19.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
NM4-COMP-2020-0-6

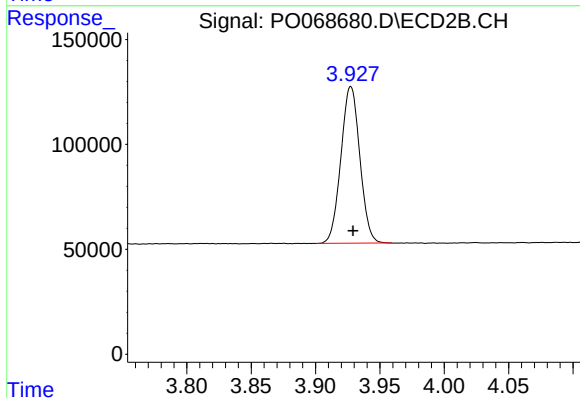


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 764671
Conc: 20.68 ng/ml

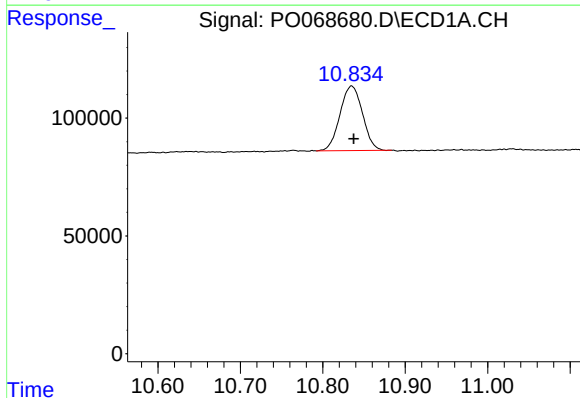

#2 Decachlorobiphenyl

R.T.: 10.835 min
Delta R.T.: -0.003 min
Response: 519643
Conc: 11.85 ng/ml

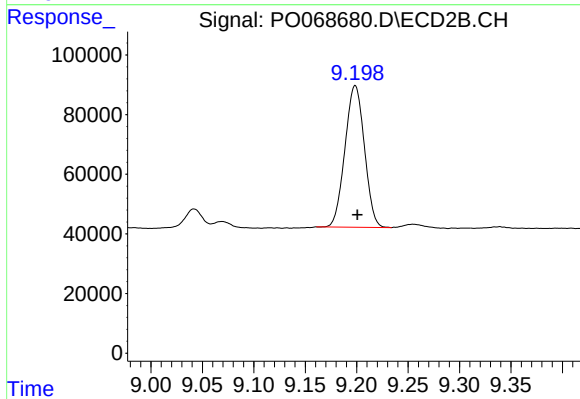

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.002 min
Response: 625719
Conc: 14.69 ng/ml