

Data Path : P:\HPCHEM1\ECD_0\Data\P0060118\
 Data File : P0045294.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 May 2018 19:15
 Operator : SM/UA
 Sample : J3184-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUCT-BANK-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 00:58:13 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.275	5527413	7122807	26.463	25.687
2) SA Decachlor...	9.281	7.996	5215322	6367266	22.708	22.592
Target Compounds						
22) L5 AR-1248-2	0.000	4.833	0	353207	N.D.	34.326 #
32) L7 AR-1260-2	0.000	5.881	0	227521	N.D.	10.769 #
34) L7 AR-1260-4	0.000	6.715	0	239845	N.D.	6.092 #
35) L7 AR-1260-5	0.000	7.047	0	199216	N.D.	7.238 #
36) L8 AR-1262-1	0.000	5.881	0	227521	N.D.	12.019 #
40) L8 AR-1262-5	0.000	6.715	0	239845	N.D.	4.402 #
41) L9 AR-1268-1	0.000	7.047	0	199216	N.D.	3.611 #
42) L9 AR-1268-2	0.000	7.047	0	199216	N.D.	3.901 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO060118\
Data File : PO045294.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 19:15
Operator : SM/UA
Sample : J3184-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 00:58:13 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

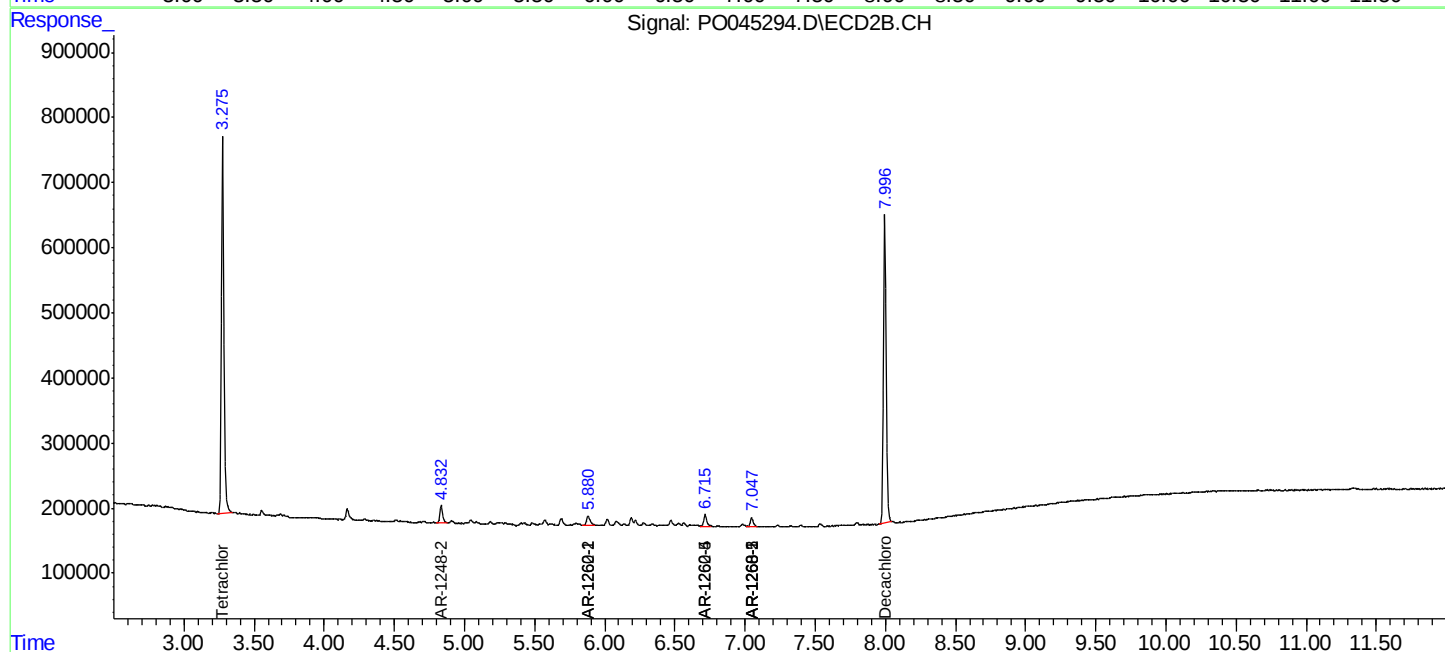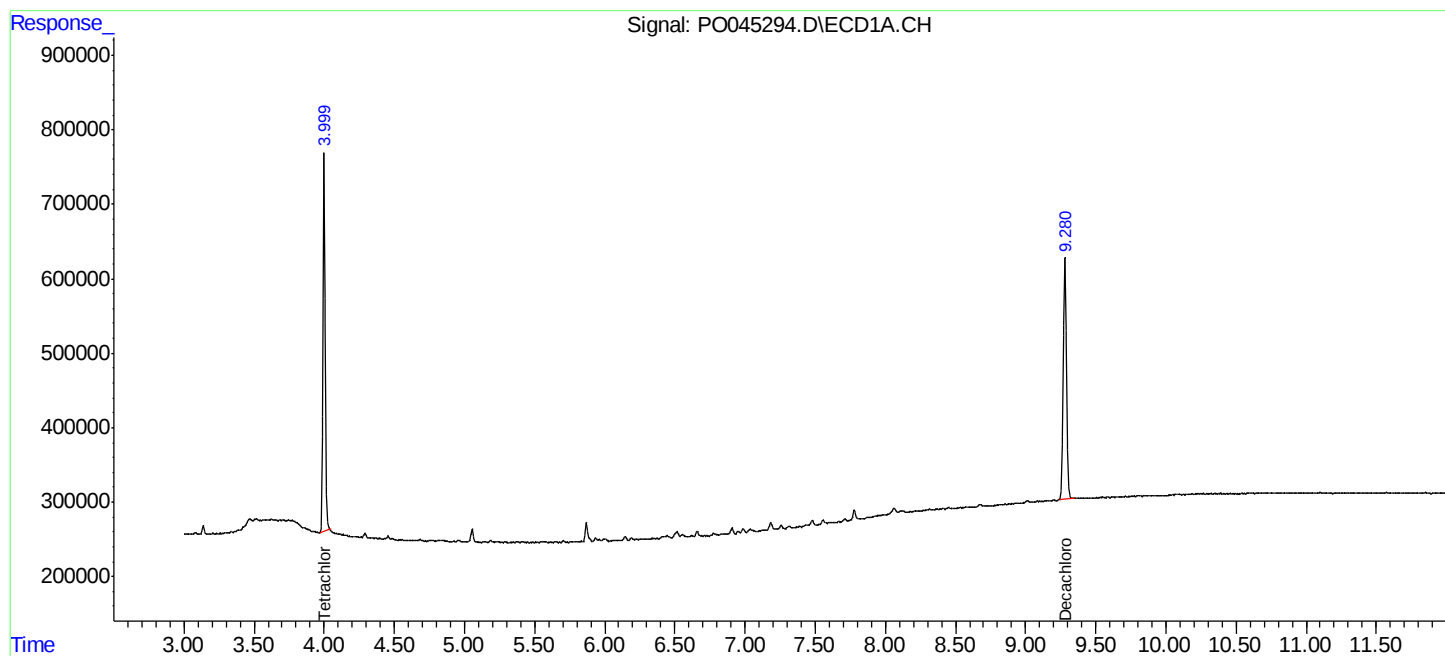


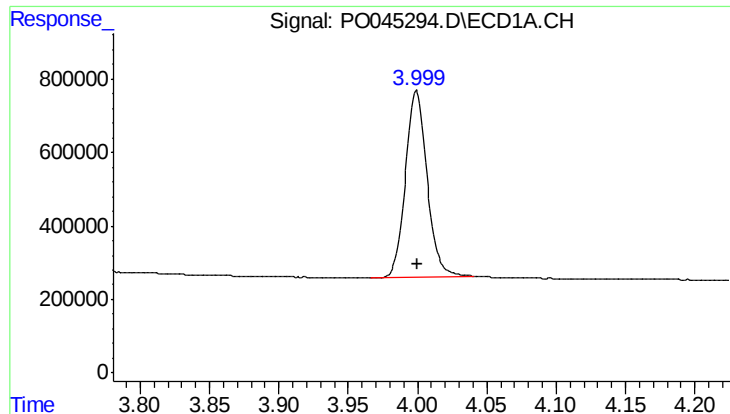

#1 Tetrachloro-m-xylene


R.T.: 3.999 min
Delta R.T.: -0.001 min
Response: 5527413
Conc: 26.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

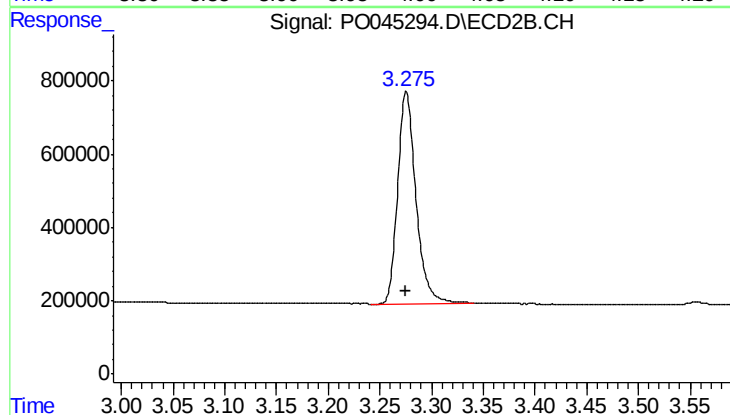


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: 0.000 min
Response: 7122807
Conc: 25.69 ng/ml

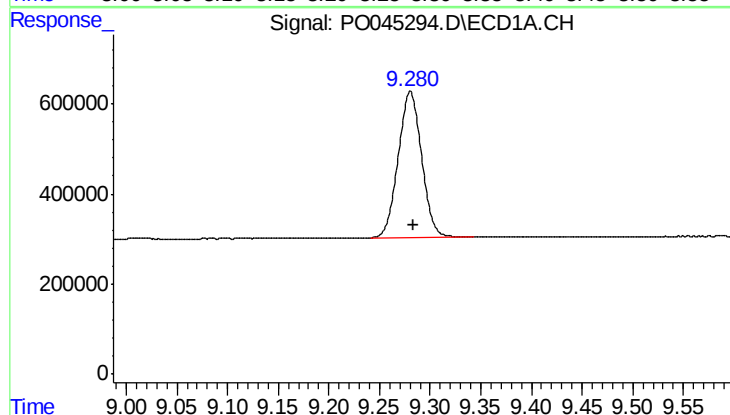


#2 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: -0.003 min
Response: 5215322
Conc: 22.71 ng/ml

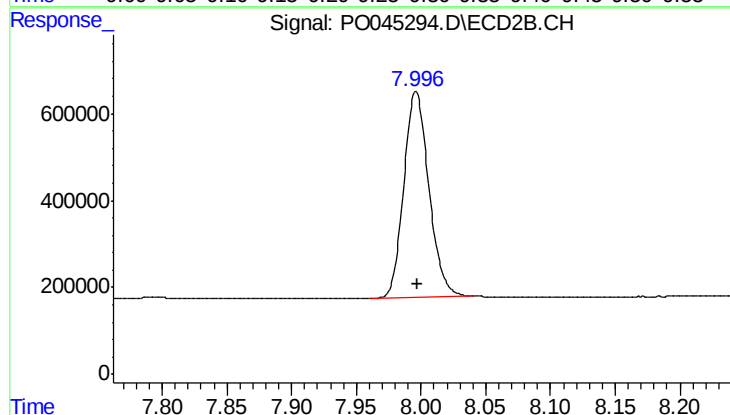

#2 Decachlorobiphenyl


R.T.: 7.996 min
Delta R.T.: -0.001 min
Response: 6367266
Conc: 22.59 ng/ml

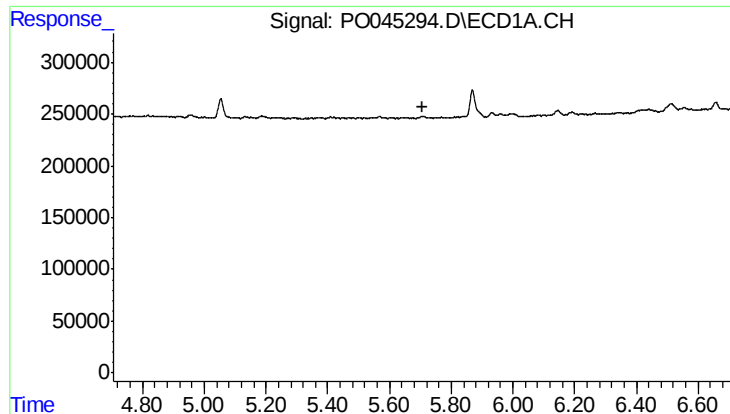

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

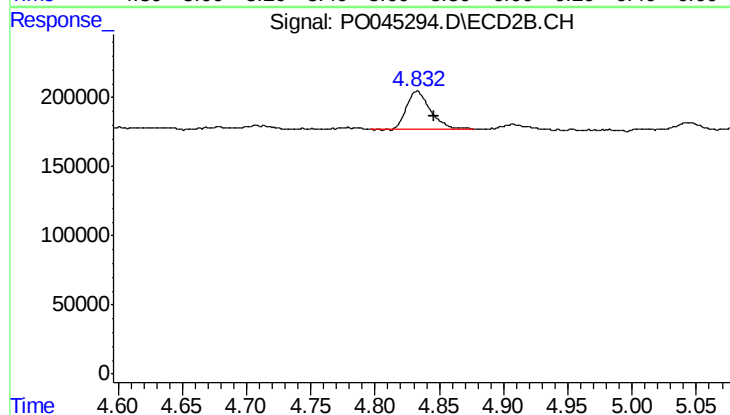


#22 AR-1248-2

R.T.: 4.833 min
Delta R.T.: -0.013 min
Response: 353207
Conc: 34.33 ng/ml

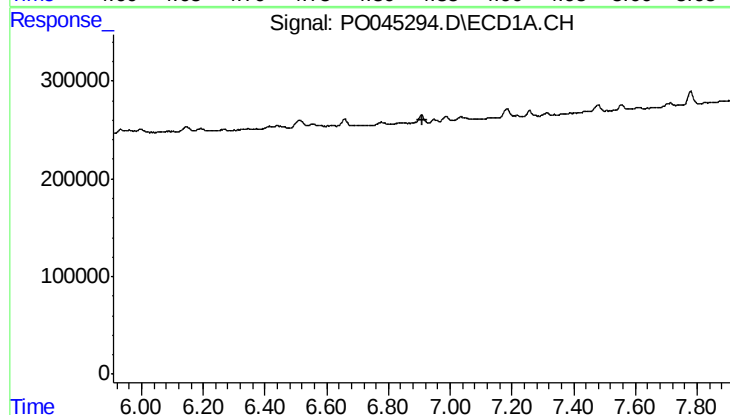


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.909 min
Response: 0
Conc: N.D.

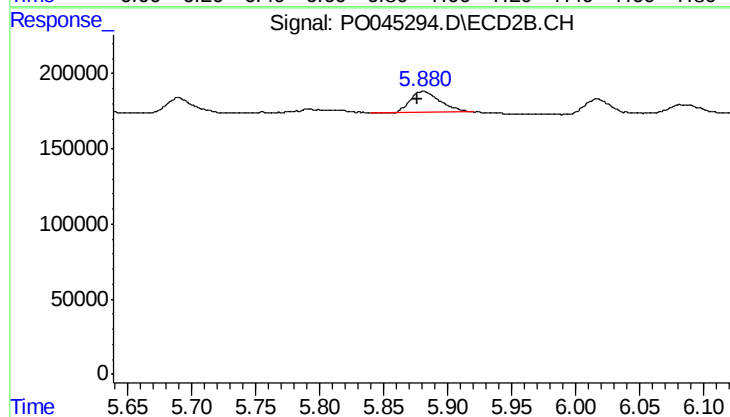

#32 AR-1260-2


R.T.: 5.881 min
Delta R.T.: 0.004 min
Response: 227521
Conc: 10.77 ng/ml

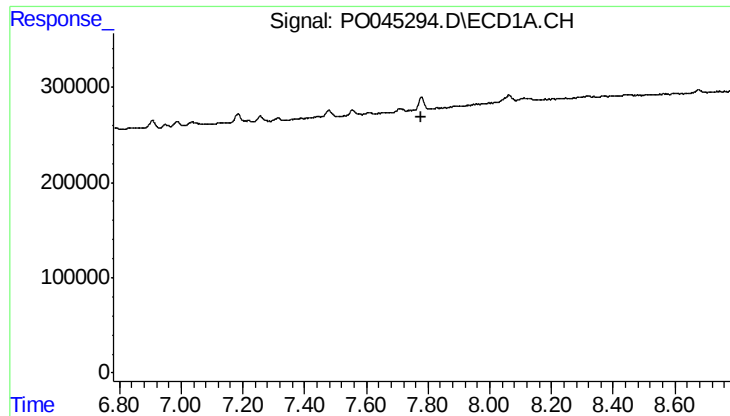

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

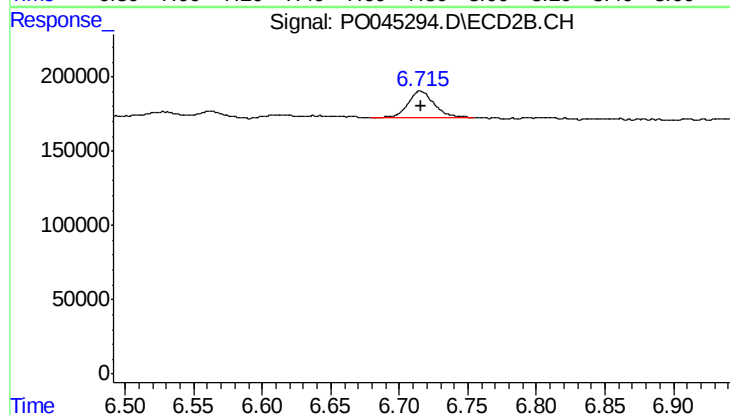


#34 AR-1260-4

R.T.: 6.715 min
Delta R.T.: 0.000 min
Response: 239845
Conc: 6.09 ng/ml

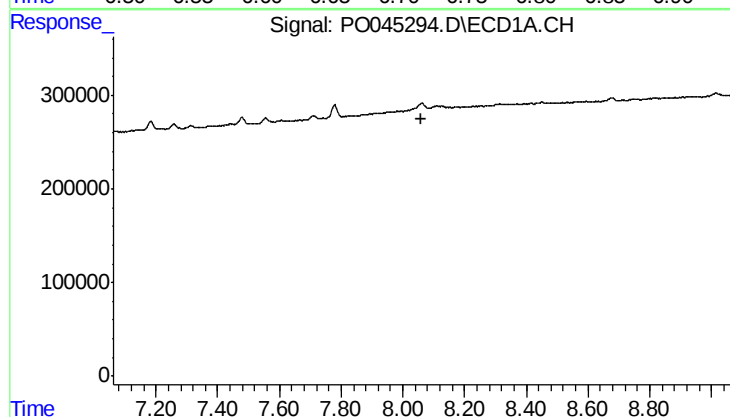


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.062 min
Response: 0
Conc: N.D.

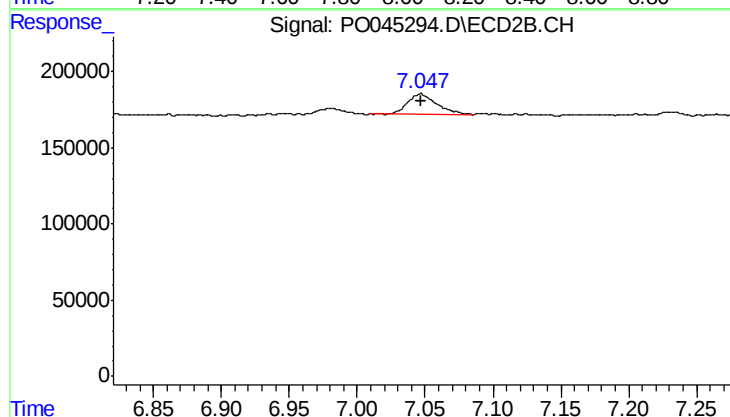

#35 AR-1260-5


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 199216
Conc: 7.24 ng/ml

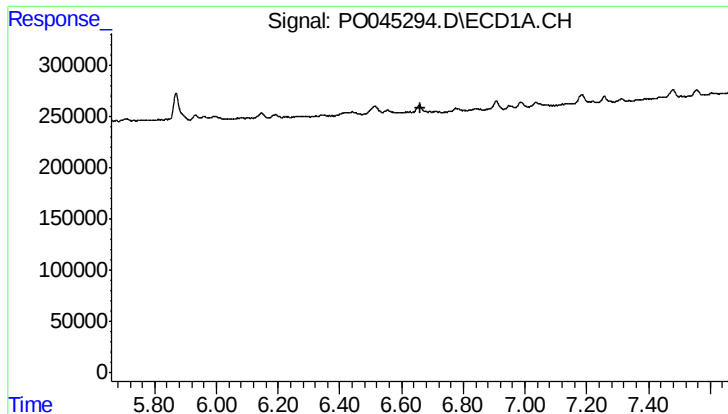

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 6.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

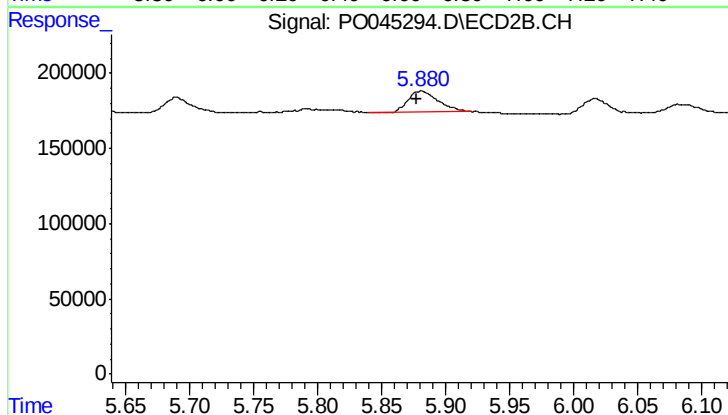


#36 AR-1262-1

R.T.: 5.881 min
Delta R.T.: 0.003 min
Response: 227521
Conc: 12.02 ng/ml

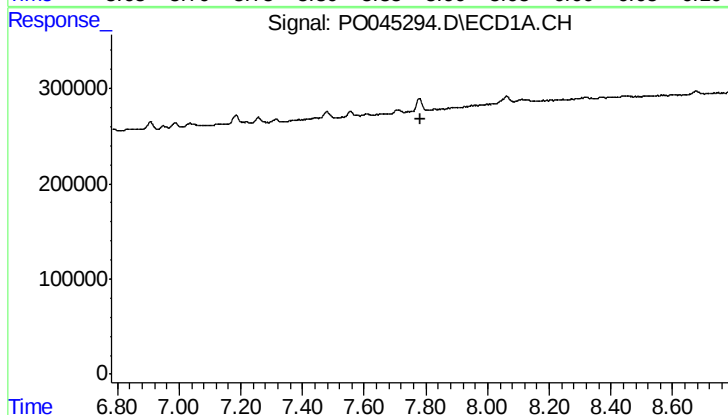


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

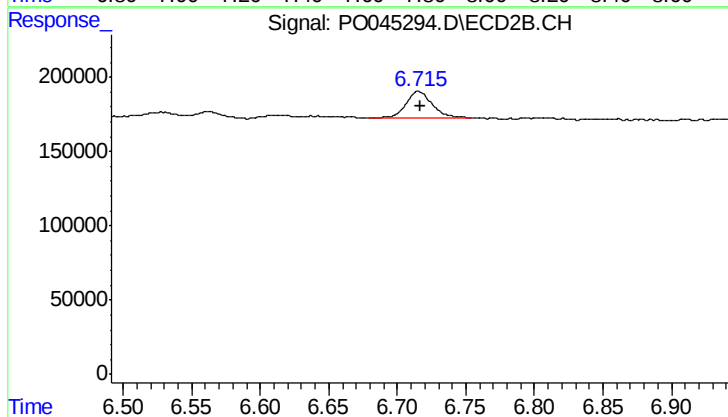

#40 AR-1262-5


R.T.: 6.715 min
Delta R.T.: -0.001 min
Response: 239845
Conc: 4.40 ng/ml

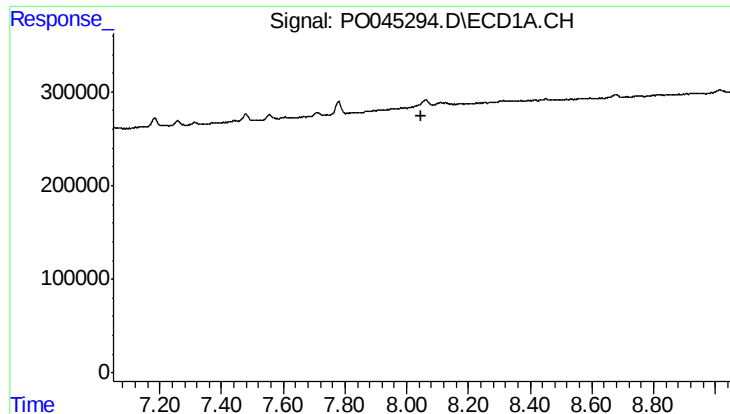

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-C

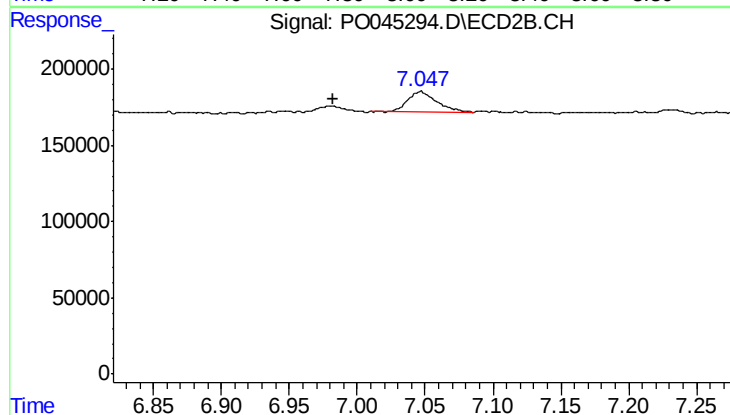


#41 AR-1268-1

R.T.: 7.047 min
Delta R.T.: 0.064 min
Response: 199216
Conc: 3.61 ng/ml

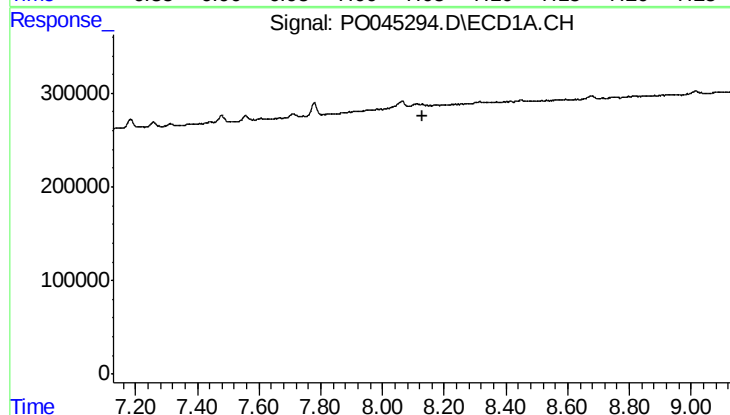

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.128 min
Response: 0
Conc: N.D.

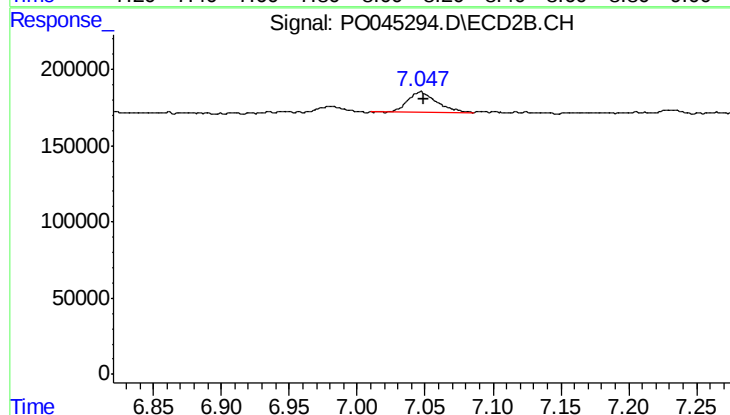

#42 AR-1268-2

R.T.: 7.047 min
Delta R.T.: -0.002 min
Response: 199216
Conc: 3.90 ng/ml