

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
 Data File : P0045291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 May 2018 18:30
 Operator : SM/UA
 Sample : J3184-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DUCT-BANK-MANHOLE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 01:36:51 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.275	5256576	6481625	25.166	23.375
2) SA Decachlor...	9.281	7.997	4895719	5798701	21.316	20.574

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 18:30
Operator : SM/UA
Sample : J3184-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-MANHOLE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 01:36:51 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

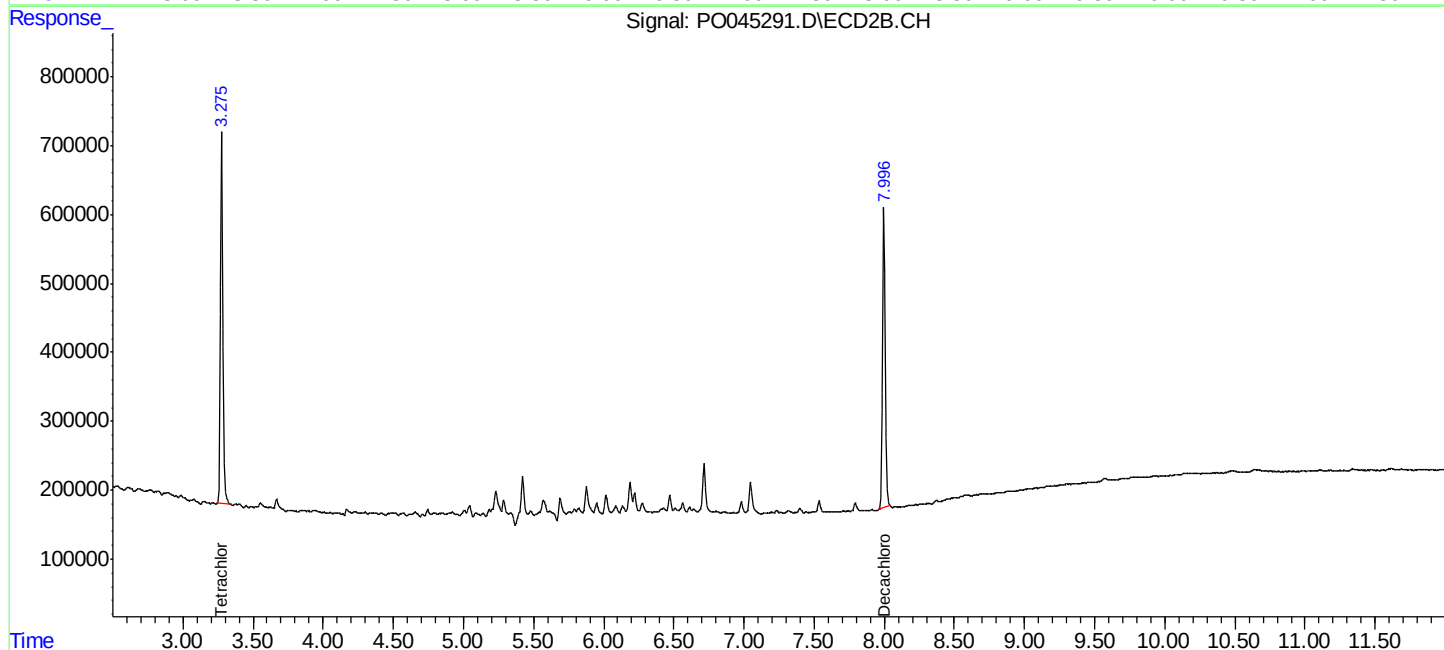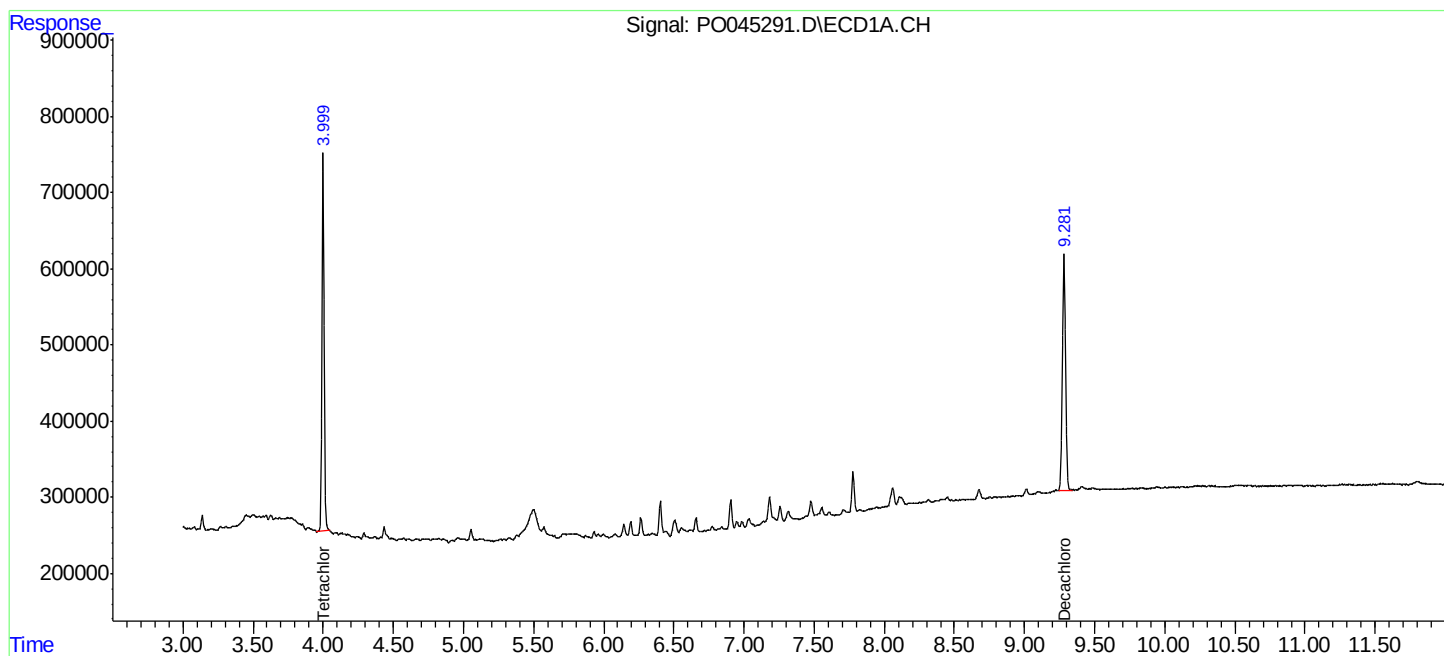


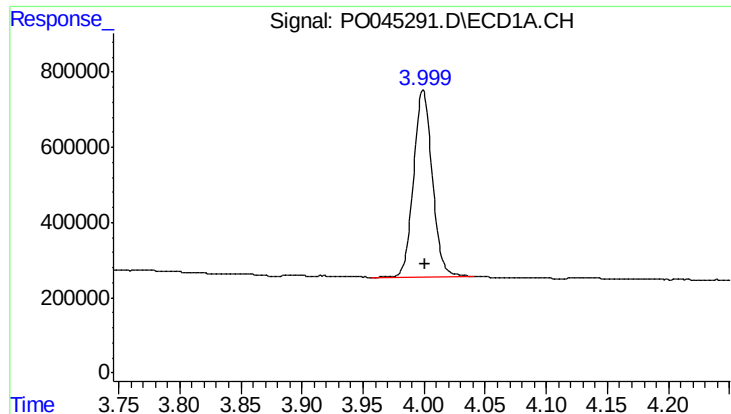

#1 Tetrachloro-m-xylene


R.T.: 3.999 min
Delta R.T.: -0.001 min
Response: 5256576
Conc: 25.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK-MANHOLE

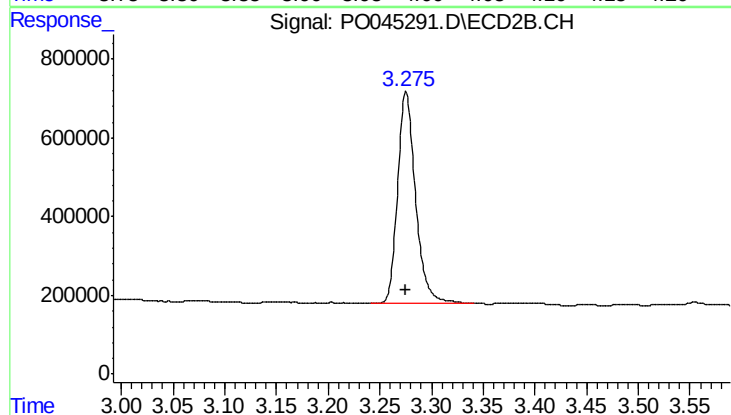


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: 0.000 min
Response: 6481625
Conc: 23.37 ng/ml

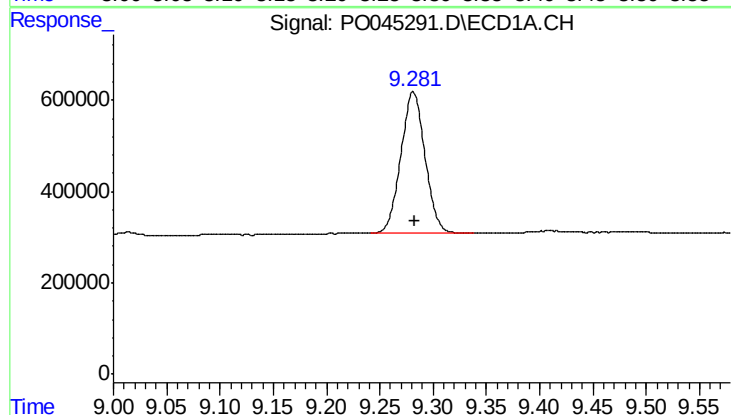

#2 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: -0.002 min
Response: 4895719
Conc: 21.32 ng/ml

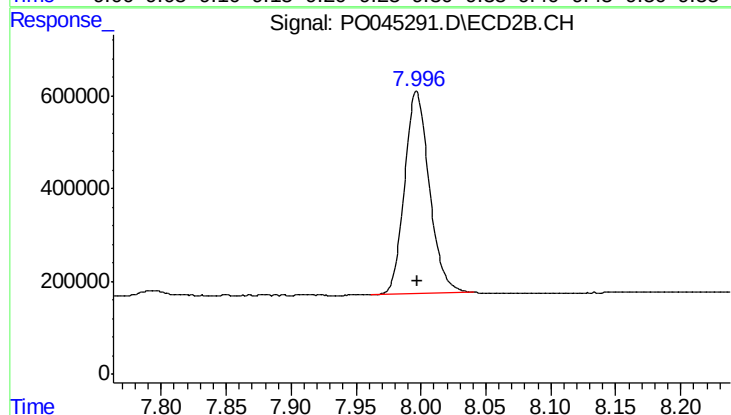

#2 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 5798701
Conc: 20.57 ng/ml