

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD_0\Data\P0060118\
 Data File : P0045295.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 May 2018 19:30
 Operator : SM/UA
 Sample : J3197-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 01:43:35 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.275	4634024	5888597	22.186	21.236
2) SA Decachlor...	9.280	7.996	3626263	4395076	15.789	15.594

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 19:30
Operator : SM/UA
Sample : J3197-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 01:43:35 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

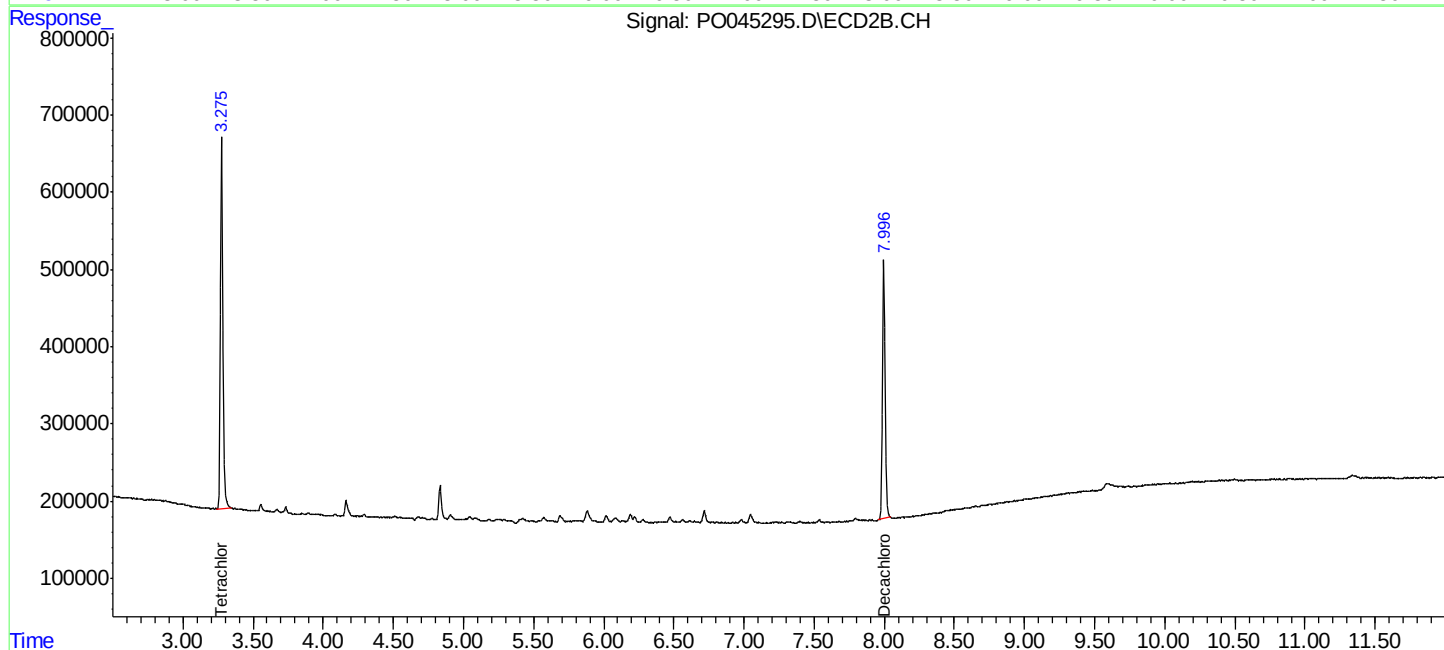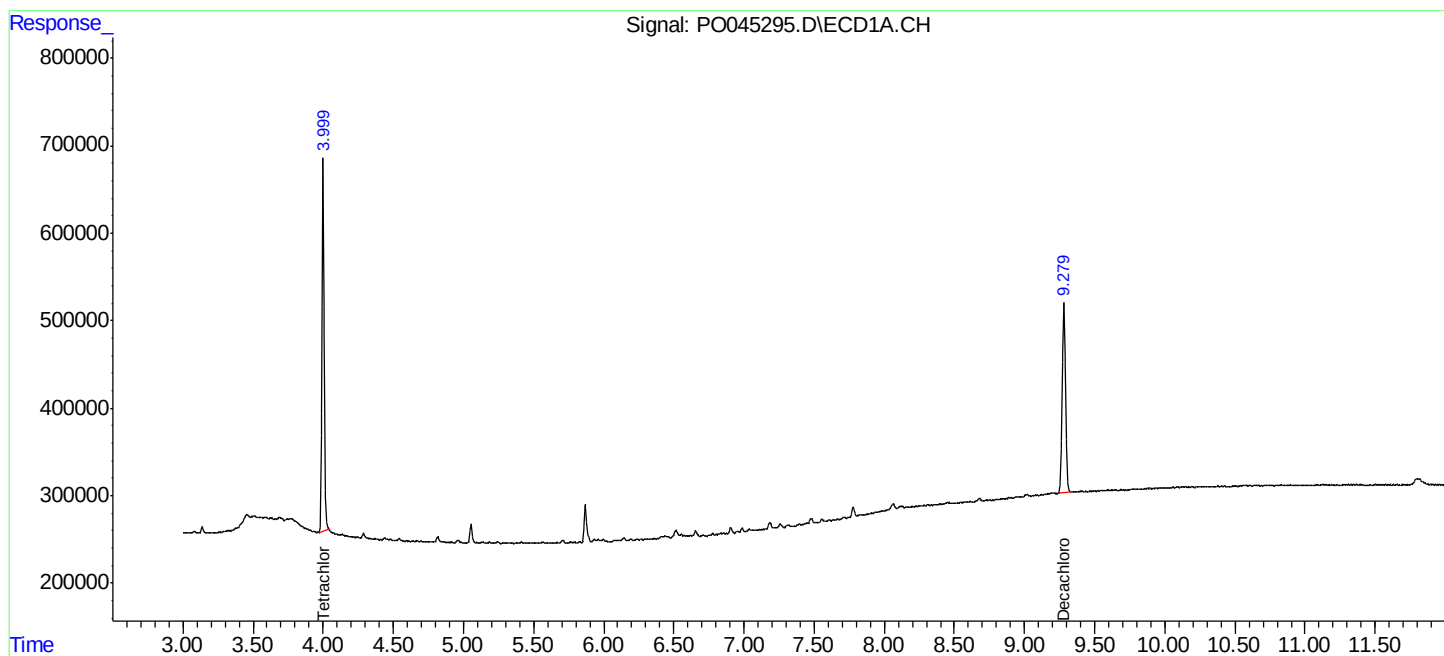


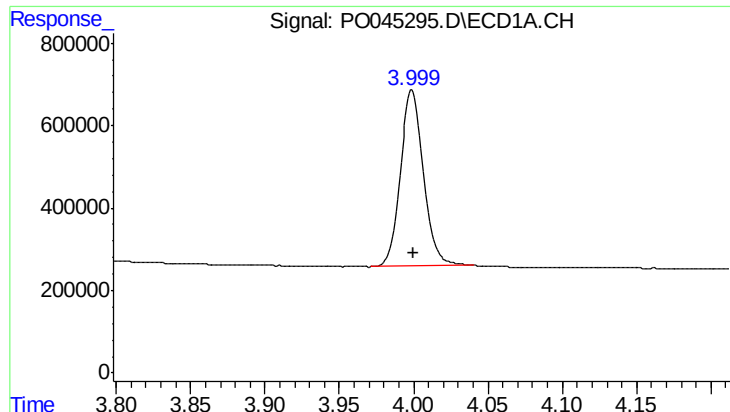

#1 Tetrachloro-m-xylene


R.T.: 3.999 min
Delta R.T.: -0.001 min
Response: 4634024
Conc: 22.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S

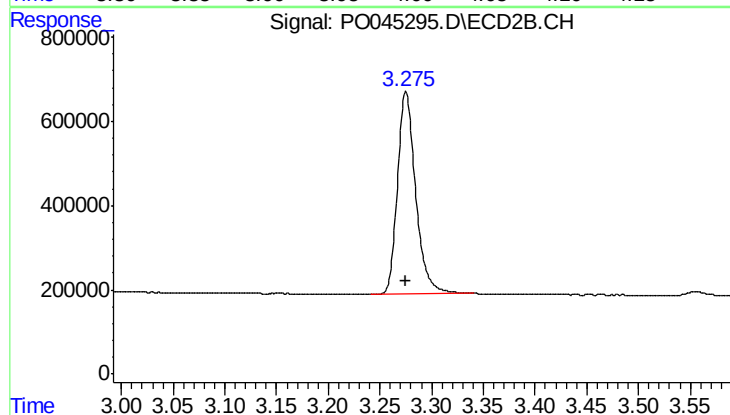


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: 0.000 min
Response: 5888597
Conc: 21.24 ng/ml

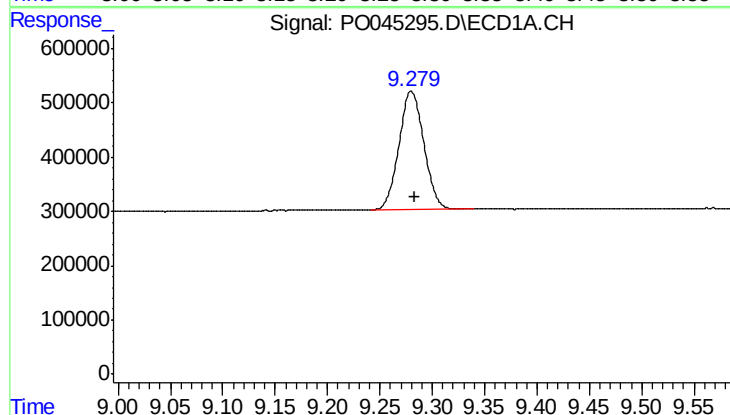

#2 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: -0.003 min
Response: 3626263
Conc: 15.79 ng/ml

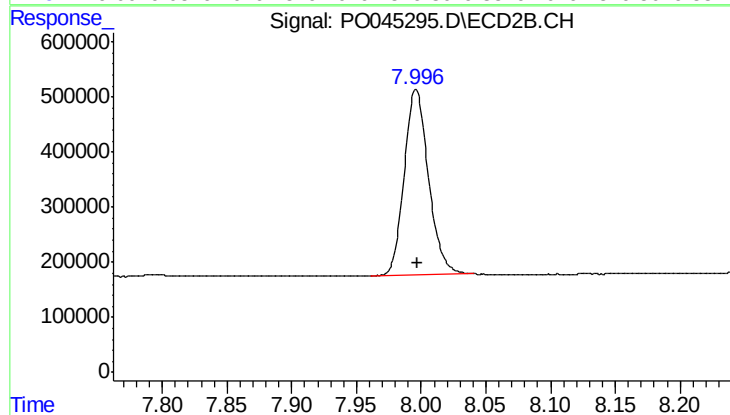

#2 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: -0.001 min
Response: 4395076
Conc: 15.59 ng/ml