

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
 Data File : P0045300.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 May 2018 20:46
 Operator : SM/UA
 Sample : J3197-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 05:58:45 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.997	3.274	5347987	6852805	25.604	24.713
2) SA Decachlor...	9.279	7.995	4551993	5652732	19.820	20.056

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 20:46
Operator : SM/UA
Sample : J3197-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:58:45 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

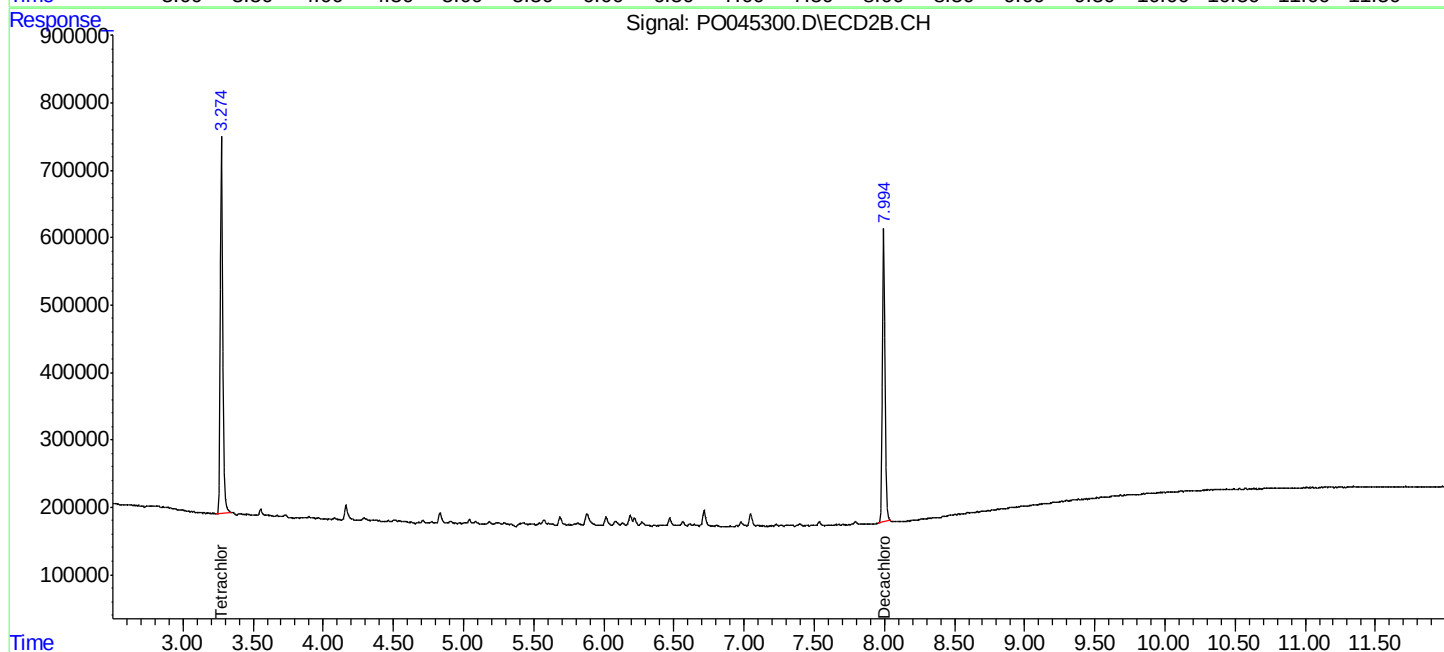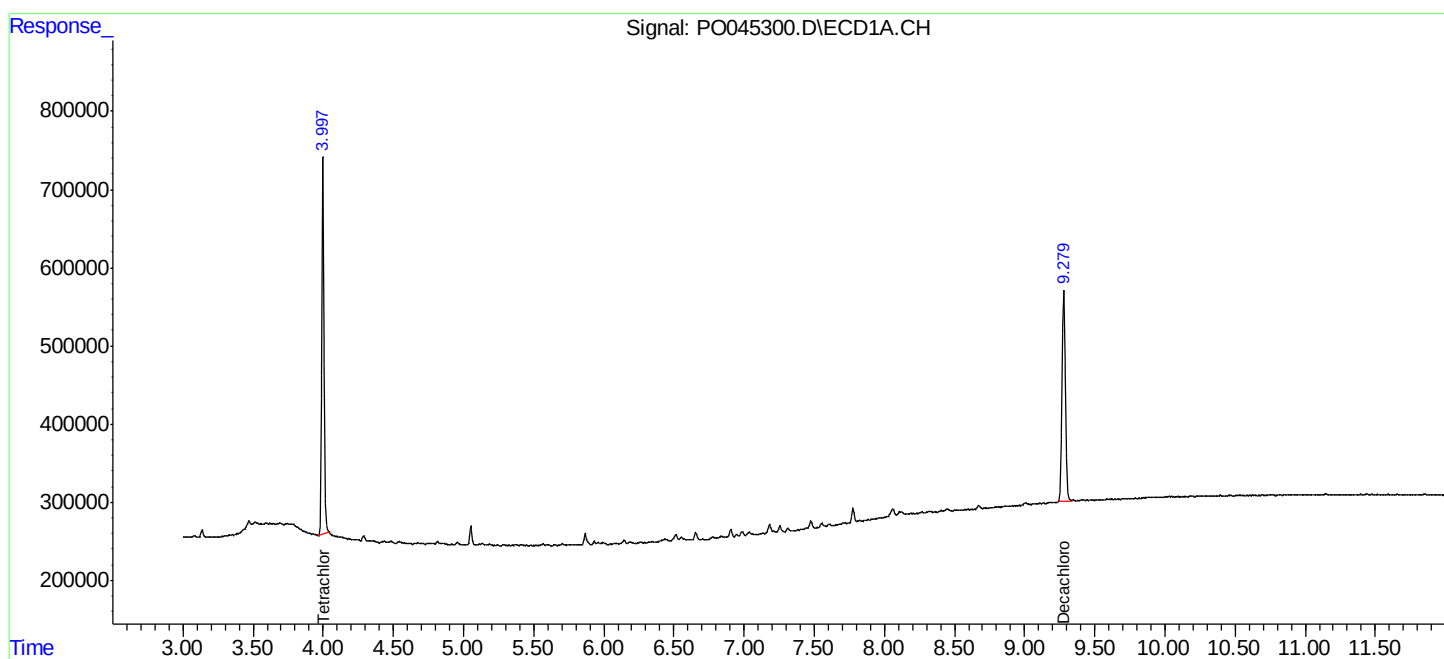


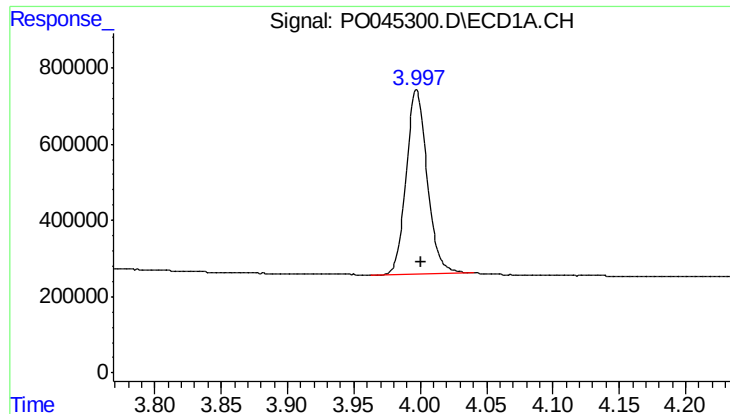

#1 Tetrachloro-m-xylene


R.T.: 3.997 min
Delta R.T.: -0.003 min
Response: 5347987
Conc: 25.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-D

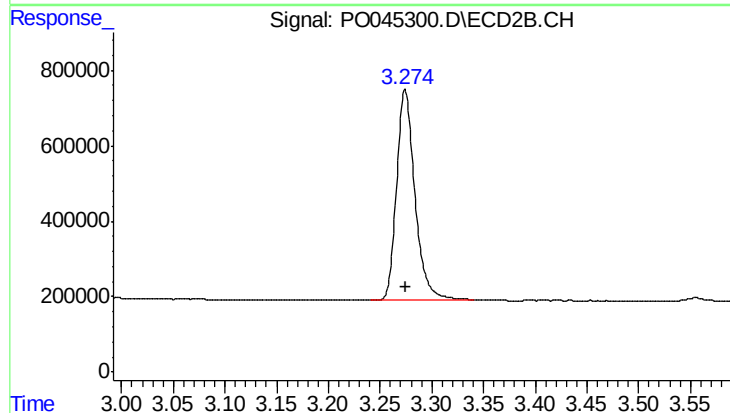


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 6852805
Conc: 24.71 ng/ml

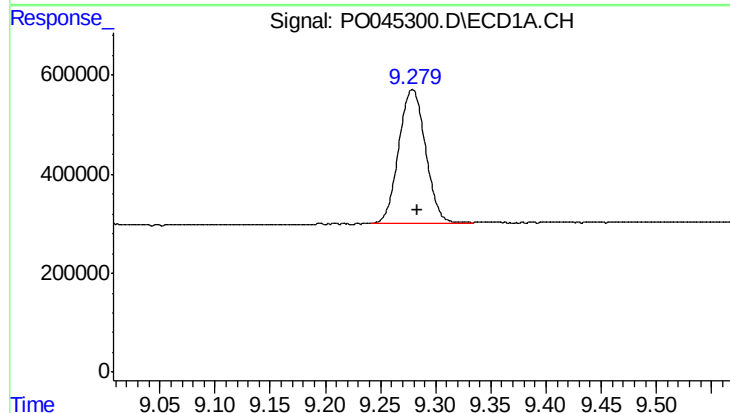

#2 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: -0.004 min
Response: 4551993
Conc: 19.82 ng/ml

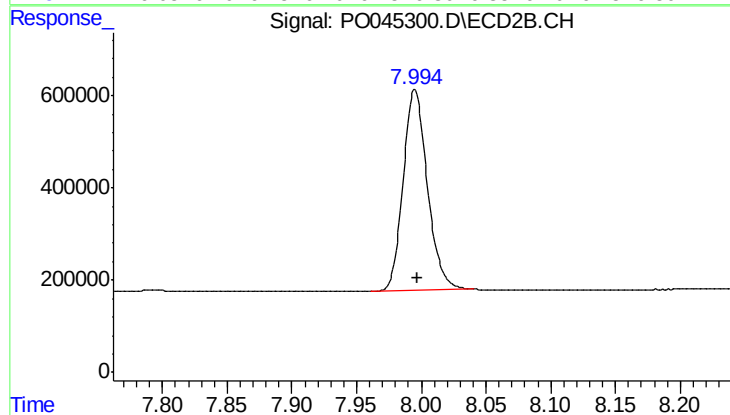

#2 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.002 min
Response: 5652732
Conc: 20.06 ng/ml