

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 23:32
Operator : SM/UA
Sample : J3171-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
052418-JETT-F-U-M

Manual Integrations
APPROVED

UGO
6/6/2018 4:19:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 04:38:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.275	5221371	6591580	24.998	23.771
2) SA Decachlor...	9.281	7.995	4791824	6176961	20.864	21.917m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\PO060118\
Data File : PO045311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2018 23:32
Operator : SM/UA
Sample : J3171-11
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
052418-JETT-F-U-M


Manual Integrations
APPROVED

UGO
6/6/2018 4:19:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 04:38:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

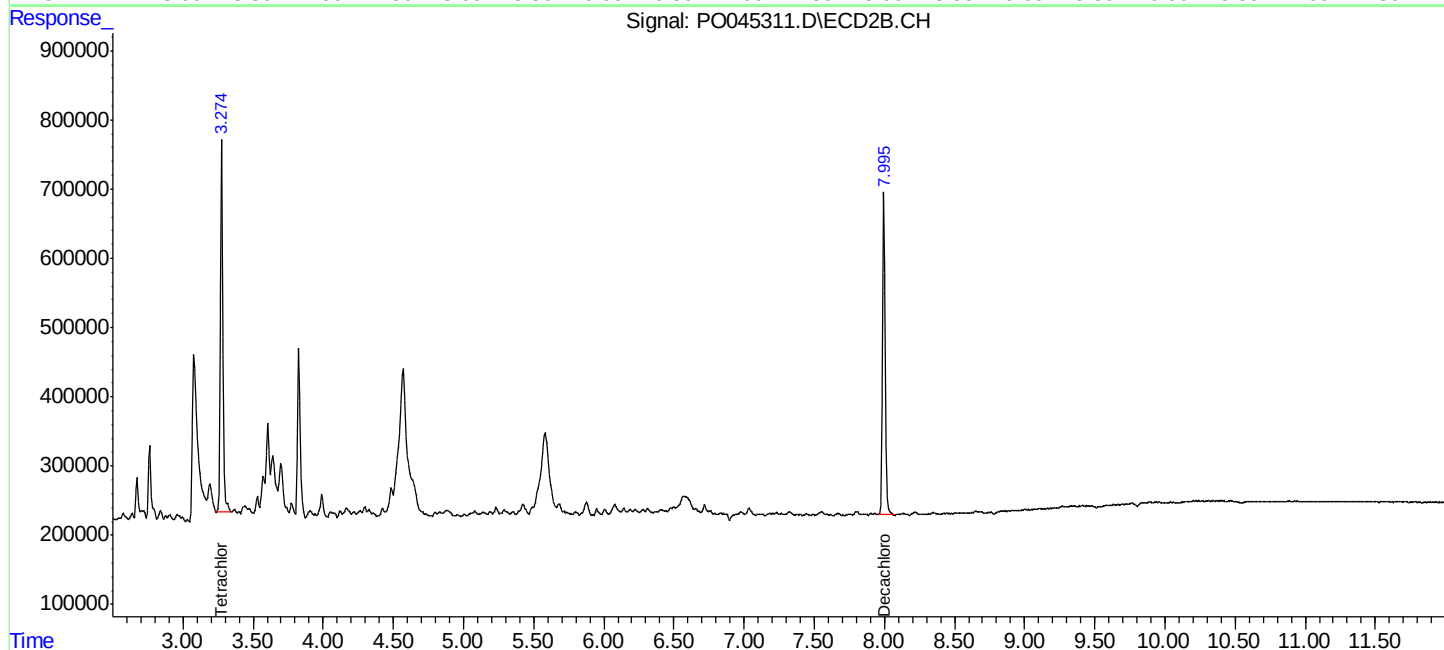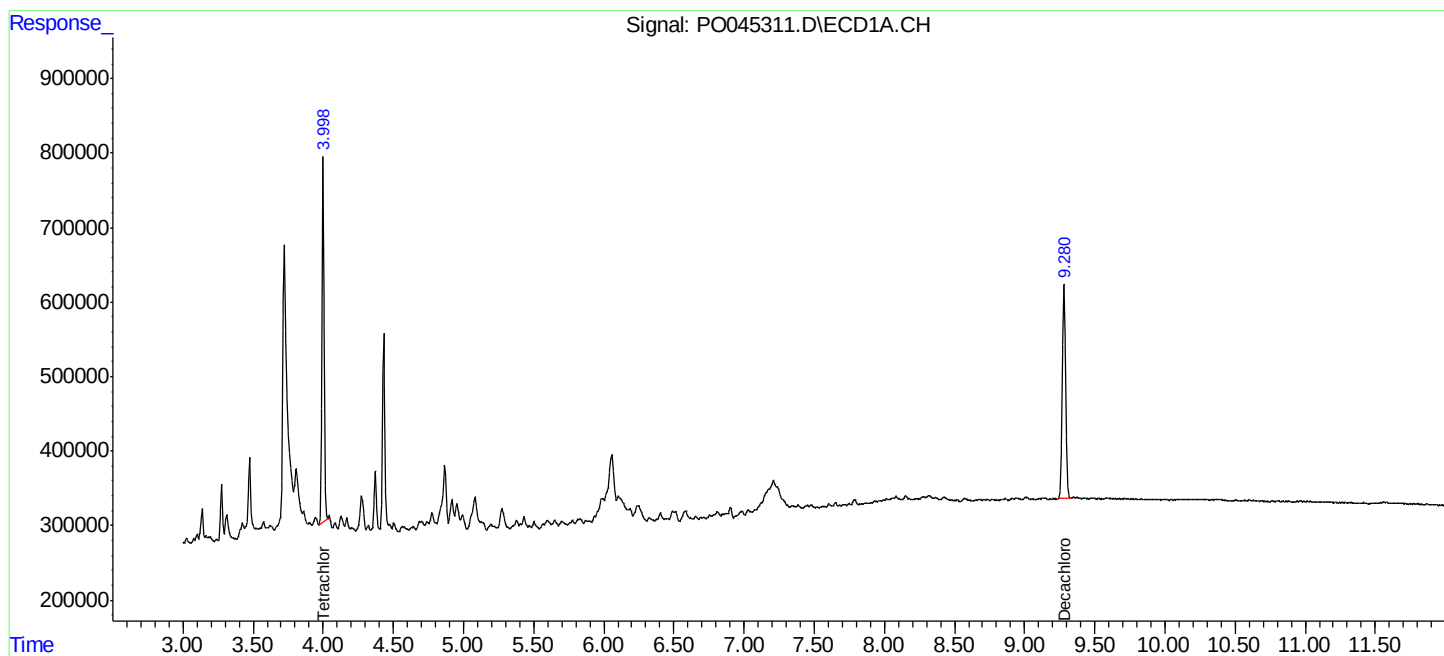

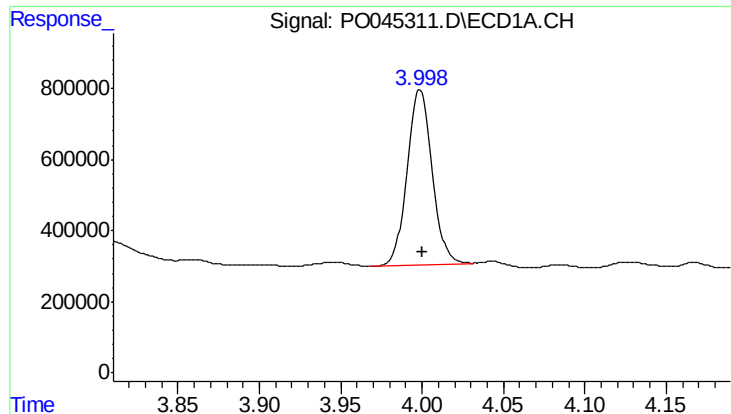


#1 Tetrachloro-m-xylene

R.T.: 3.999 min
Delta R.T.: -0.002 min
Response: 5221371
Conc: 25.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
052418-JETT-F-U-M


Manual Integrations
APPROVED

UGO
6/6/2018 4:19:13 PM

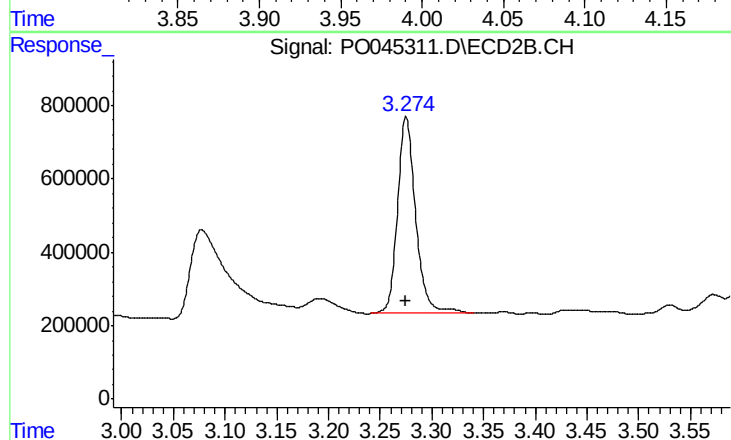


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: 0.000 min
Response: 6591580
Conc: 23.77 ng/ml

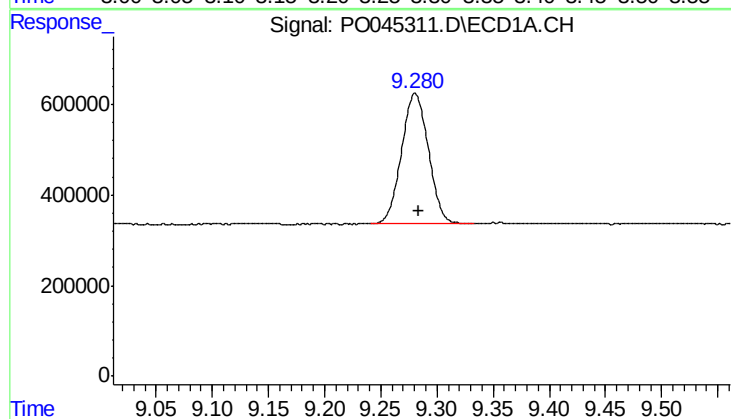

#2 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: -0.003 min
Response: 4791824
Conc: 20.86 ng/ml

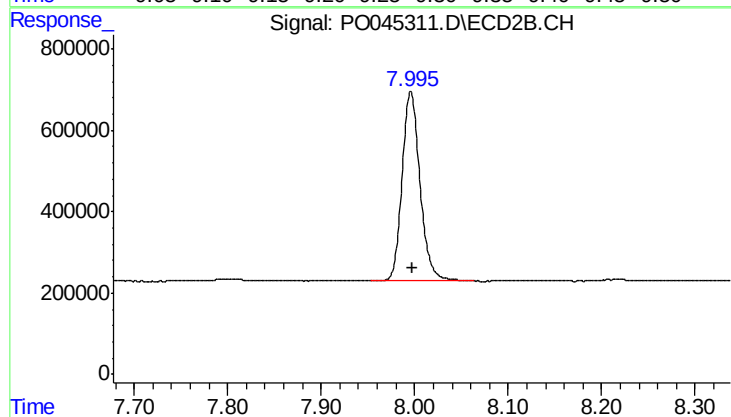

#2 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.002 min
Response: 6176961
Conc: 21.92 ng/ml m