

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045320.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2018 1:48
Operator : SM/UA
Sample : J3172-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
052518-SIDI-F-U-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:18:33 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.998	3.274	5208591	6114935	24.937	22.052
2) SA Decachlor...	9.280	7.995	4347245	5569315	18.928	19.761

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060118\
Data File : P0045320.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2018 1:48
Operator : SM/UA
Sample : J3172-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
052518-SIDI-F-U-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:18:33 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

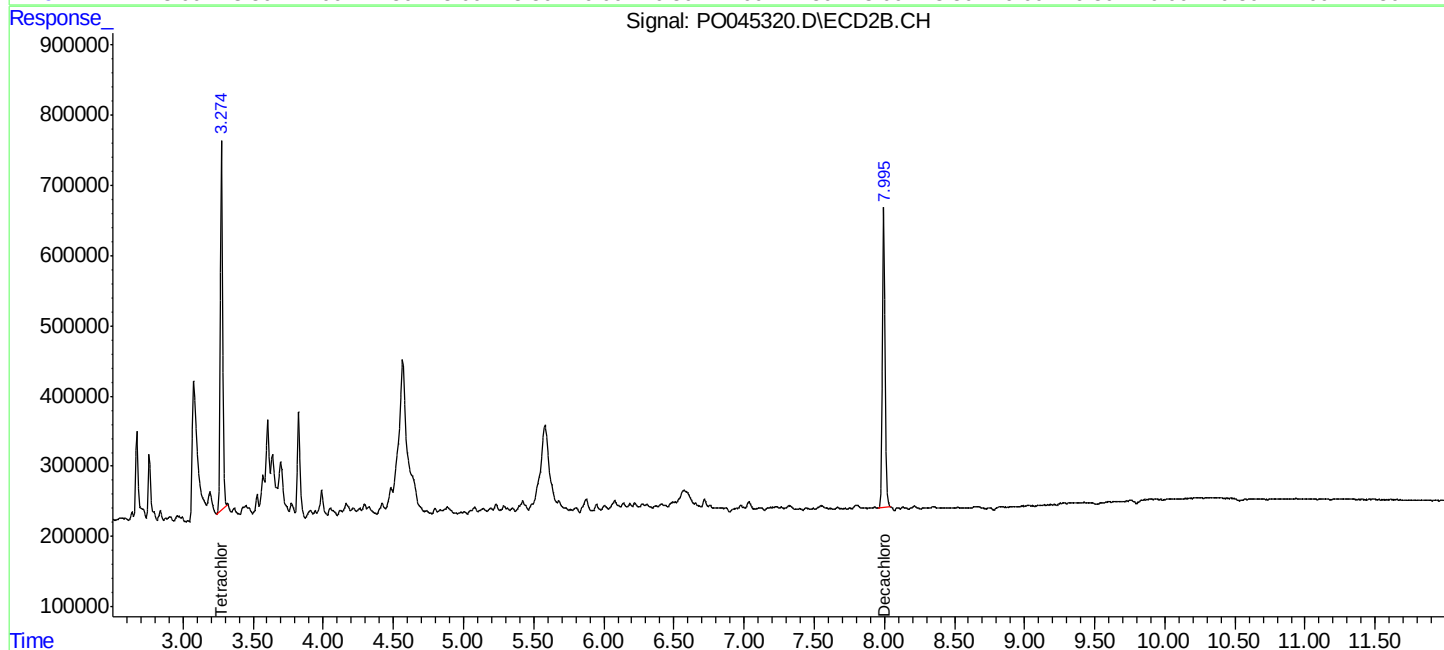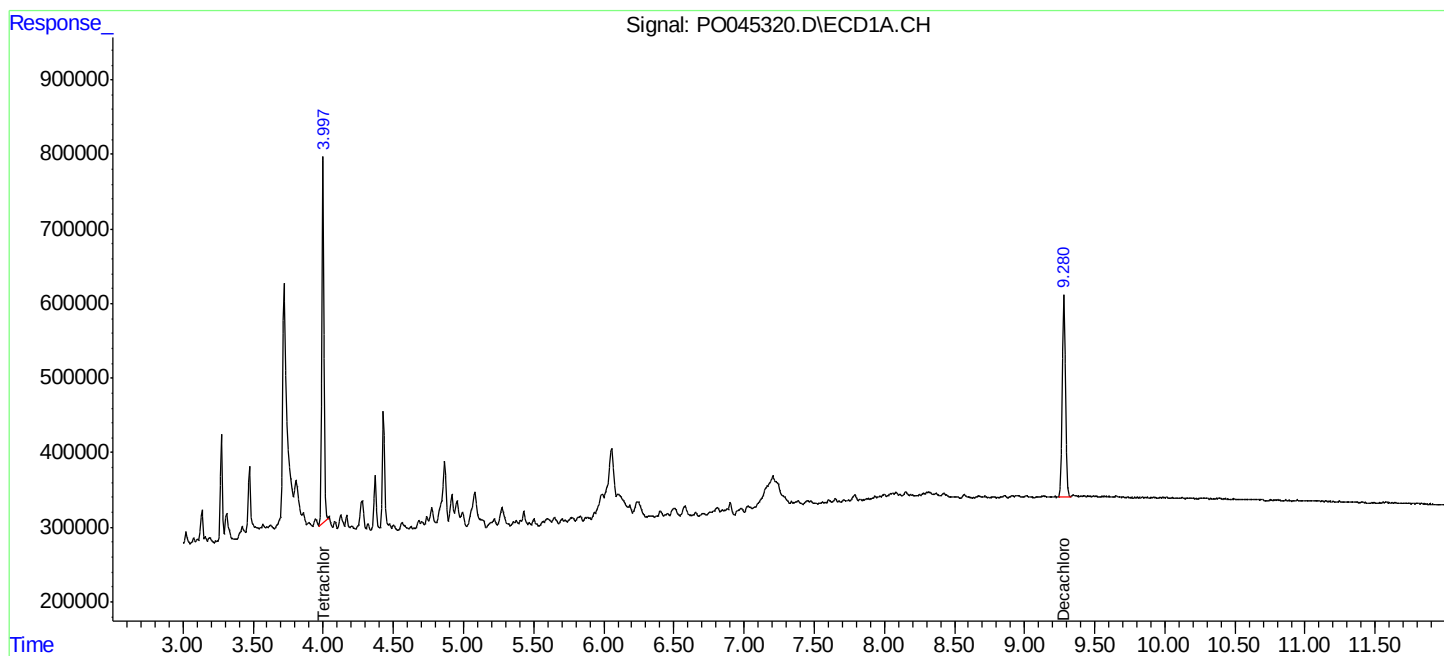


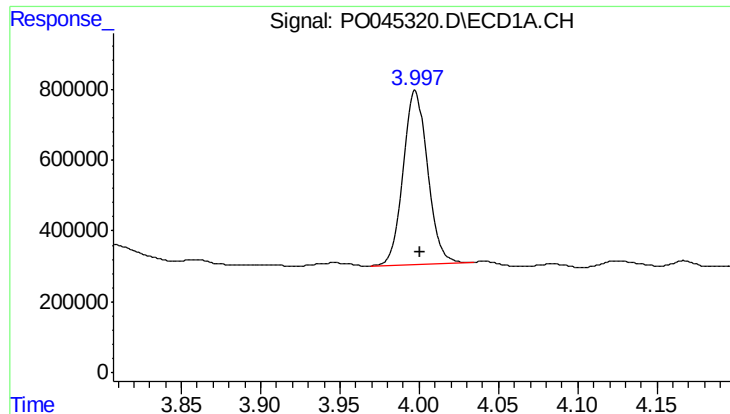

#1 Tetrachloro-m-xylene


R.T.: 3.998 min
Delta R.T.: -0.003 min
Response: 5208591
Conc: 24.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
052518-SIDI-F-U-S

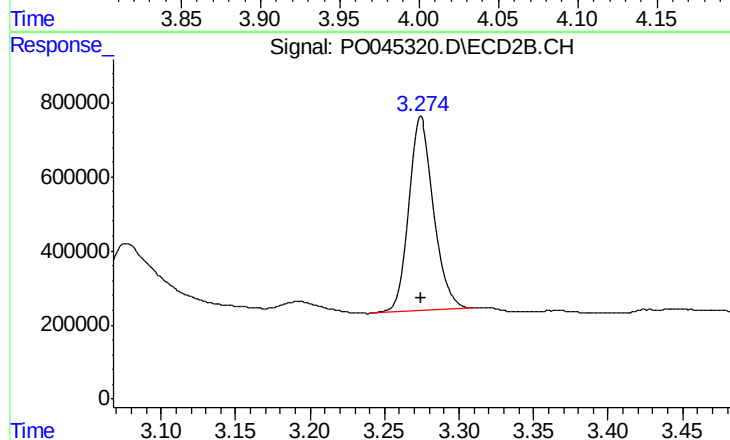


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 6114935
Conc: 22.05 ng/ml

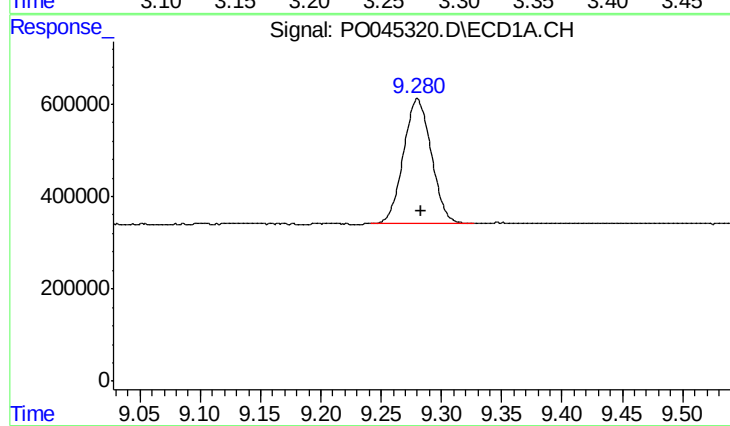

#2 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: -0.003 min
Response: 4347245
Conc: 18.93 ng/ml

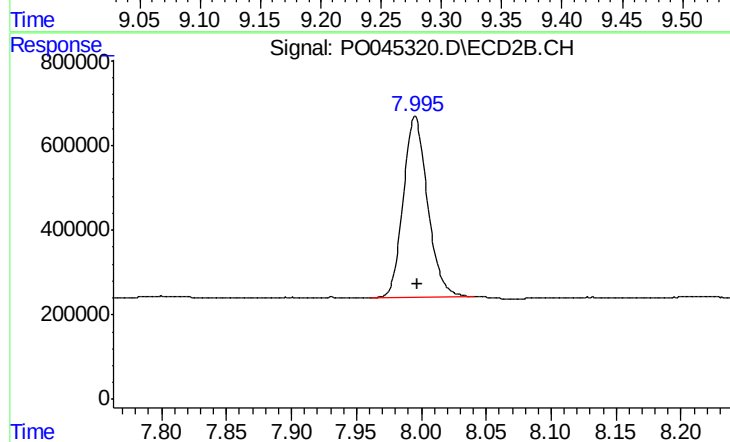

#2 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.002 min
Response: 5569315
Conc: 19.76 ng/ml