

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
 Data File : P0068744.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2020 20:40
 Operator : DD\AJ
 Sample : L2827-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-052620-SR-01

Manual Integrations
 APPROVED

Sohil
 6/3/2020 9:25:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 04:11:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 29 02:25:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.915	3.926	71955	127697	2.321m	3.457 #
2) SA Decachlor...	10.833	9.199	85366	113730	1.980	2.678m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
Data File : P0068744.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2020 20:40
Operator : DD\AJ
Sample : L2827-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-01


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 04:11:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 29 02:25:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

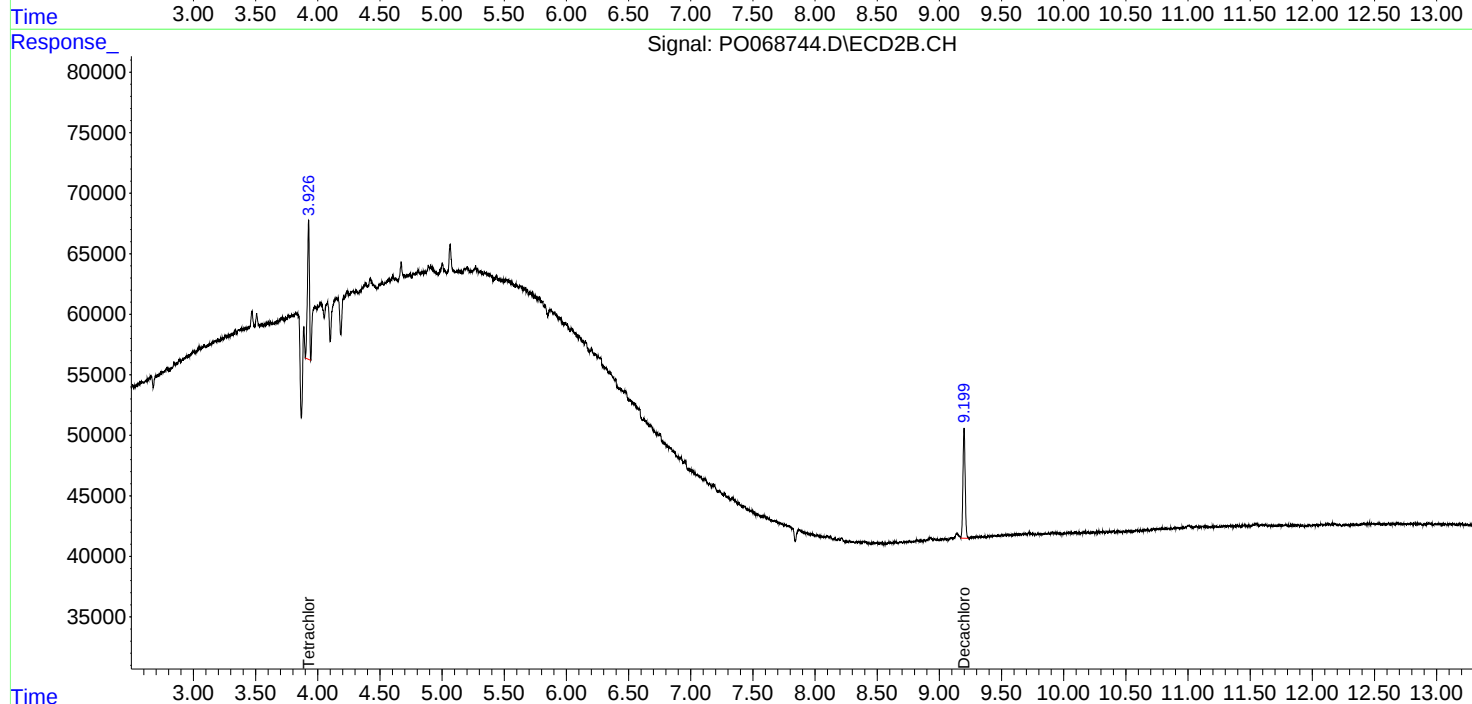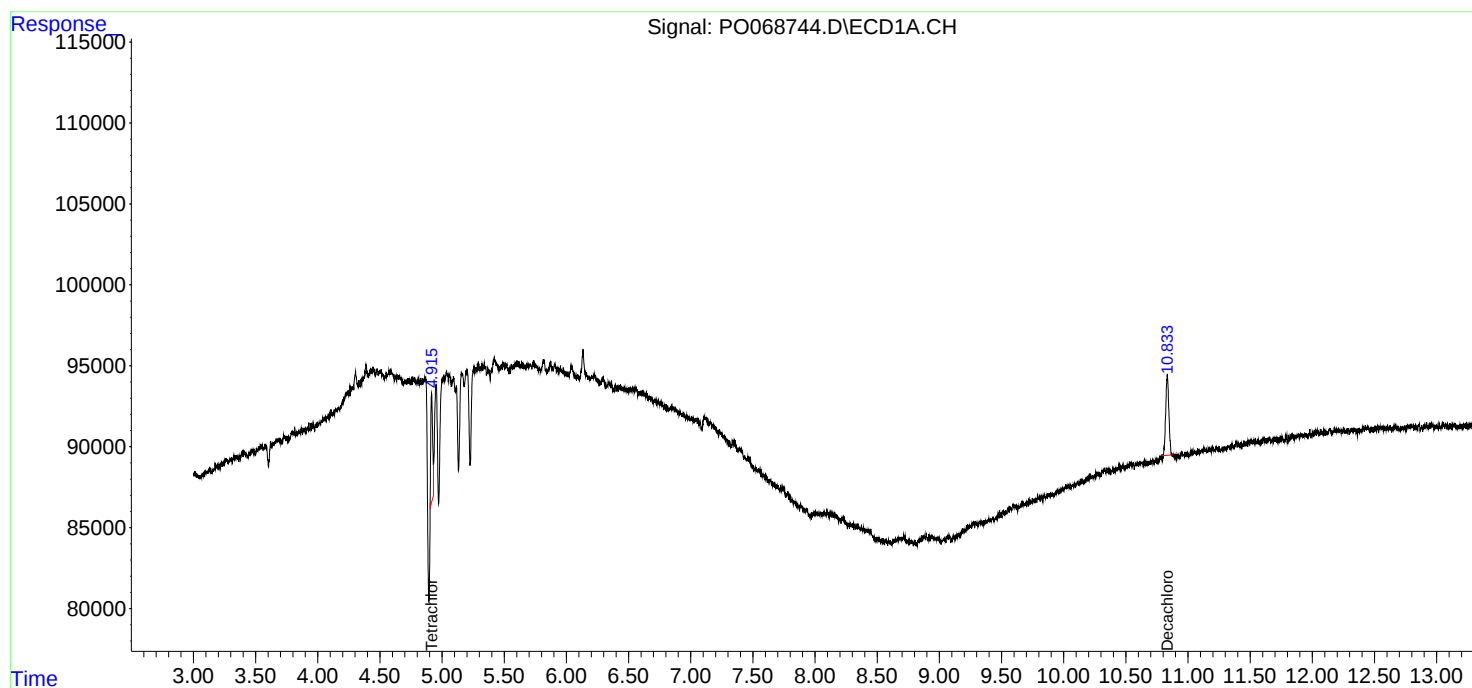

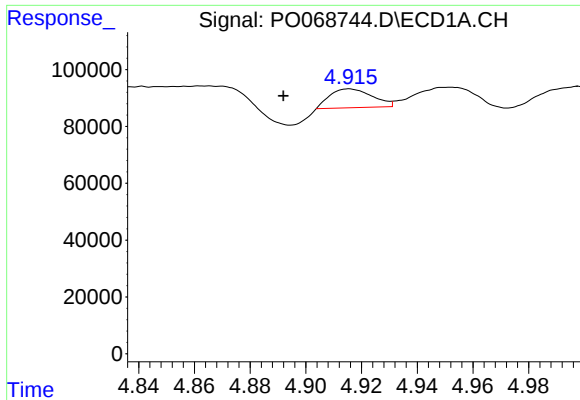


#1 Tetrachloro-m-xylene

R.T.: 4.915 min
Delta R.T.: 0.023 min
Response: 71955
Conc: 2.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-01


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:03 AM

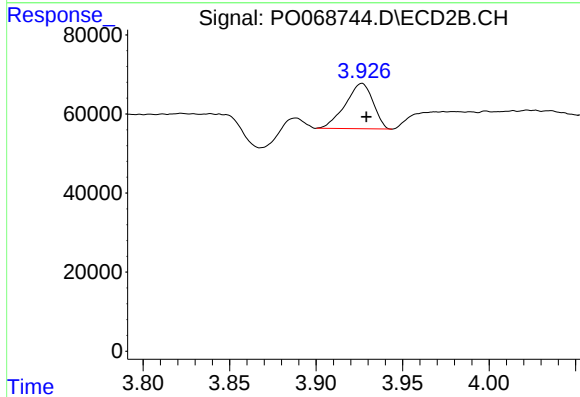


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 127697
Conc: 3.46 ng/ml

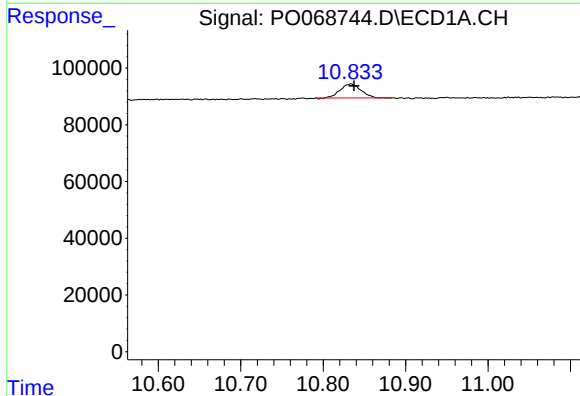

#2 Decachlorobiphenyl

R.T.: 10.833 min
Delta R.T.: -0.004 min
Response: 85366
Conc: 1.98 ng/ml

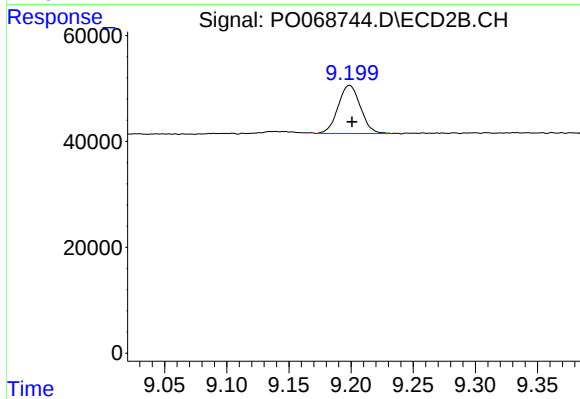

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.002 min
Response: 113730
Conc: 2.68 ng/ml m