

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
 Data File : P0068745.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2020 21:13
 Operator : DD\AJ
 Sample : L2827-02 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-052620-SR-02

Manual Integrations
 APPROVED

Sohil
 6/3/2020 9:25:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 04:11:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 29 02:25:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.887	3.927	44047	49841	1.421m	1.349
2) SA Decachlor...	10.830	9.197	55377	71163	1.284	1.676 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
Data File : P0068745.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2020 21:13
Operator : DD\AJ
Sample : L2827-02 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-02


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 04:11:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 29 02:25:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

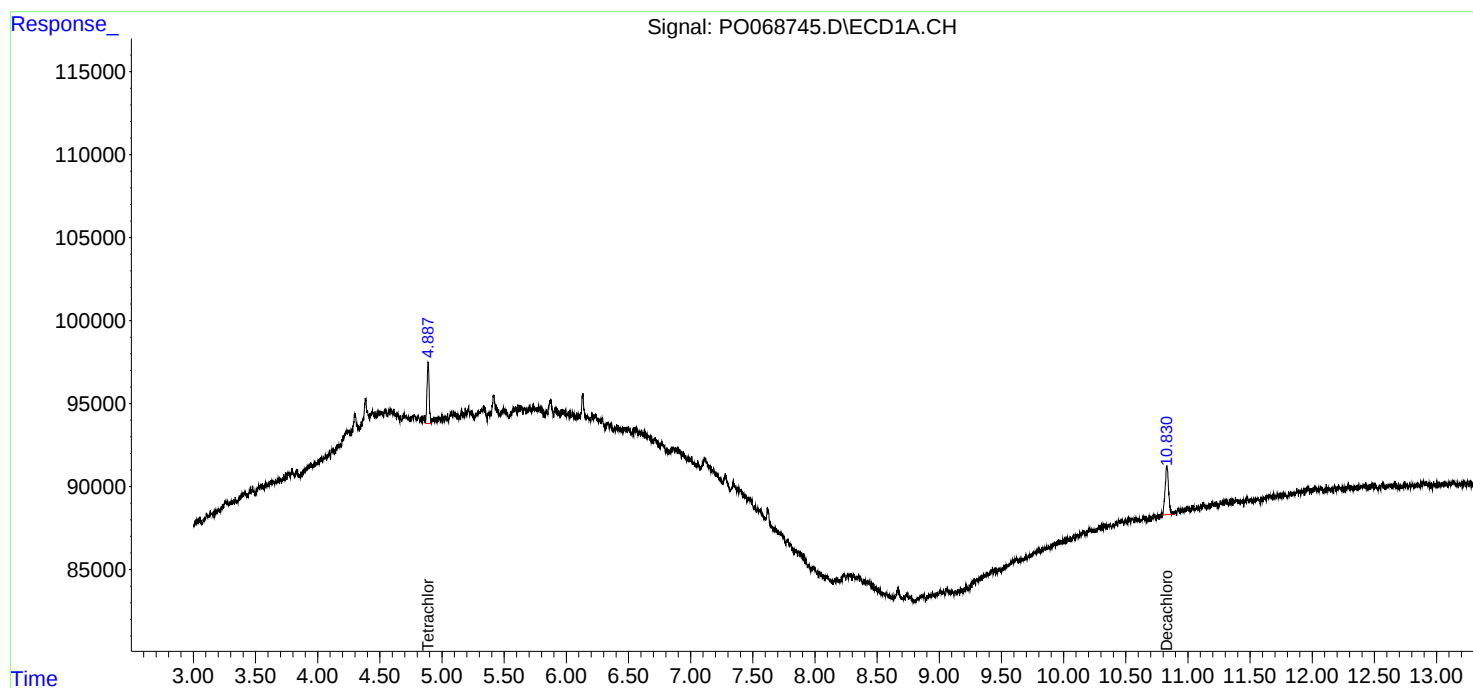

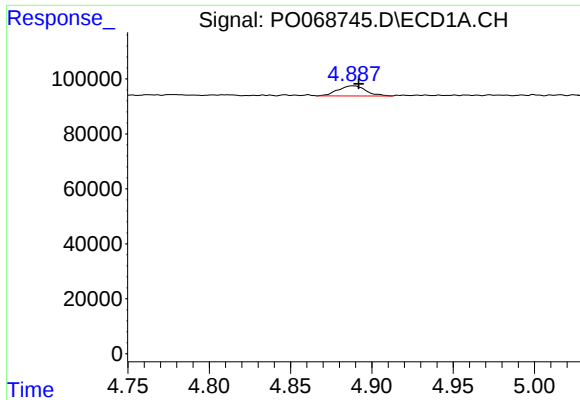


#1 Tetrachloro-m-xylene

R.T.: 4.887 min
Delta R.T.: -0.005 min
Response: 44047
Conc: 1.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-02


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:04 AM

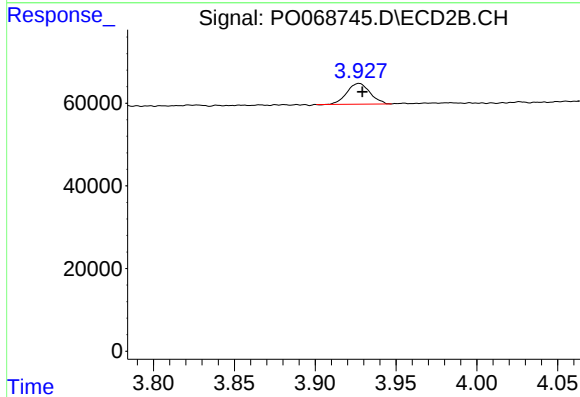


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 49841
Conc: 1.35 ng/ml

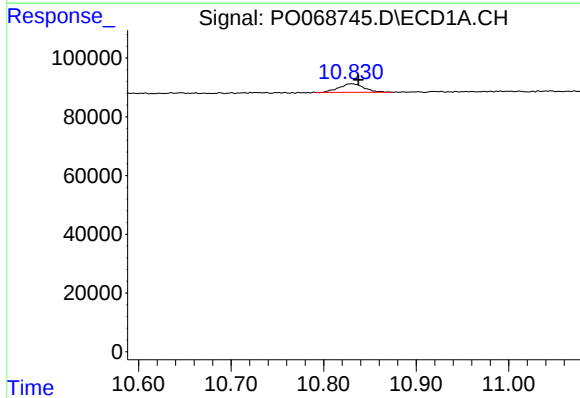

#2 Decachlorobiphenyl

R.T.: 10.830 min
Delta R.T.: -0.007 min
Response: 55377
Conc: 1.28 ng/ml

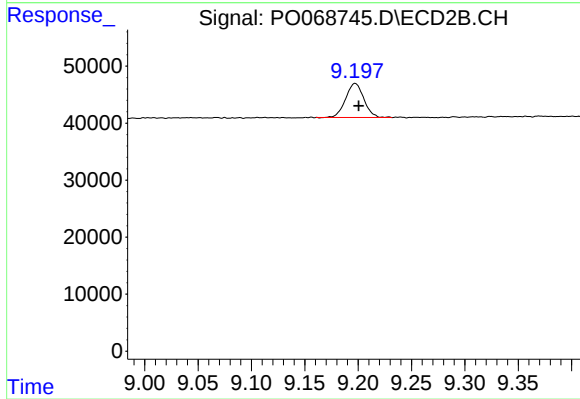

#2 Decachlorobiphenyl

R.T.: 9.197 min
Delta R.T.: -0.003 min
Response: 71163
Conc: 1.68 ng/ml