

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
 Data File : P0068746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2020 21:45
 Operator : DD\AJ
 Sample : L2827-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-052620-SR-03

Manual Integrations
 APPROVED

Sohil
 6/3/2020 9:25:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 04:13:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 29 02:25:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.887	3.926	66615	86063	2.149	2.330
2) SA Decachlor...	10.830	9.196	101048	139716	2.343	3.290m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060120\
Data File : P0068746.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2020 21:45
Operator : DD\AJ
Sample : L2827-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-03


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 04:13:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 29 02:25:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

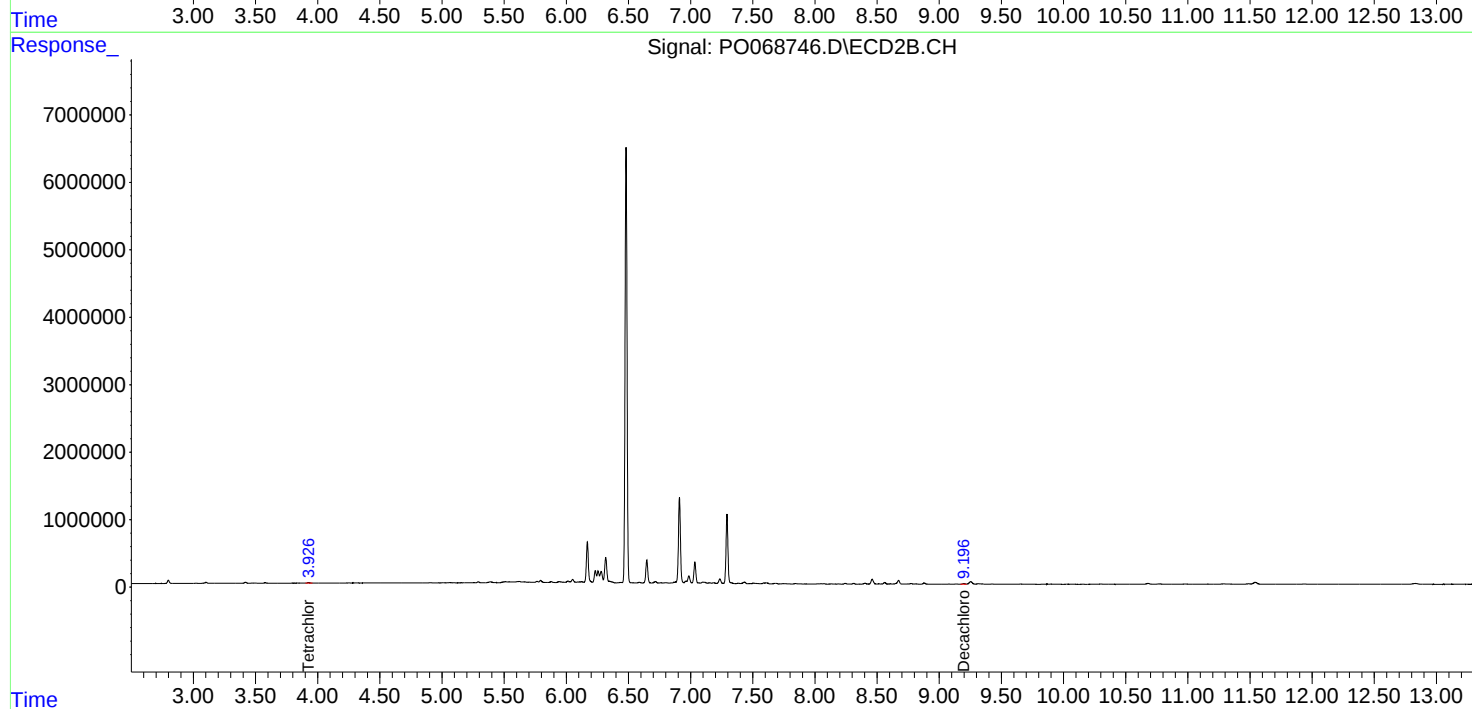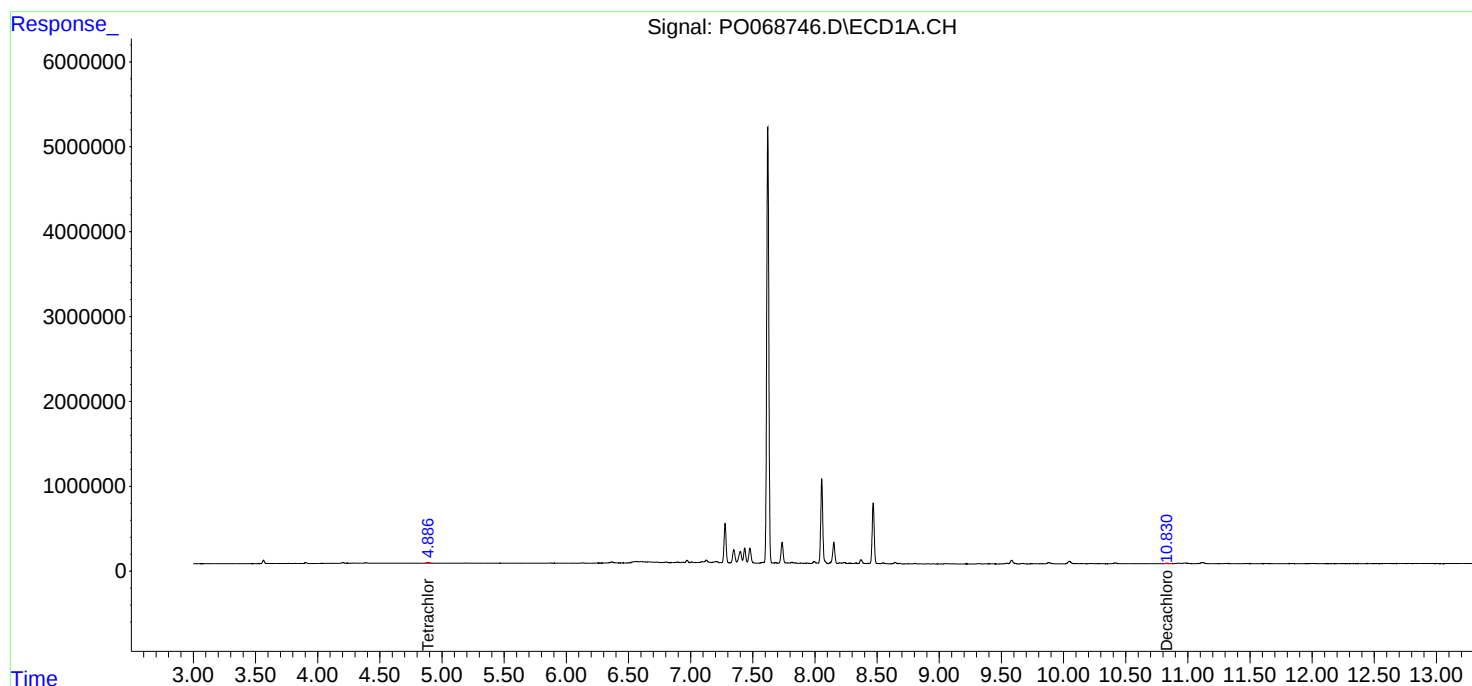

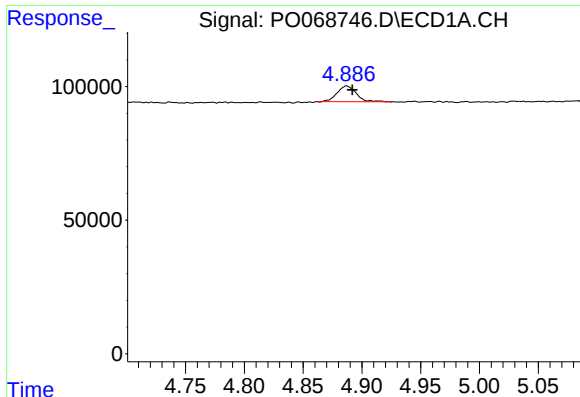


#1 Tetrachloro-m-xylene

R.T.: 4.887 min
Delta R.T.: -0.005 min
Response: 66615
Conc: 2.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-052620-SR-03


Manual Integrations
APPROVED

Sohil
6/3/2020 9:25:06 AM

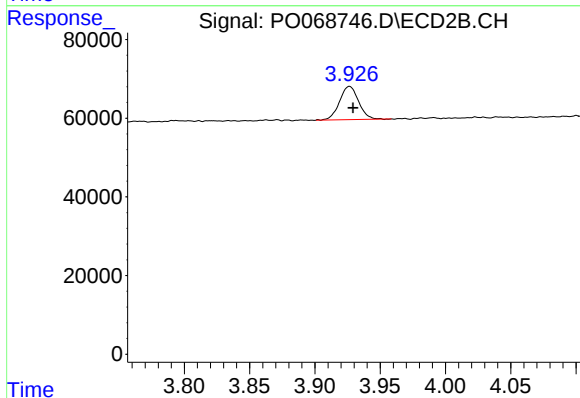


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 86063
Conc: 2.33 ng/ml

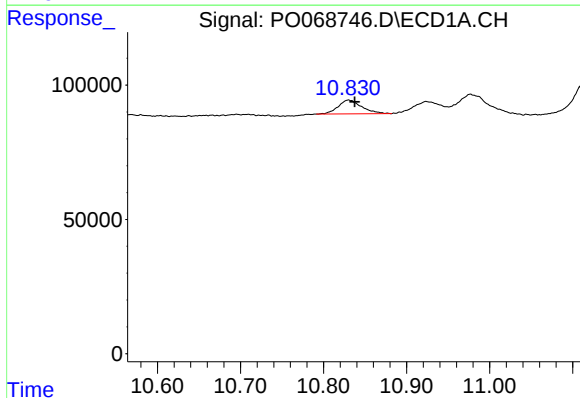

#2 Decachlorobiphenyl

R.T.: 10.830 min
Delta R.T.: -0.008 min
Response: 101048
Conc: 2.34 ng/ml

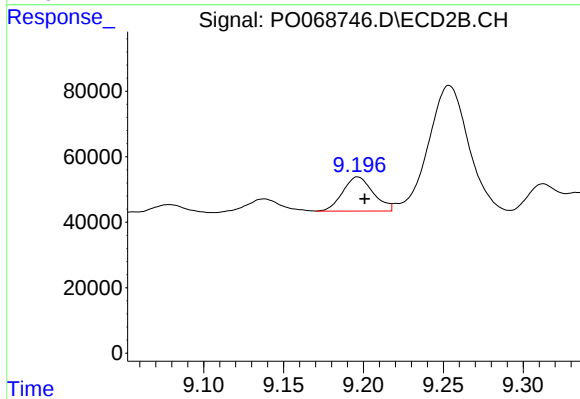

#2 Decachlorobiphenyl

R.T.: 9.196 min
Delta R.T.: -0.005 min
Response: 139716
Conc: 3.29 ng/ml m