

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060318\
Data File : P0045362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2018 17:27
Operator : SM/UA
Sample : J3171-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
052418-SIDI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:33:06 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.274	4102586	5407779	19.641	19.502
2) SA Decachlor...	9.280	7.996	4587275	5725956	19.973	20.316

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060318\
Data File : P0045362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2018 17:27
Operator : SM/UA
Sample : J3171-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
052418-SIDI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:33:06 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

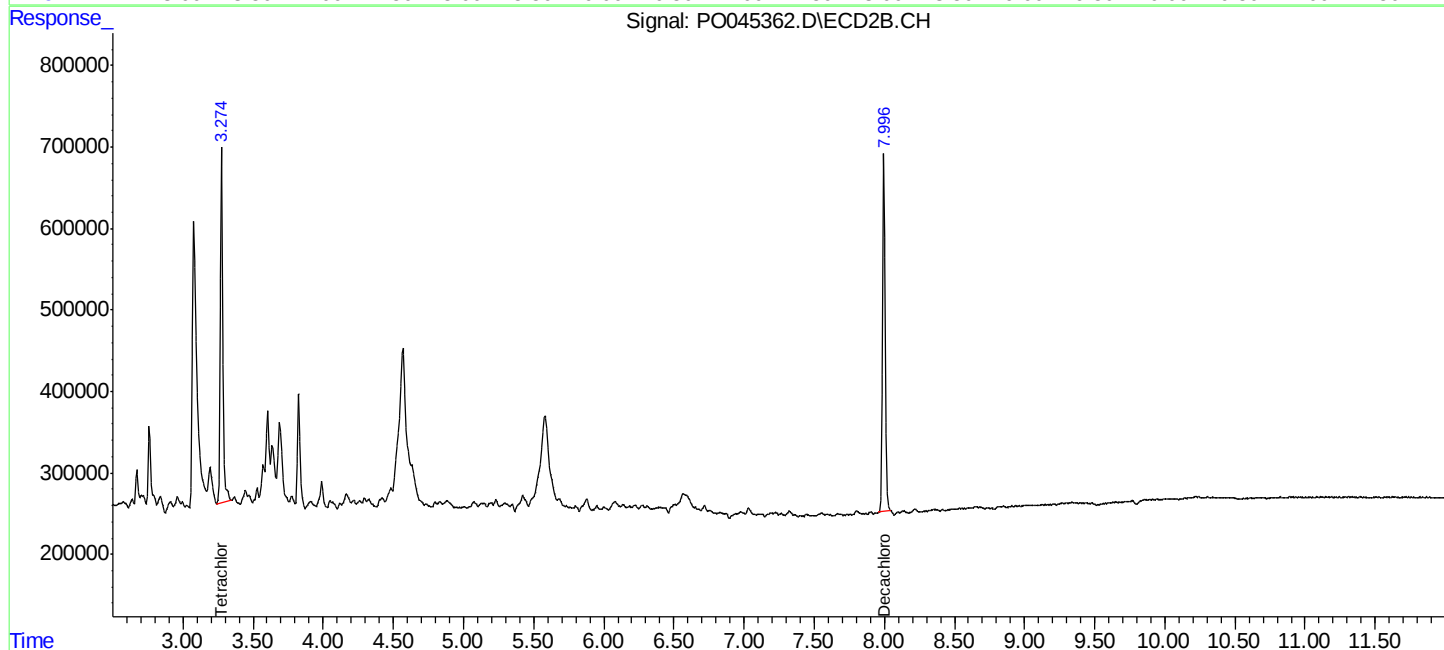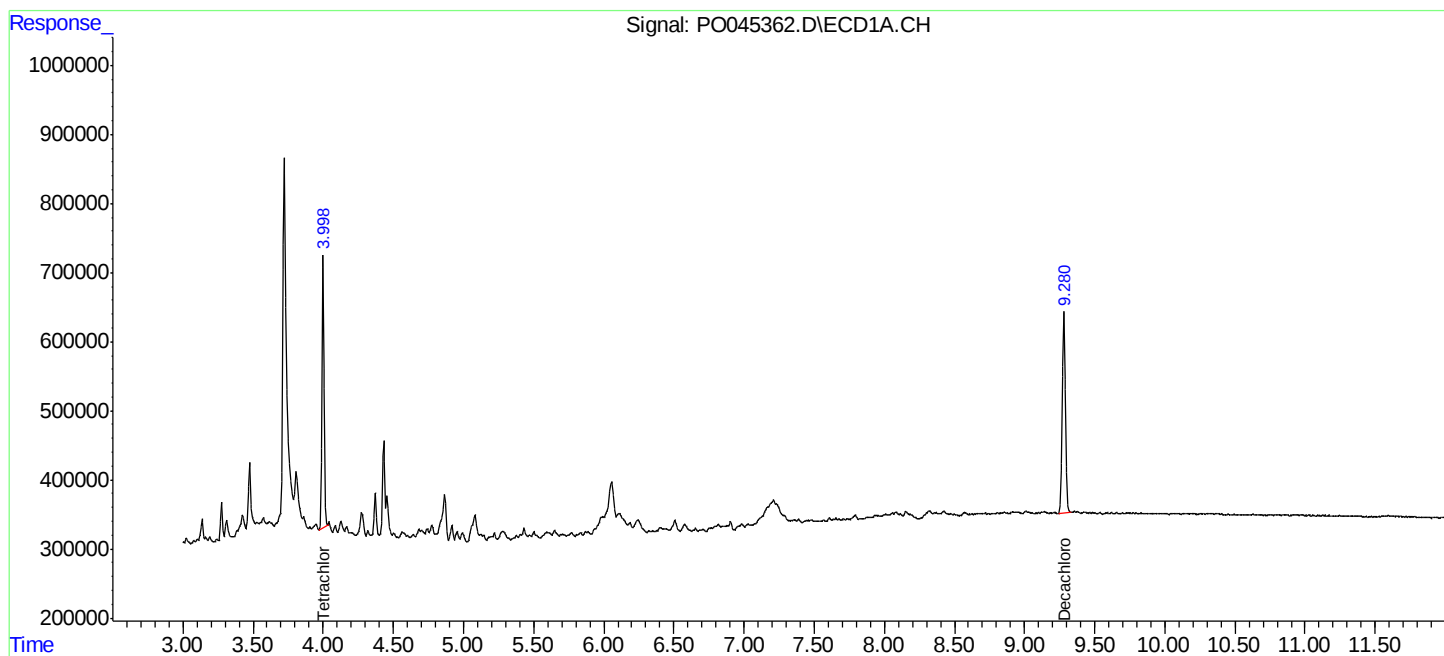


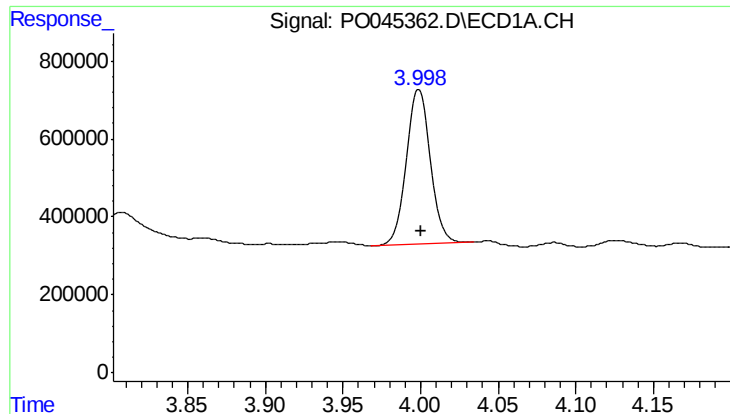

#1 Tetrachloro-m-xylene


R.T.: 3.999 min
Delta R.T.: -0.001 min
Response: 4102586
Conc: 19.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
052418-SIDI-E-D-S

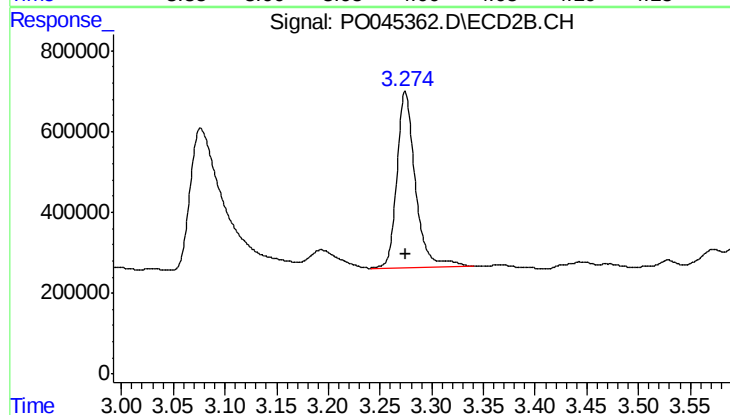


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 5407779
Conc: 19.50 ng/ml

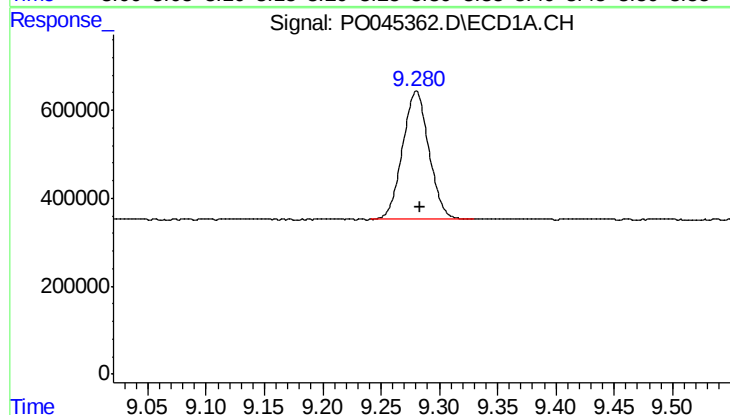

#2 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: -0.003 min
Response: 4587275
Conc: 19.97 ng/ml

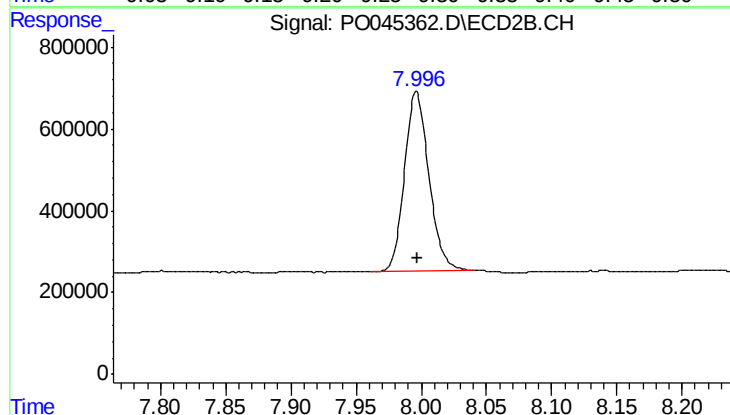

#2 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: -0.001 min
Response: 5725956
Conc: 20.32 ng/ml