

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
 Data File : P0056754.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2019 9:13
 Operator : SM/SJ
 Sample : K3104-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIT-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 09:27:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.251	3.570	834171	596016	21.789	18.073
2) SA Decachlor...	9.827	8.504	890403	541754	18.140	15.194
Target Compounds						
32) L7 AR-1260-2	0.000	6.287	0	19376	N.D.	7.861 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
Data File : P0056754.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2019 9:13
Operator : SM/SJ
Sample : K3104-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIT-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 09:27:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

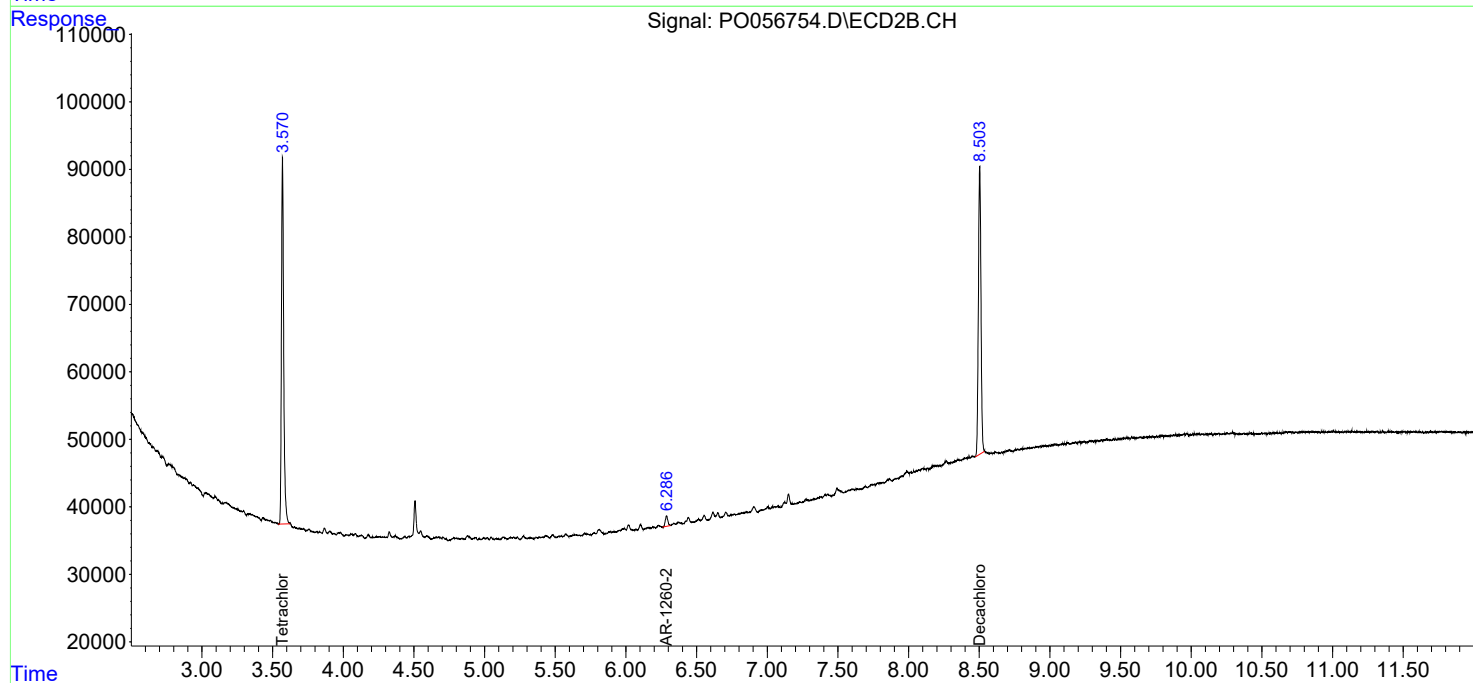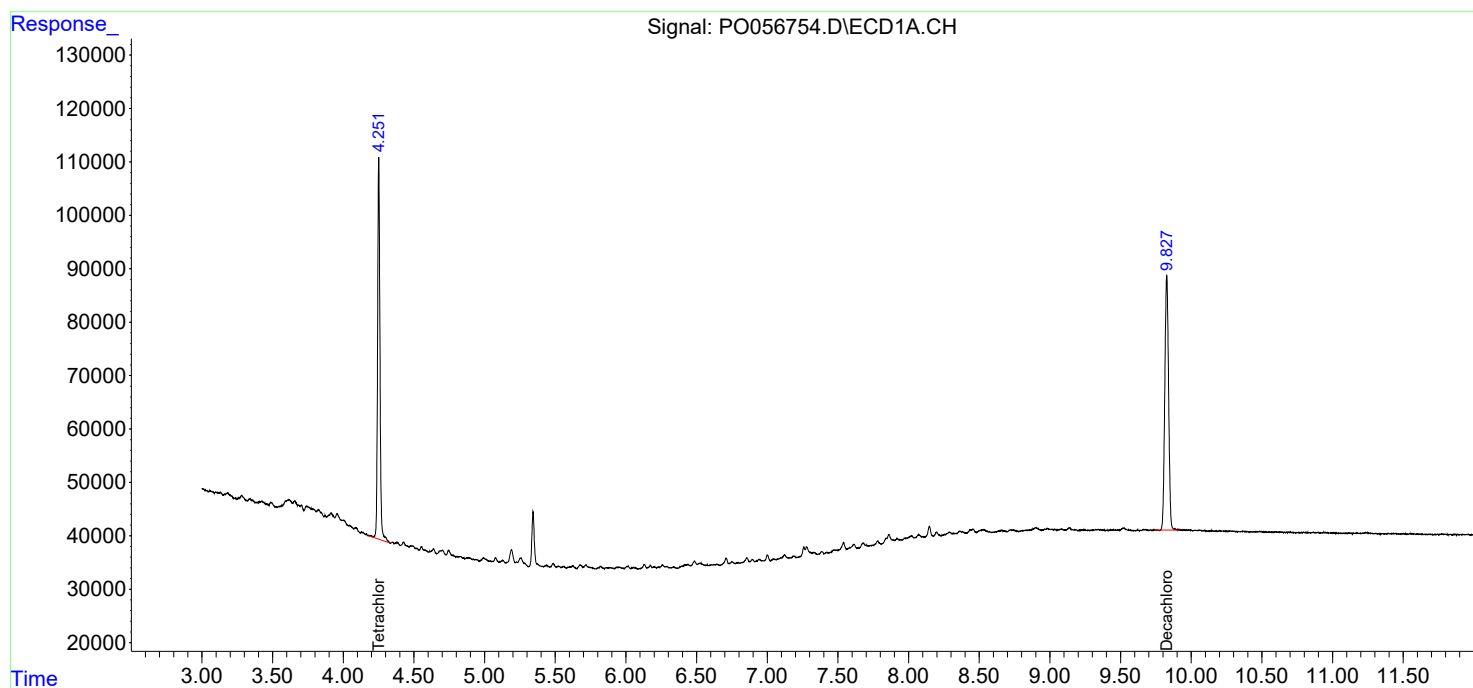


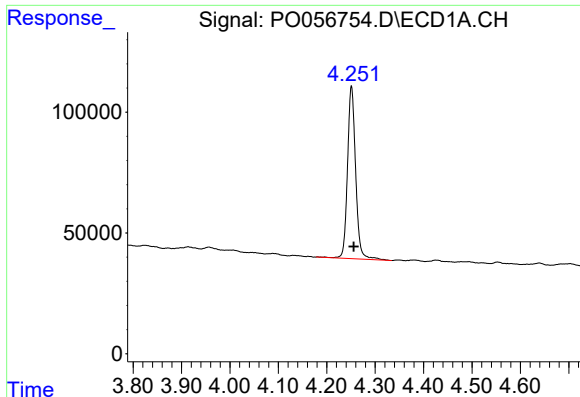

#1 Tetrachloro-m-xylene


R.T.: 4.251 min
Delta R.T.: -0.005 min
Response: 834171
Conc: 21.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIT-WATER

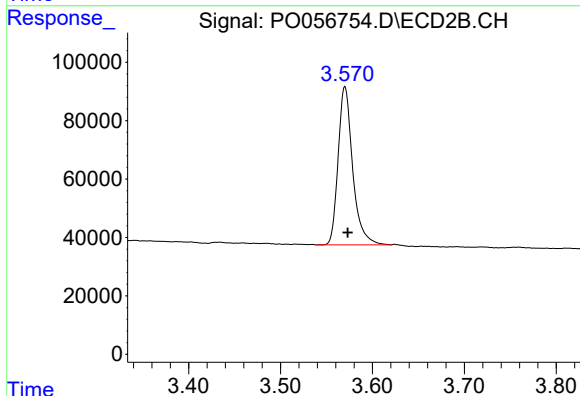


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: -0.003 min
Response: 596016
Conc: 18.07 ng/ml

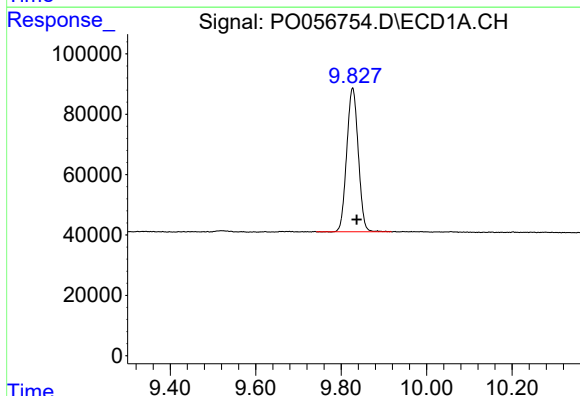


#2 Decachlorobiphenyl

R.T.: 9.827 min
Delta R.T.: -0.009 min
Response: 890403
Conc: 18.14 ng/ml

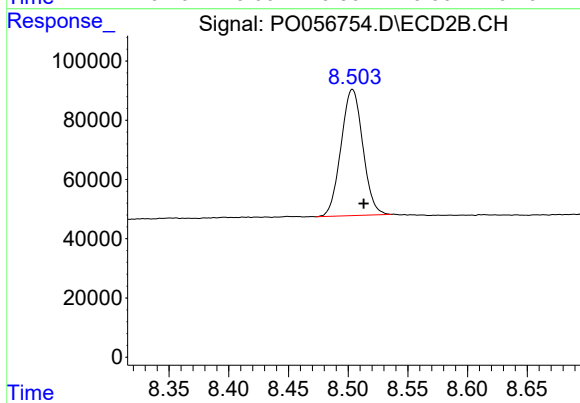

#2 Decachlorobiphenyl


R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 541754
Conc: 15.19 ng/ml

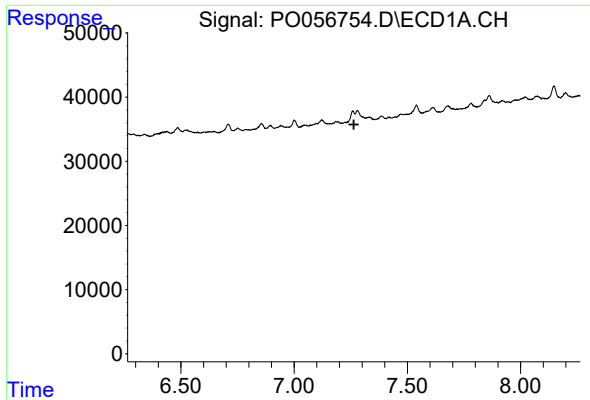

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PIT-WATER

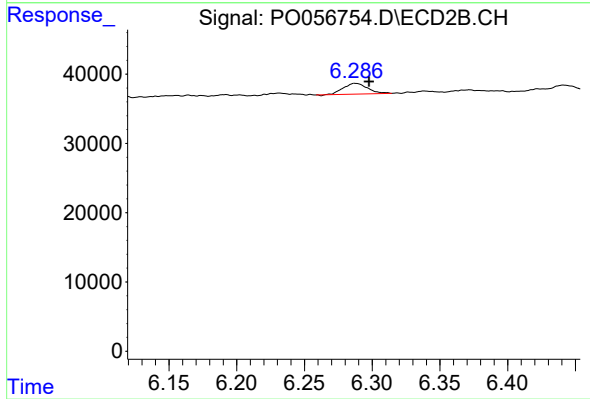

#32 AR-1260-2

R.T.: 6.287 min
Delta R.T.: -0.010 min
Response: 19376
Conc: 7.86 ng/ml