

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
 Data File : P0056809.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 00:50
 Operator : SM/SJ
 Sample : K3097-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0440-PR-3(PASSAIC)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 07:04:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.249	3.567	768613	627048	20.077	19.014
2) SA Decachlor...	9.821	8.501	653309	418575	13.310	11.739

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
Data File : P0056809.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 00:50
Operator : SM/SJ
Sample : K3097-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0440-PR-3(PASSAIC)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:04:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

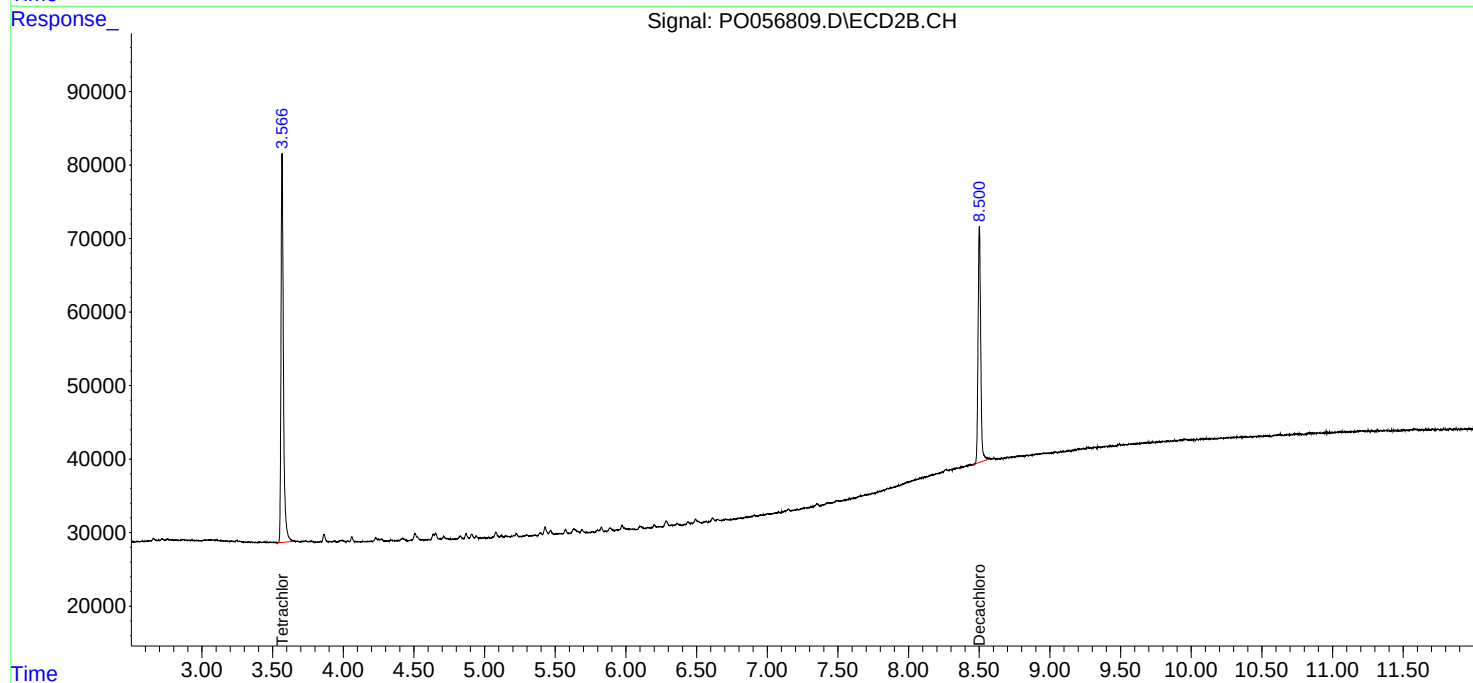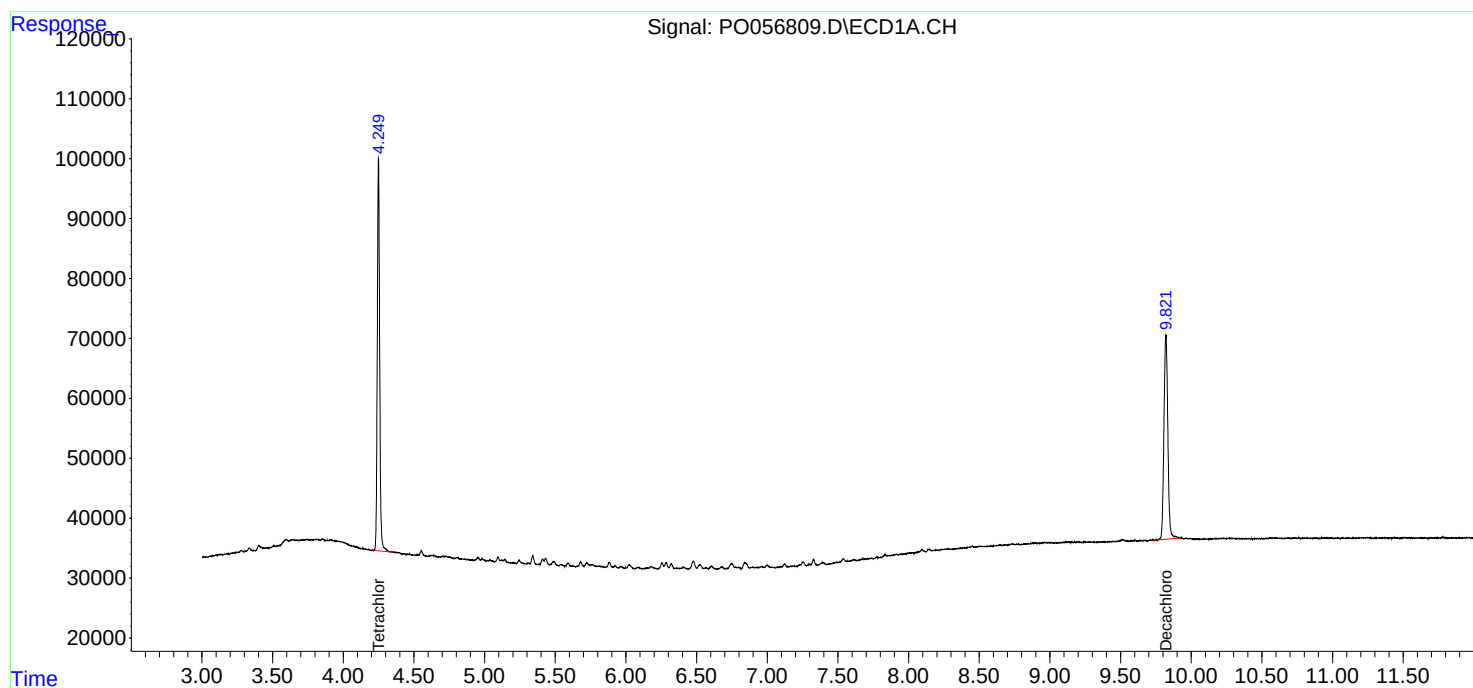


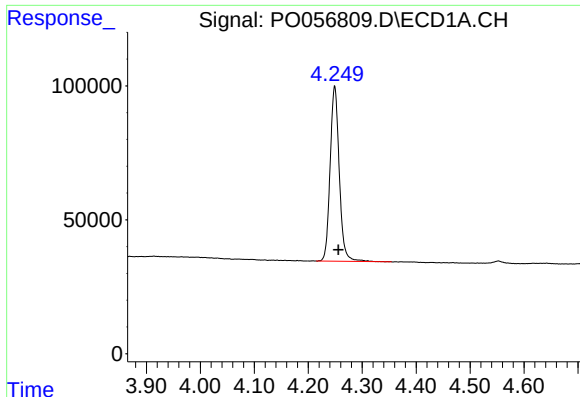

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.007 min
Response: 768613
Conc: 20.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
0440-PR-3(PASSAIC)

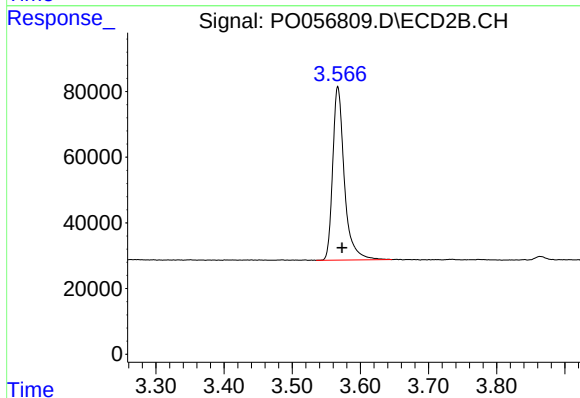


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.006 min
Response: 627048
Conc: 19.01 ng/ml

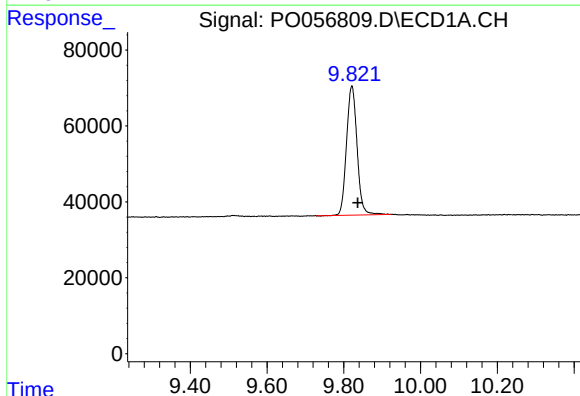

#2 Decachlorobiphenyl

R.T.: 9.821 min
Delta R.T.: -0.015 min
Response: 653309
Conc: 13.31 ng/ml

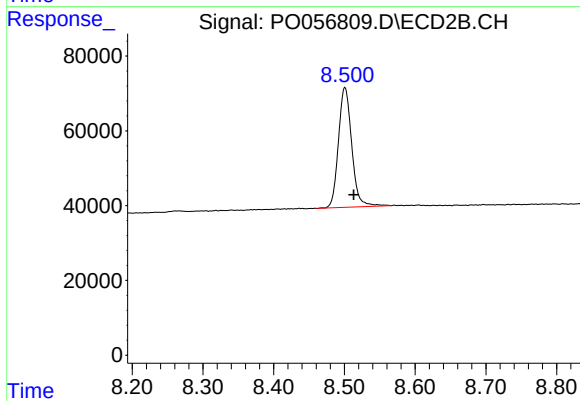

#2 Decachlorobiphenyl

R.T.: 8.501 min
Delta R.T.: -0.012 min
Response: 418575
Conc: 11.74 ng/ml