

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
 Data File : P0056785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2019 18:04
 Operator : SM/SJ
 Sample : K3097-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0422-HR-2(HACKENSACK)

Manual Integrations
 APPROVED

Ankita
 6/4/2019 4:05:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:51:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.248	3.568	729577	634136	19.057m	19.229
2) SA Decachlor...	9.823	8.501	994464	584513	20.261	16.393

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060319\
Data File : P0056785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2019 18:04
Operator : SM/SJ
Sample : K3097-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0422-HR-2(HACKENSACK)


Manual Integrations
APPROVED

Ankita
6/4/2019 4:05:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:51:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

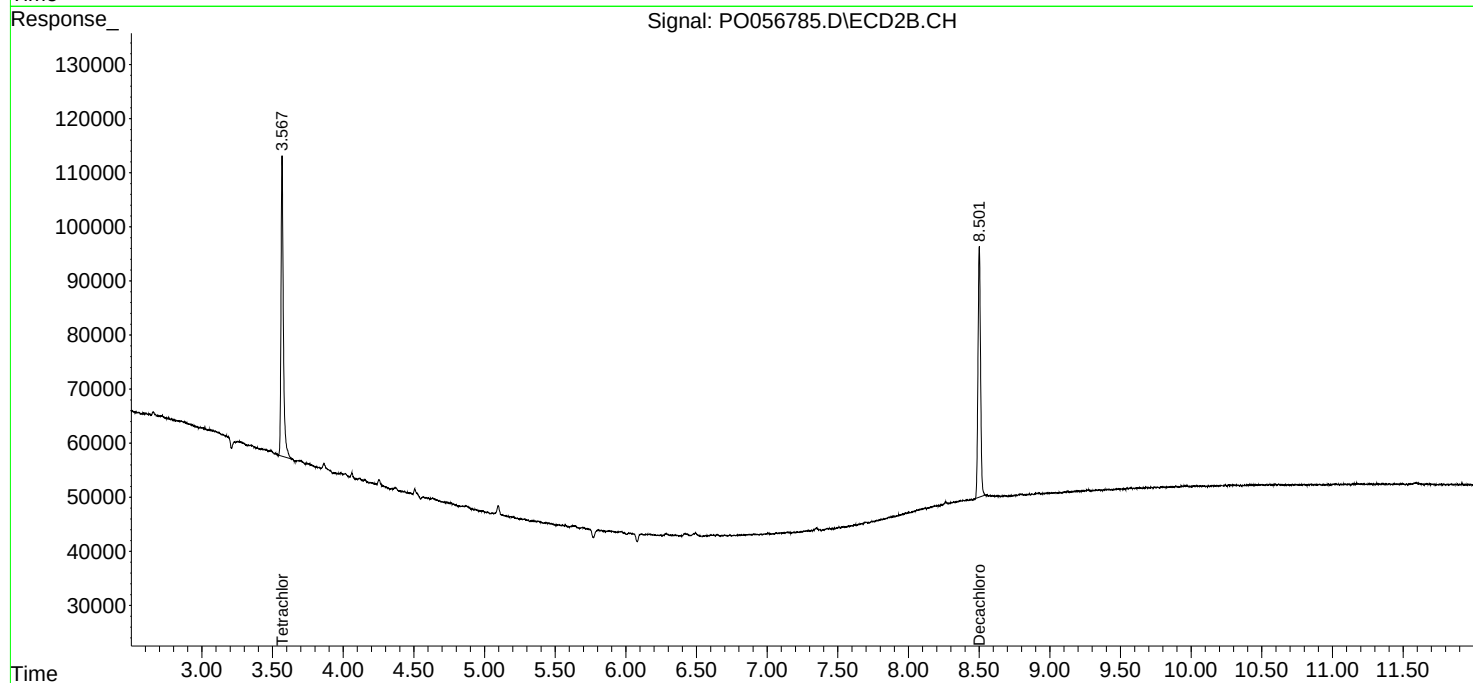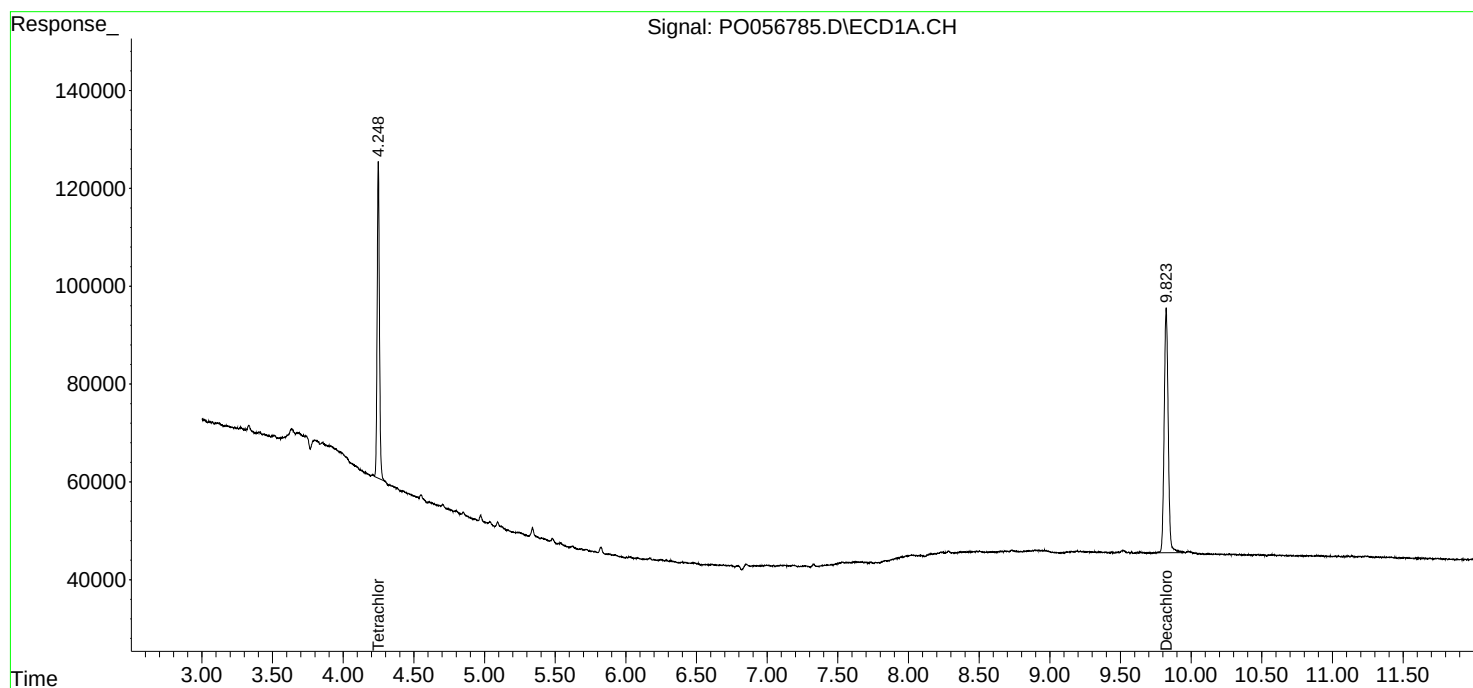

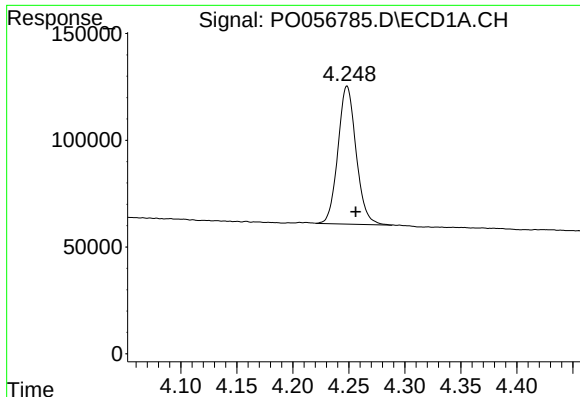


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.008 min
Response: 729577
Conc: 19.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0422-HR-2(HACKENSACK)


Manual Integrations
APPROVED

Ankita
6/4/2019 4:05:43 PM

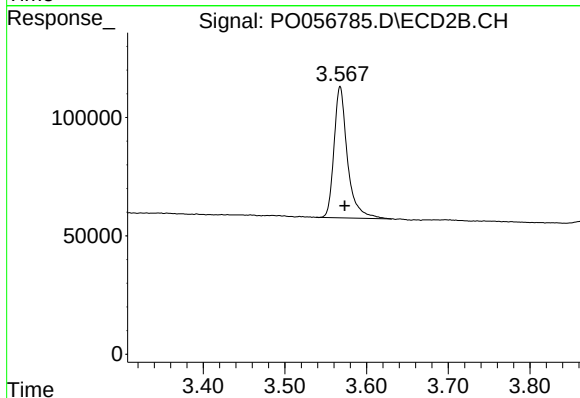


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.005 min
Response: 634136
Conc: 19.23 ng/ml

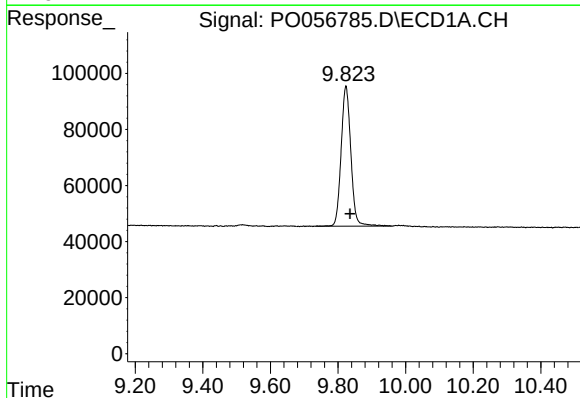

#2 Decachlorobiphenyl

R.T.: 9.823 min
Delta R.T.: -0.013 min
Response: 994464
Conc: 20.26 ng/ml

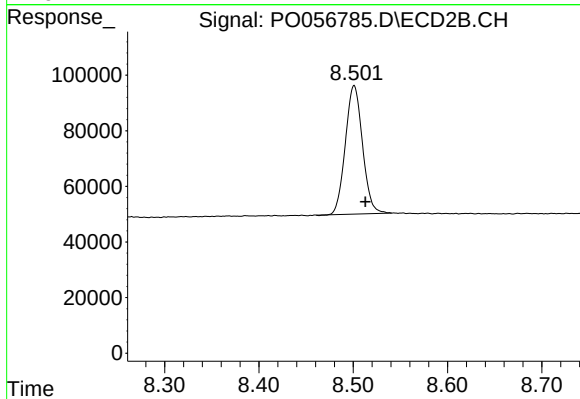

#2 Decachlorobiphenyl

R.T.: 8.501 min
Delta R.T.: -0.012 min
Response: 584513
Conc: 16.39 ng/ml