

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056834.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 16:21
 Operator : SM/SJ
 Sample : K3090-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 16:36:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.249	3.567	1175792	881565	30.713	26.732
2)	SA Decachlor...	9.821	8.500	1182703	807015	24.096	22.633
Target Compounds							
3)	L1 AR-1016-1	0.000	4.634	0	18075	N.D.	14.363 #
4)	L1 AR-1016-2	0.000	4.653	0	19688	N.D.	10.928 #
12)	L3 AR-1232-2	0.000	4.653	0	19688	N.D.	20.258 #
16)	L4 AR-1242-1	0.000	4.634	0	18075	N.D.	14.593 #
17)	L4 AR-1242-2	0.000	4.653	0	19688	N.D.	10.948 #
21)	L5 AR-1248-1	0.000	4.634	0	18075	N.D.	19.300 #
35)	L7 AR-1260-5	8.095	0.000	129070	0	26.990	N.D. #
37)	L8 AR-1262-2	8.095	0.000	129070	0	16.930	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056834.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 16:21
Operator : SM/SJ
Sample : K3090-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-4-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 16:36:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

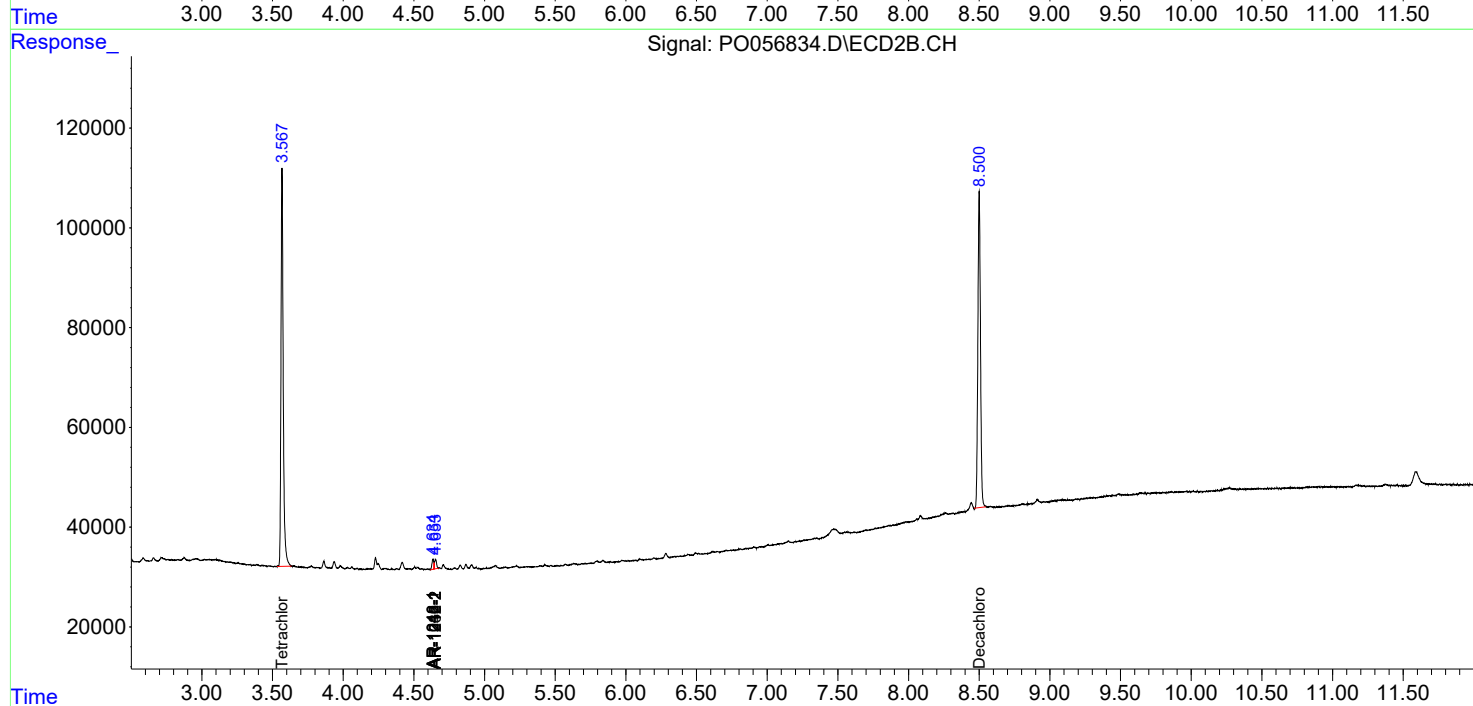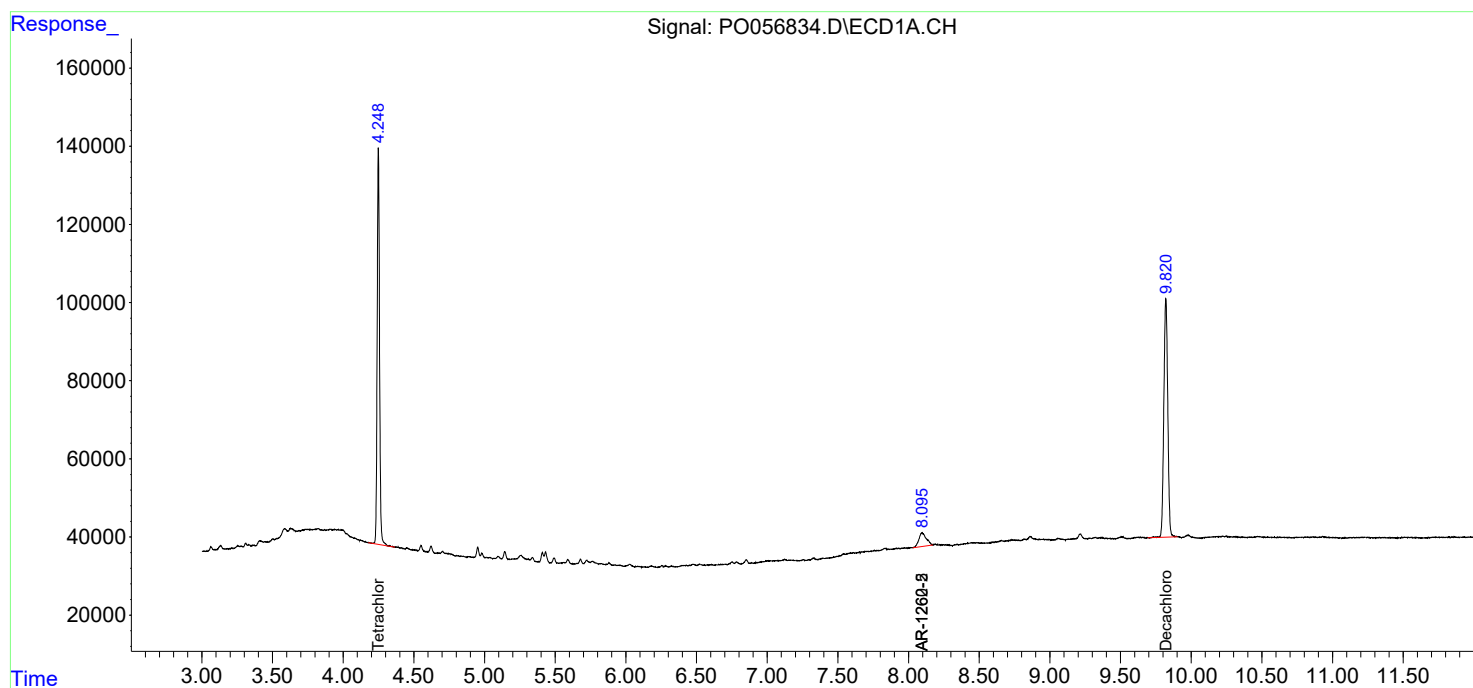


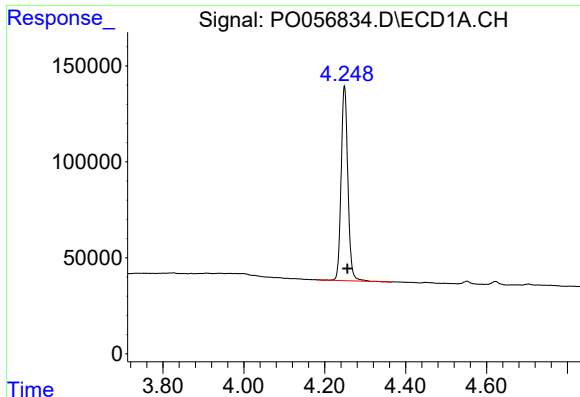

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.007 min
Response: 1175792
Conc: 30.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-S

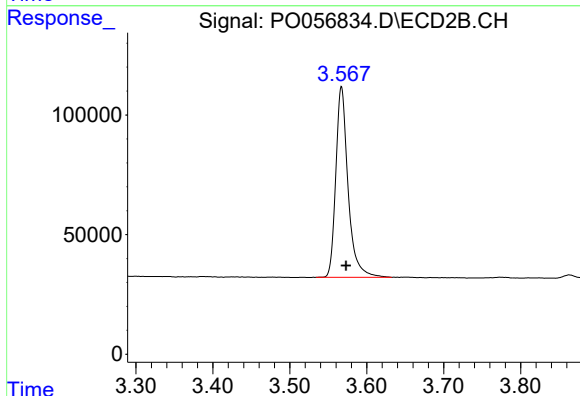


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.006 min
Response: 881565
Conc: 26.73 ng/ml

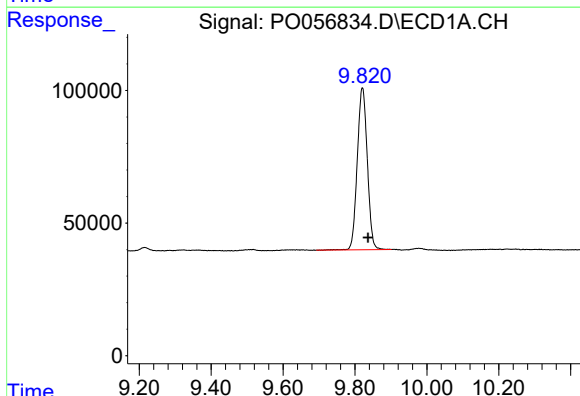


#2 Decachlorobiphenyl

R.T.: 9.821 min
Delta R.T.: -0.016 min
Response: 1182703
Conc: 24.10 ng/ml

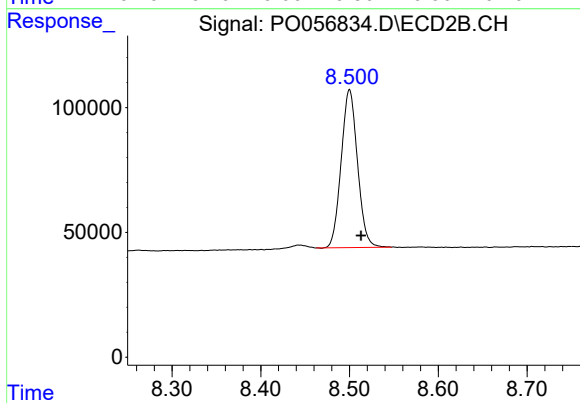

#2 Decachlorobiphenyl


R.T.: 8.500 min
Delta R.T.: -0.013 min
Response: 807015
Conc: 22.63 ng/ml

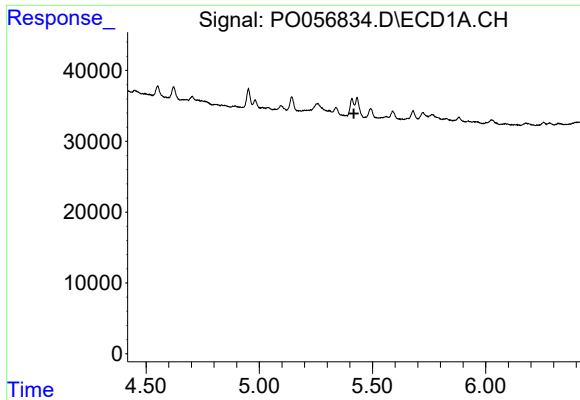

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4-S

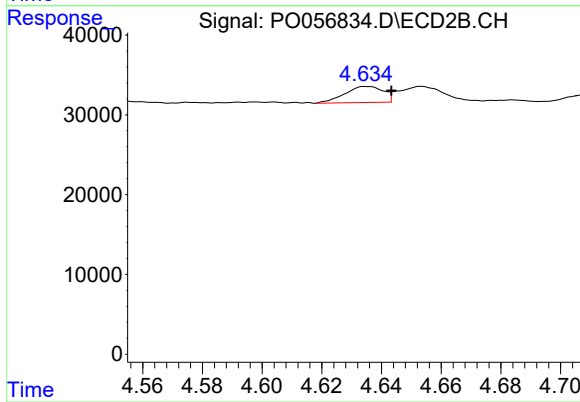


#3 AR-1016-1

R.T.: 4.634 min
Delta R.T.: -0.009 min
Response: 18075
Conc: 14.36 ng/ml

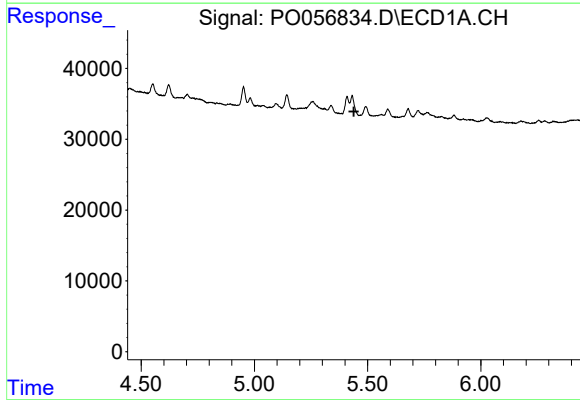


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

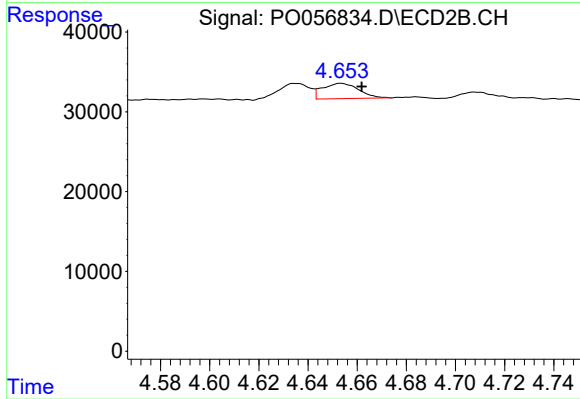

#4 AR-1016-2

R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 19688
Conc: 10.93 ng/ml

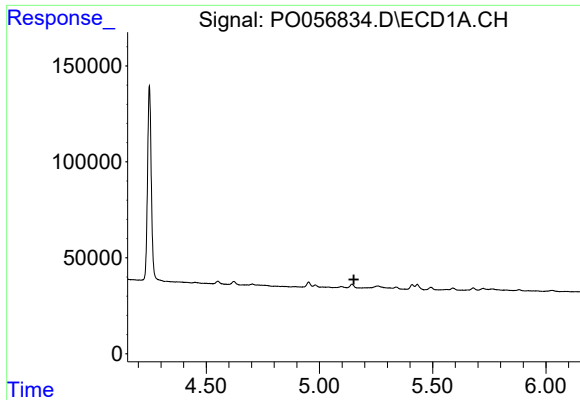

#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4-S

#12 AR-1232-2


R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 19688
Conc: 20.26 ng/ml

#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

#16 AR-1242-1


R.T.: 4.634 min
Delta R.T.: -0.008 min
Response: 18075
Conc: 14.59 ng/ml

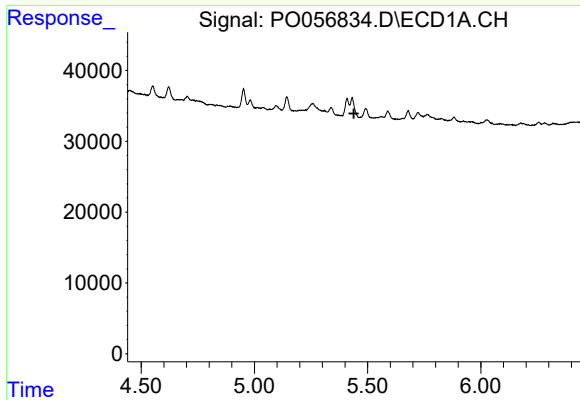

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4-S

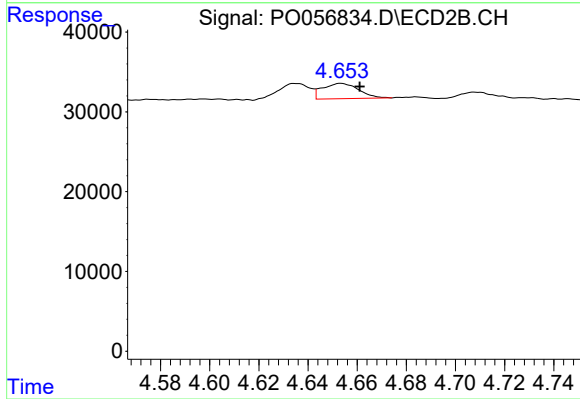


#17 AR-1242-2

R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 19688
Conc: 10.95 ng/ml

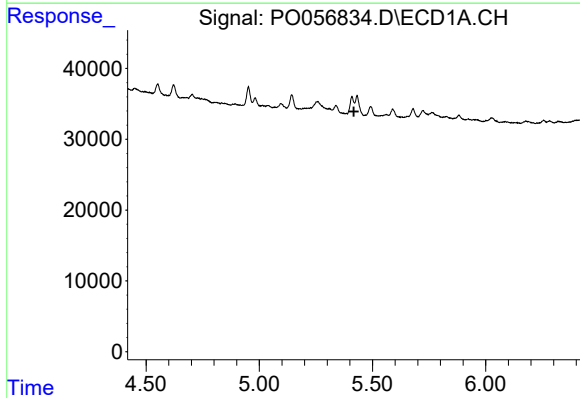


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

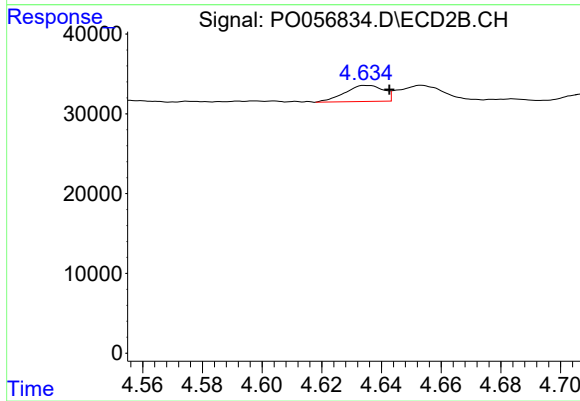

#21 AR-1248-1


R.T.: 4.634 min
Delta R.T.: -0.008 min
Response: 18075
Conc: 19.30 ng/ml

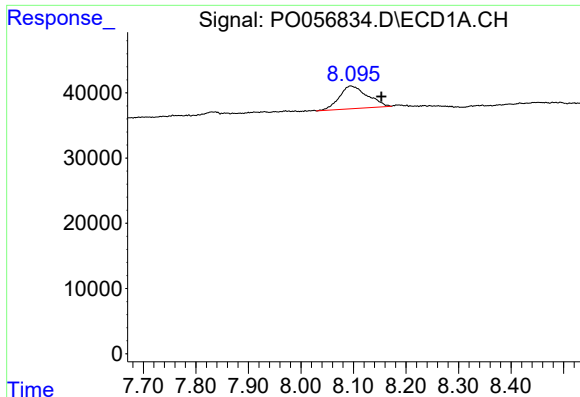

#35 AR-1260-5


R.T.: 8.095 min
Delta R.T.: -0.058 min
Response: 129070
Conc: 26.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-S

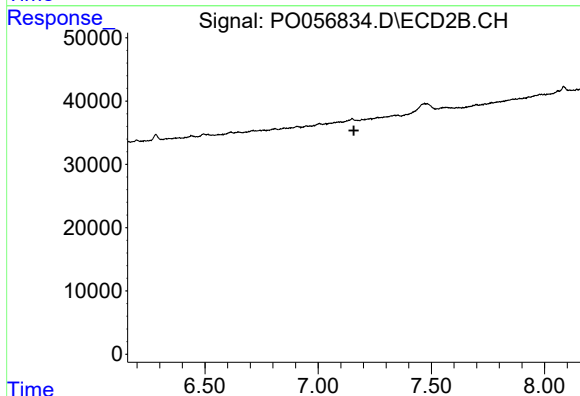


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

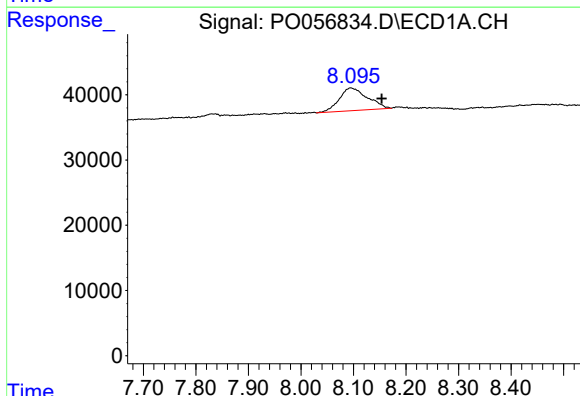

#37 AR-1262-2

R.T.: 8.095 min
Delta R.T.: -0.059 min
Response: 129070
Conc: 16.93 ng/ml

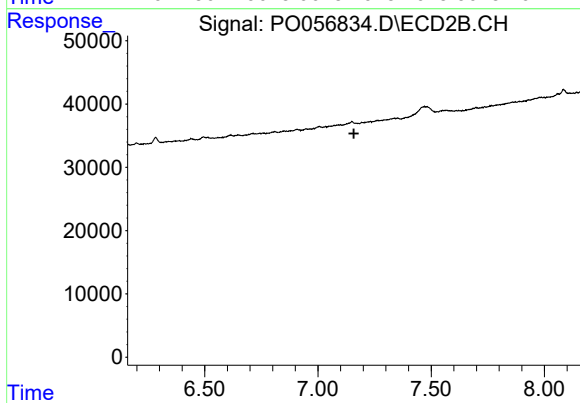

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.