

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056855.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 22:19
 Operator : SM/SJ
 Sample : K3174-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-008-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:19:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.250	3.569	857804	747719	22.407	22.673
2)	SA Decachlor...	9.822	8.503	615528	409092	12.540	11.473
Target Compounds							
35)	L7 AR-1260-5	8.183	0.000	12334	0	2.579	N.D. #
37)	L8 AR-1262-2	8.183	0.000	12334	0	1.618	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056855.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 22:19
Operator : SM/SJ
Sample : K3174-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-008-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:19:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

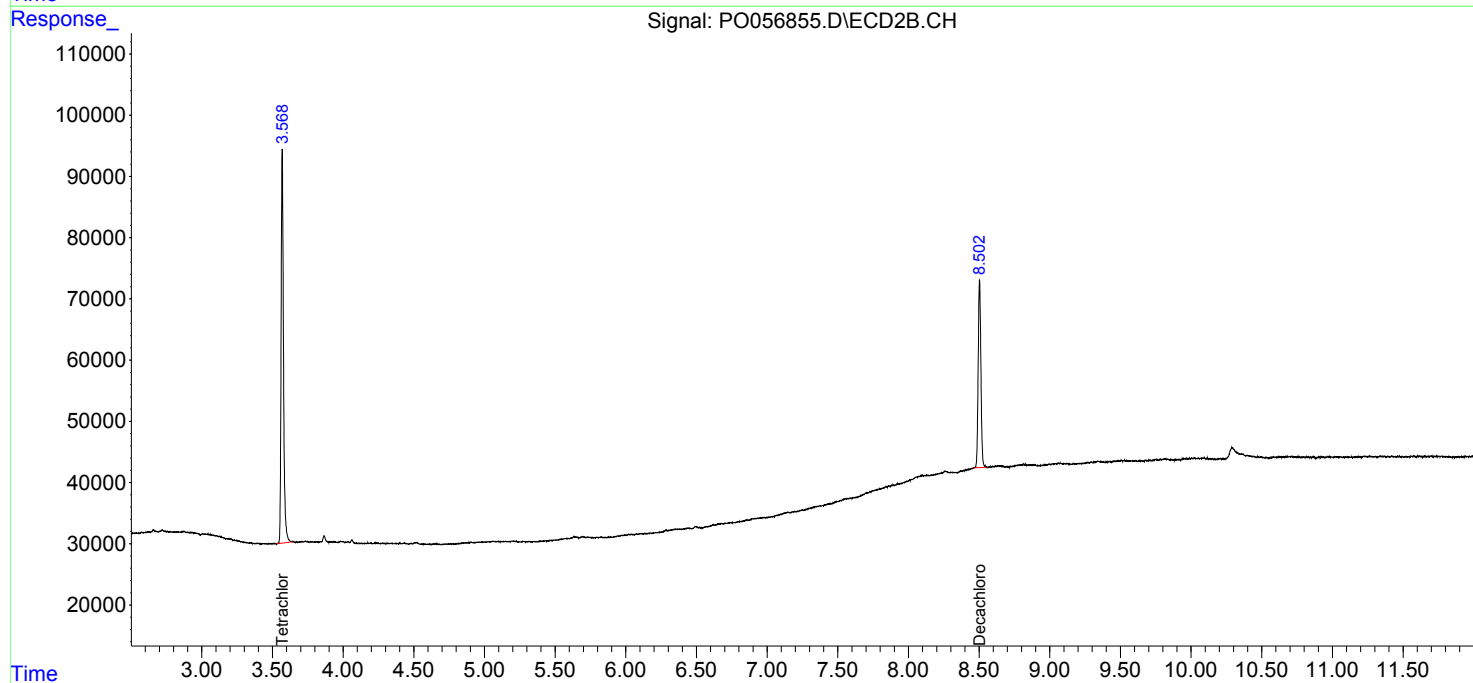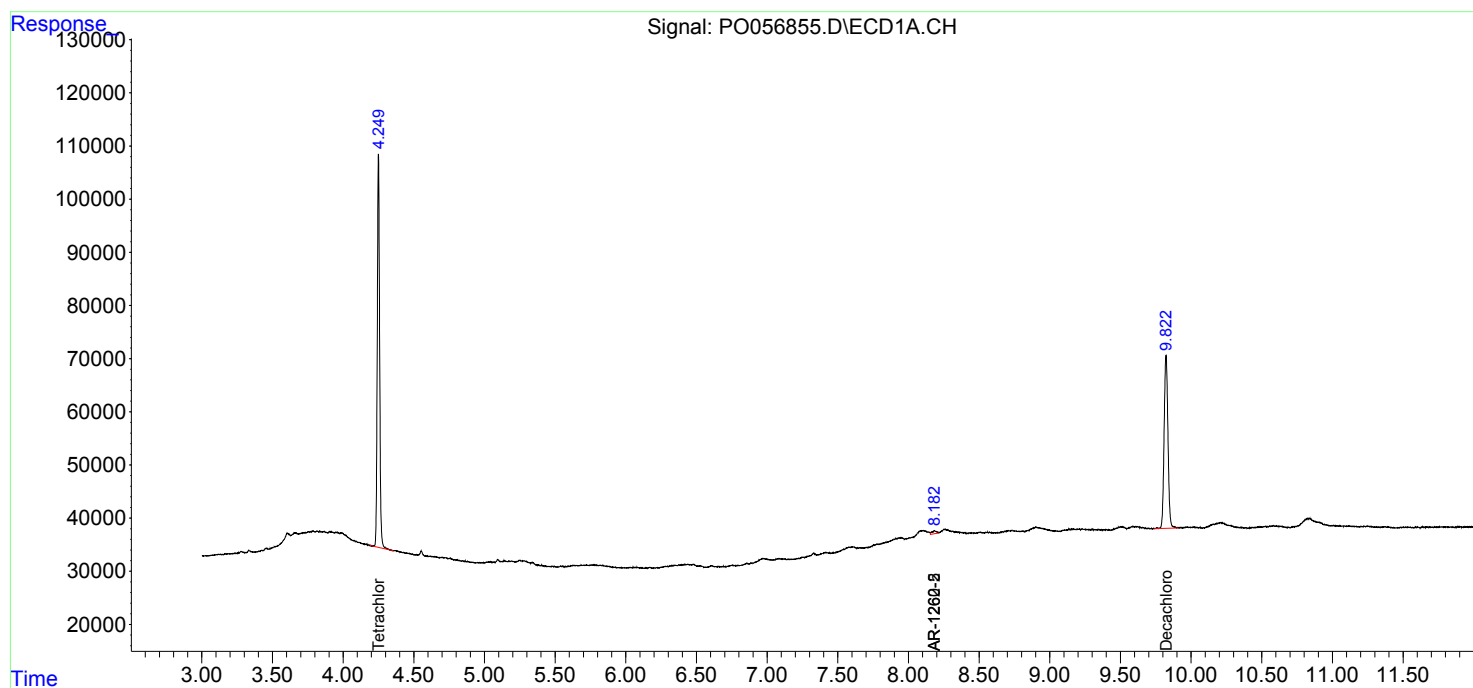


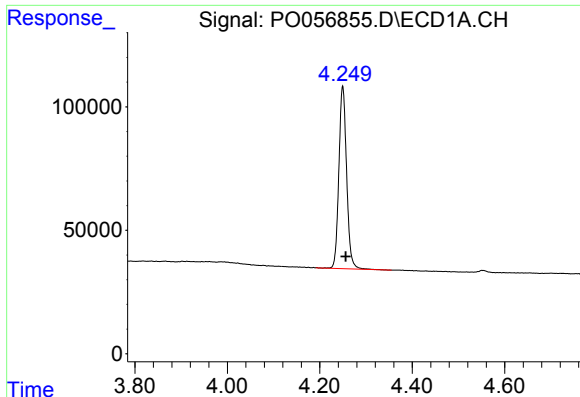

#1 Tetrachloro-m-xylene


R.T.: 4.250 min
Delta R.T.: -0.006 min
Response: 857804
Conc: 22.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-008-ABCD

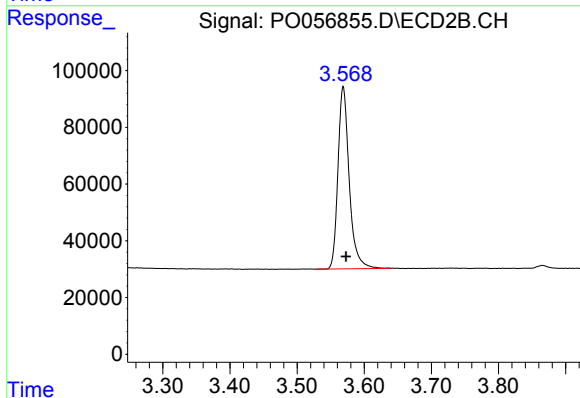


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.004 min
Response: 747719
Conc: 22.67 ng/ml

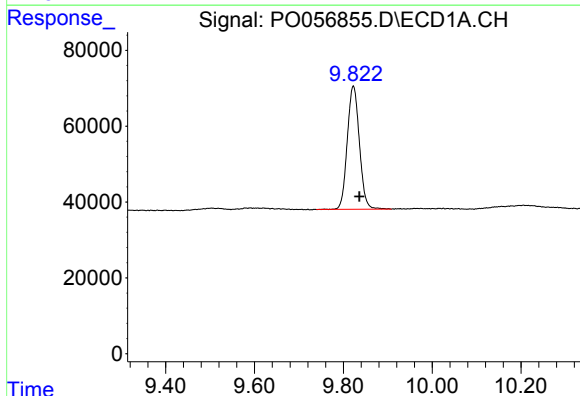


#2 Decachlorobiphenyl

R.T.: 9.822 min
Delta R.T.: -0.014 min
Response: 615528
Conc: 12.54 ng/ml

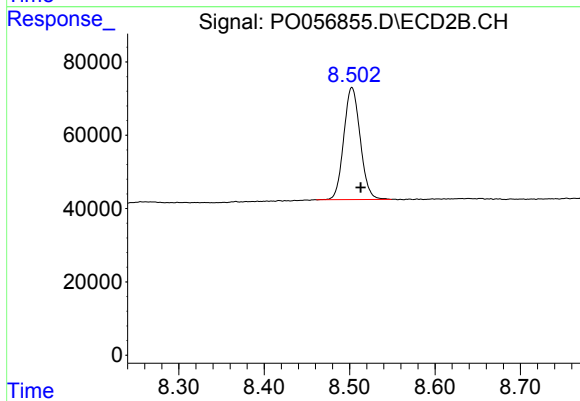

#2 Decachlorobiphenyl


R.T.: 8.503 min
Delta R.T.: -0.010 min
Response: 409092
Conc: 11.47 ng/ml

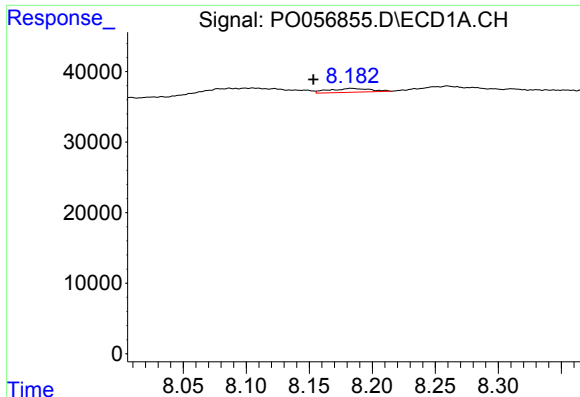

#35 AR-1260-5


R.T.: 8.183 min
Delta R.T.: 0.030 min
Response: 12334
Conc: 2.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-008-ABCD

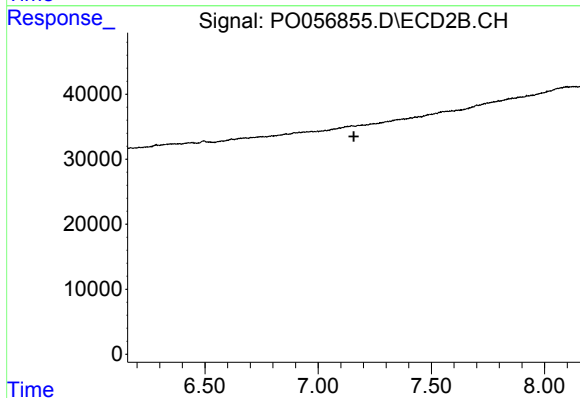


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

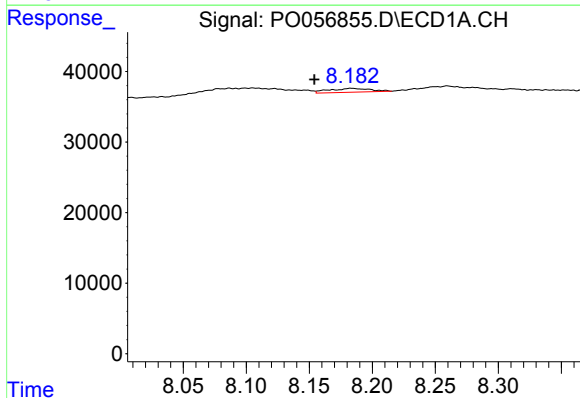

#37 AR-1262-2

R.T.: 8.183 min
Delta R.T.: 0.029 min
Response: 12334
Conc: 1.62 ng/ml

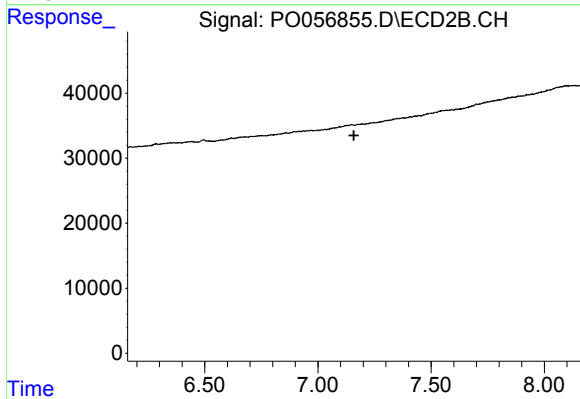

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.