

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056857.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 22:52
 Operator : SM/SJ
 Sample : K3175-01MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:20:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.249	3.569	1043162	861917	27.248	26.136
2)	SA Decachlor...	9.822	8.502	721634	491972	14.702	13.797
Target Compounds							
3)	L1 AR-1016-1	5.431	4.636	458588	155344	254.967	123.437 #
4)	L1 AR-1016-2	5.431	4.655	458588	217313	182.626	120.620 #
5)	L1 AR-1016-3	5.493	4.828	162707	113089	101.230	114.701
6)	L1 AR-1016-4	5.591	4.869	129007	91375	98.344	110.378
7)	L1 AR-1016-5	5.882	5.080	125144	93590	90.578	87.246
9)	L2 AR-1221-2	4.621	3.864	103466	28412	216.866	75.391 #
10)	L2 AR-1221-3	4.621	3.937	103466	85342	70.001	71.294
11)	L3 AR-1232-1	4.621	3.937	103466	85342	87.803	94.997
12)	L3 AR-1232-2	5.144	4.655	132461	217313	199.778	223.600
13)	L3 AR-1232-3	5.431	4.828	458588	113089	323.257	216.110 #
14)	L3 AR-1232-4	5.591	4.911	129007	109176	183.268	221.593
15)	L3 AR-1232-5	5.680	5.080	110375	93590	195.220	166.160
16)	L4 AR-1242-1	5.431	4.636	458588	155344	265.818	125.421 #
17)	L4 AR-1242-2	5.431	4.655	458588	217313	180.634	120.835 #
18)	L4 AR-1242-3	5.493	4.828	162707	113089	100.065	115.032
19)	L4 AR-1242-4	5.591	4.911	129007	109176	96.510	112.195
20)	L4 AR-1242-5	0.000	5.428	0	83610	N.D.	70.719 #
21)	L5 AR-1248-1	5.431	4.636	458588	155344	355.905	165.874 #
22)	L5 AR-1248-2	5.680	4.869	110375	91375	59.249	71.924
23)	L5 AR-1248-3	5.882	4.911	125144	109176	61.005	83.602 #
24)	L5 AR-1248-4	0.000	5.080	0	93590	N.D.	59.099 #
25)	L5 AR-1248-5	0.000	5.428	0	83610	N.D.	50.517 #
26)	L6 AR-1254-1	0.000	5.428	0	83610	N.D.	31.614 #
27)	L6 AR-1254-2	6.472	5.574	105067	78928	27.051	36.612 #
28)	L6 AR-1254-3	6.838	5.987	50613	131940	12.275	36.039 #
29)	L6 AR-1254-4	7.186	6.230	40178	45237	13.349	20.591 #
30)	L6 AR-1254-5	7.538	6.614	326426	231583	86.685	73.049
31)	L7 AR-1260-1	6.999	6.102	225357	184866	87.818	92.416
32)	L7 AR-1260-2	7.255	6.289	259845	225039	85.923	91.295
33)	L7 AR-1260-3	7.611	6.441	163225	197007	67.755	87.823 #
34)	L7 AR-1260-4	7.836	6.908	188100	134754	71.816	72.409
35)	L7 AR-1260-5	8.144	7.150	336979	315944	70.467	73.265
36)	L8 AR-1262-1	7.611	6.650	163225	164517	34.900	39.414
37)	L8 AR-1262-2	8.144	7.150	336979	315944	44.201	45.985
38)	L8 AR-1262-3	8.453	7.428	214957	68200	41.073	23.092 #
39)	L8 AR-1262-4	8.504	7.493	120139	222506	28.142	42.702 #
40)	L8 AR-1262-5	9.137	7.986	83394	57396	30.351	24.717
41)	L9 AR-1268-1	8.453	7.428	214957	68200	26.416	9.136 #
42)	L9 AR-1268-2	8.504	7.493	120139	222506	14.851	31.864 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056857.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 22:52
 Operator : SM/SJ
 Sample : K3175-01MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:20:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.137	7.986	83394	57396	30.580	24.589
45) L9	AR-1268-5	0.000	8.262	0	20674	N.D.	1.195 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056857.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 22:52
Operator : SM/SJ
Sample : K3175-01MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:20:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

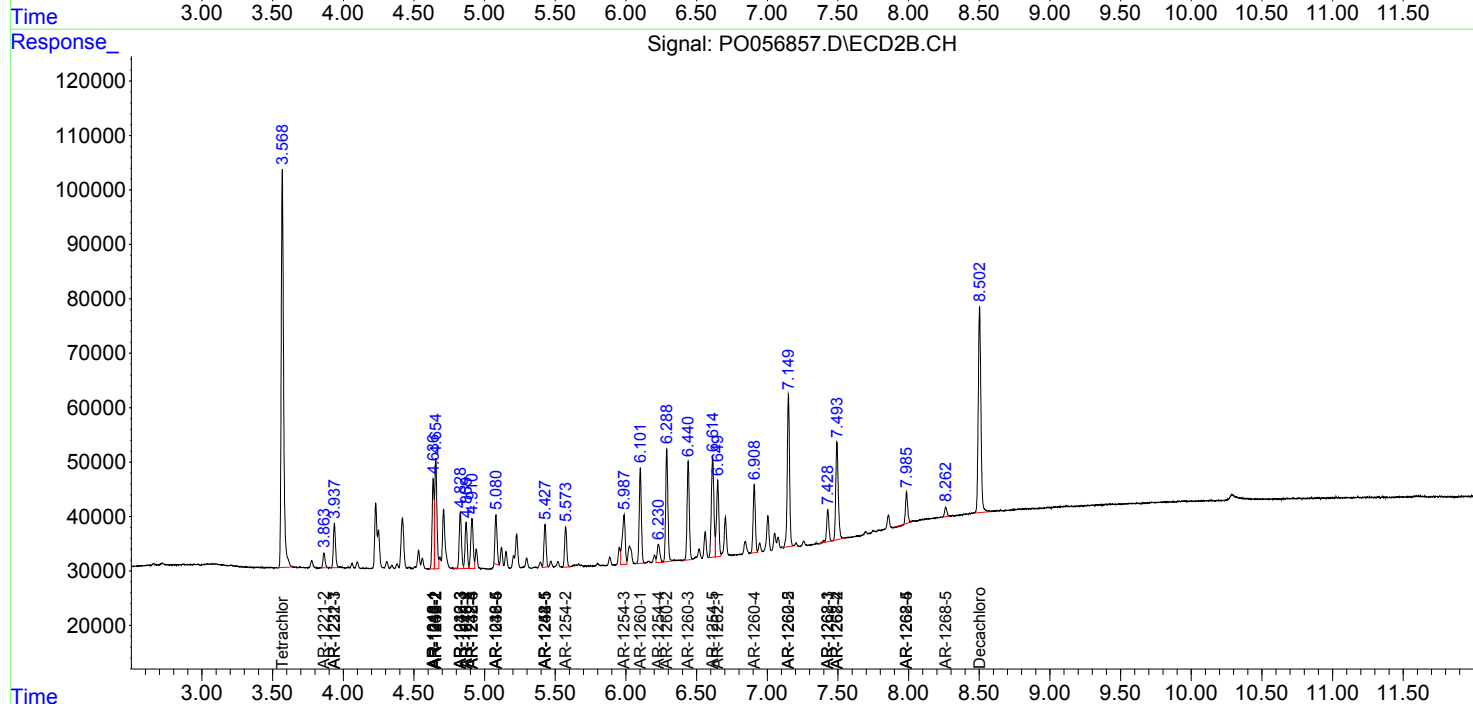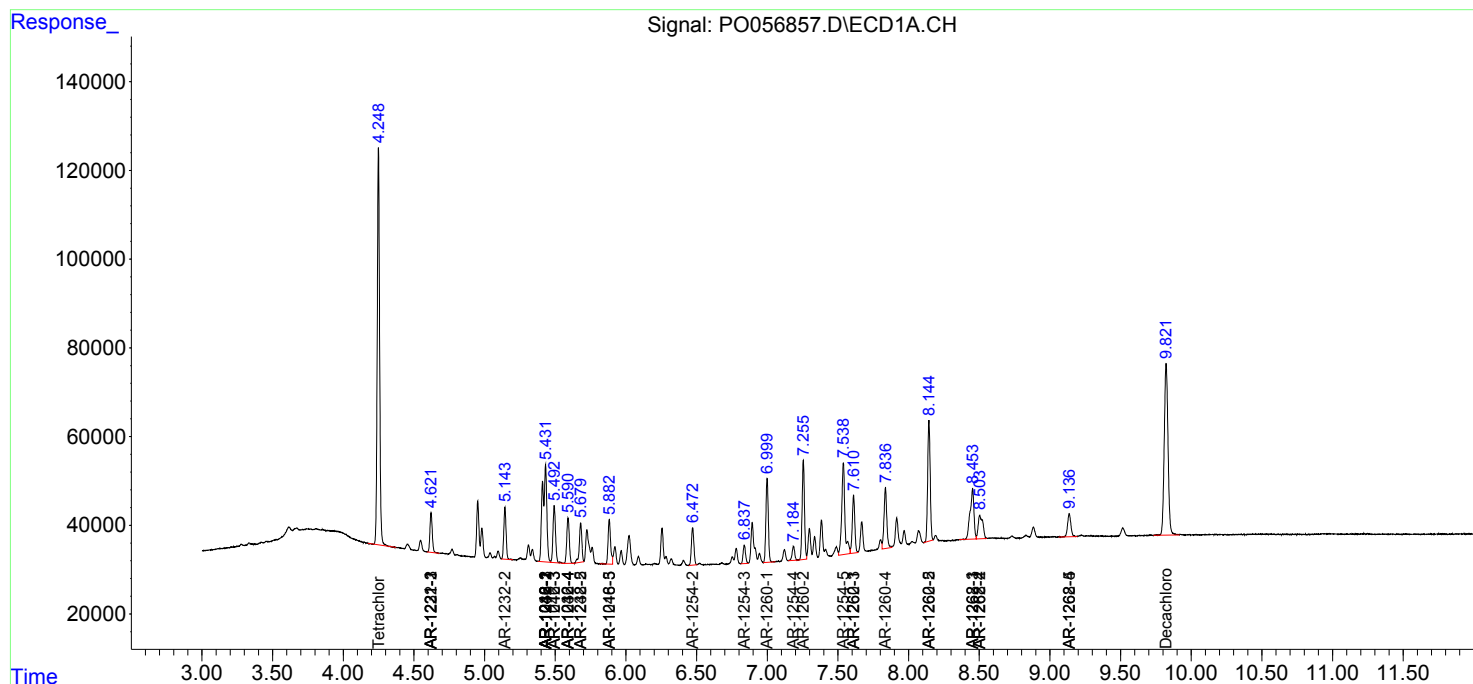


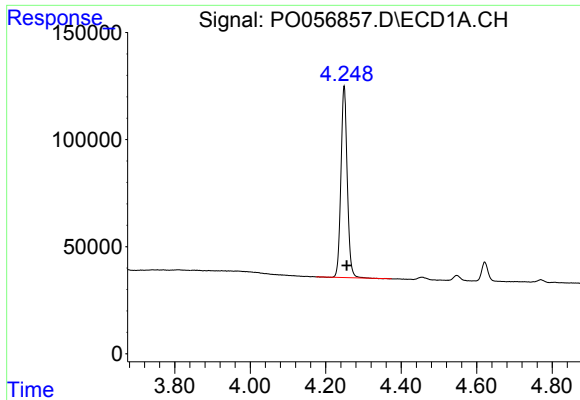

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.007 min
Response: 1043162
Conc: 27.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

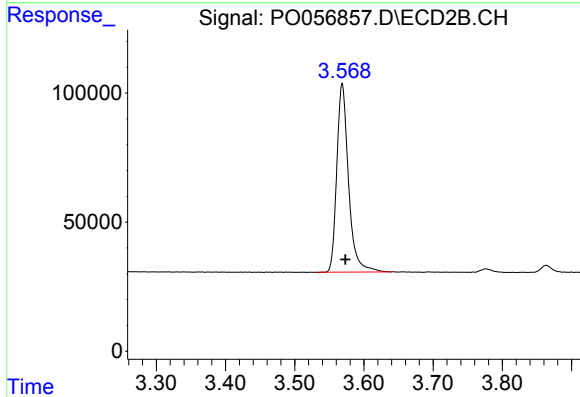


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.004 min
Response: 861917
Conc: 26.14 ng/ml

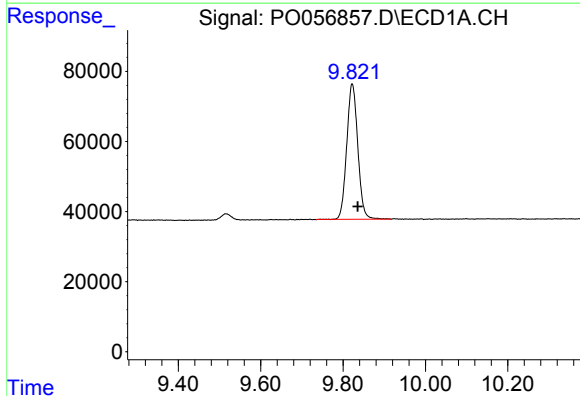


#2 Decachlorobiphenyl

R.T.: 9.822 min
Delta R.T.: -0.014 min
Response: 721634
Conc: 14.70 ng/ml

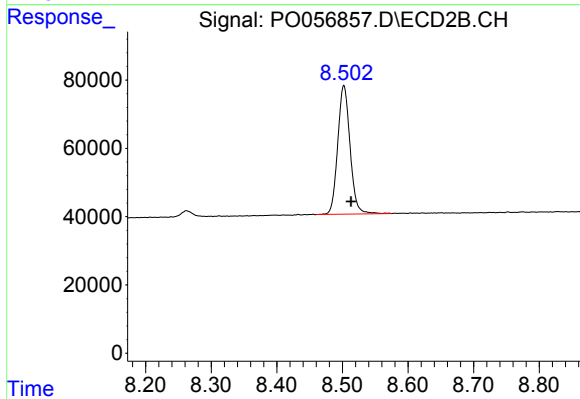

#2 Decachlorobiphenyl


R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 491972
Conc: 13.80 ng/ml

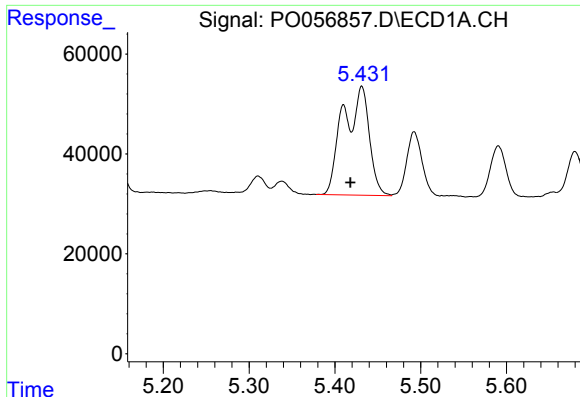

#3 AR-1016-1


R.T.: 5.431 min
Delta R.T.: 0.013 min
Response: 458588
Conc: 254.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

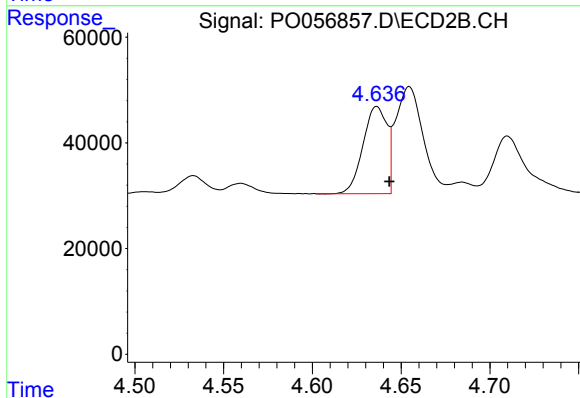


#3 AR-1016-1

R.T.: 4.636 min
Delta R.T.: -0.007 min
Response: 155344
Conc: 123.44 ng/ml

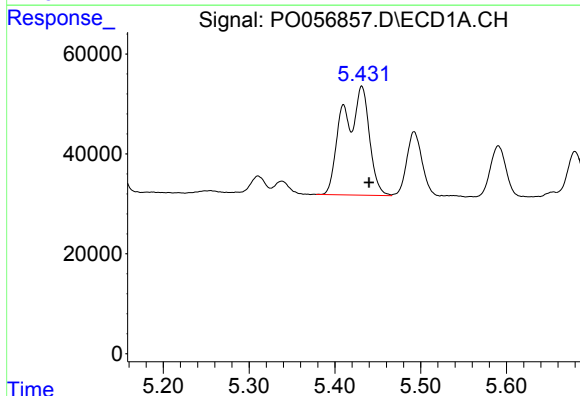


#4 AR-1016-2

R.T.: 5.431 min
Delta R.T.: -0.008 min
Response: 458588
Conc: 182.63 ng/ml

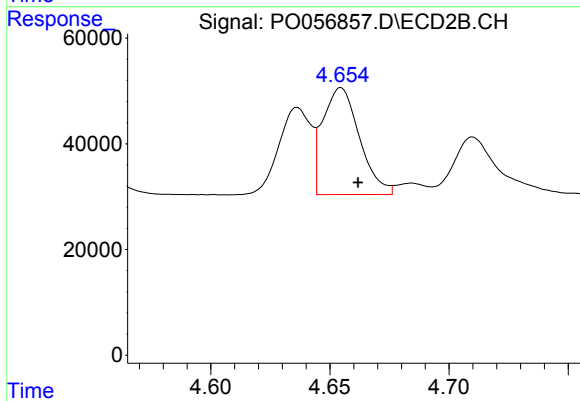

#4 AR-1016-2


R.T.: 4.655 min
Delta R.T.: -0.007 min
Response: 217313
Conc: 120.62 ng/ml

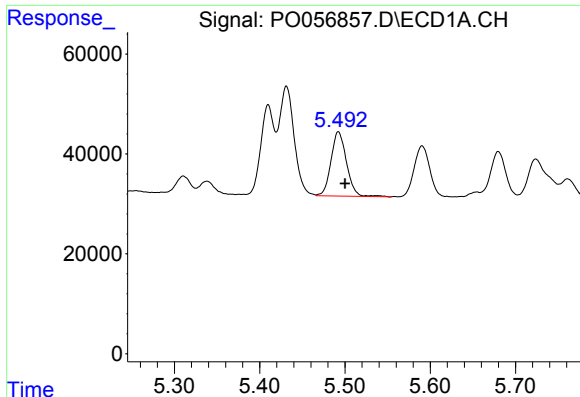

#5 AR-1016-3


R.T.: 5.493 min
Delta R.T.: -0.008 min
Response: 162707
Conc: 101.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

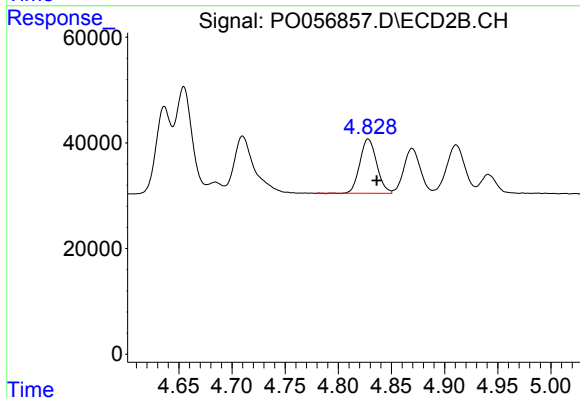


#5 AR-1016-3

R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 113089
Conc: 114.70 ng/ml

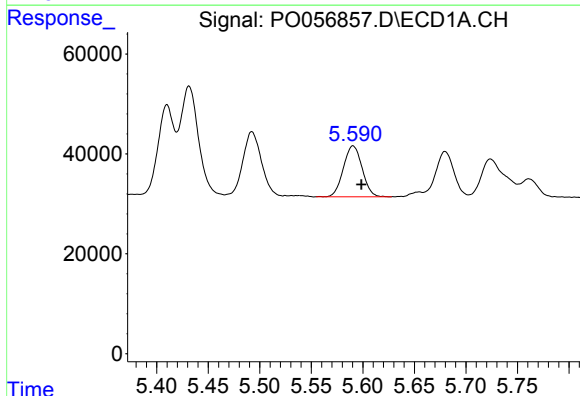


#6 AR-1016-4

R.T.: 5.591 min
Delta R.T.: -0.008 min
Response: 129007
Conc: 98.34 ng/ml

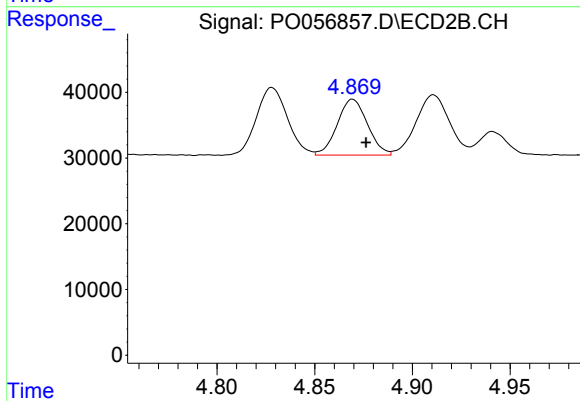

#6 AR-1016-4


R.T.: 4.869 min
Delta R.T.: -0.007 min
Response: 91375
Conc: 110.38 ng/ml

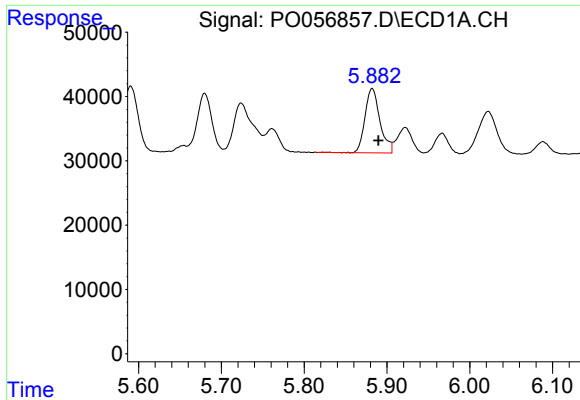

#7 AR-1016-5


R.T.: 5.882 min
Delta R.T.: -0.008 min
Response: 125144
Conc: 90.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

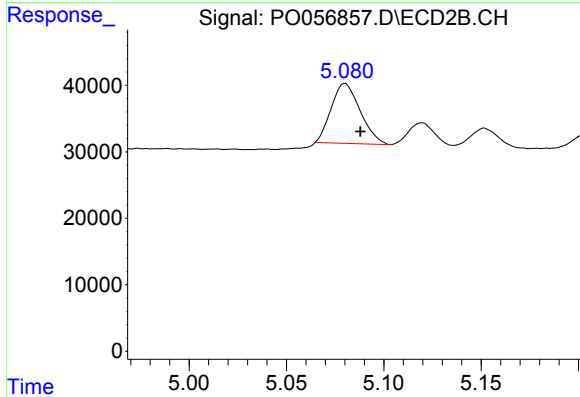


#7 AR-1016-5

R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 93590
Conc: 87.25 ng/ml

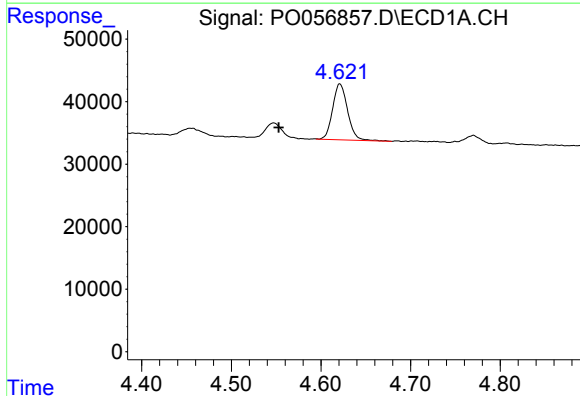


#9 AR-1221-2

R.T.: 4.621 min
Delta R.T.: 0.069 min
Response: 103466
Conc: 216.87 ng/ml

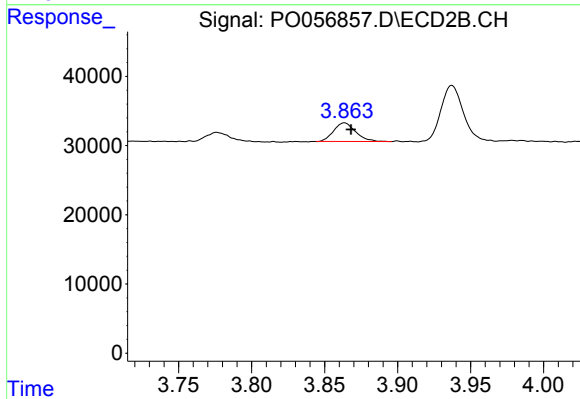

#9 AR-1221-2


R.T.: 3.864 min
Delta R.T.: -0.004 min
Response: 28412
Conc: 75.39 ng/ml

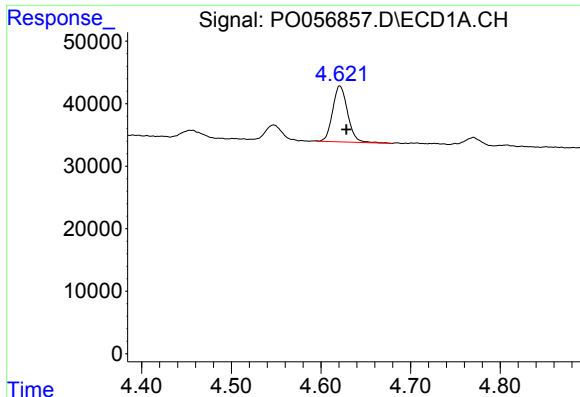

#10 AR-1221-3


R.T.: 4.621 min
Delta R.T.: -0.007 min
Response: 103466
Conc: 70.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

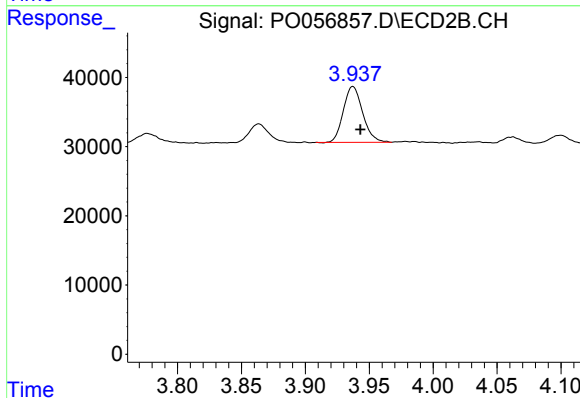


#10 AR-1221-3

R.T.: 3.937 min
Delta R.T.: -0.006 min
Response: 85342
Conc: 71.29 ng/ml

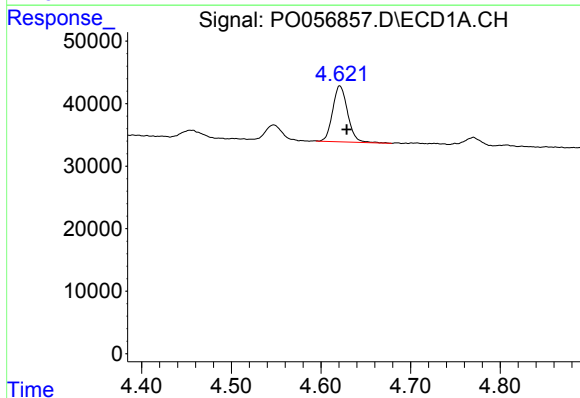


#11 AR-1232-1

R.T.: 4.621 min
Delta R.T.: -0.007 min
Response: 103466
Conc: 87.80 ng/ml

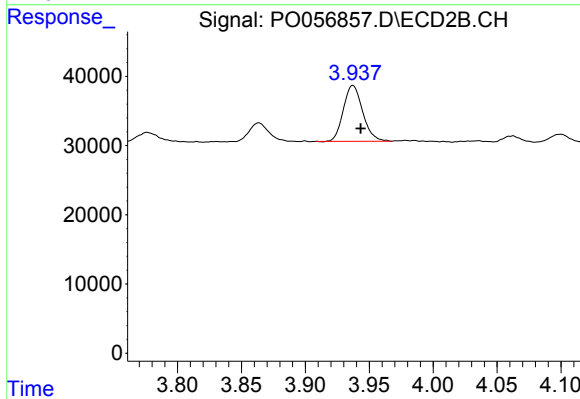

#11 AR-1232-1


R.T.: 3.937 min
Delta R.T.: -0.006 min
Response: 85342
Conc: 95.00 ng/ml

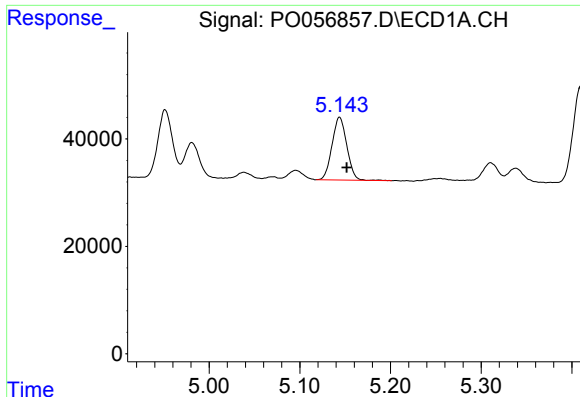

#12 AR-1232-2


R.T.: 5.144 min
Delta R.T.: -0.008 min
Response: 132461
Conc: 199.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

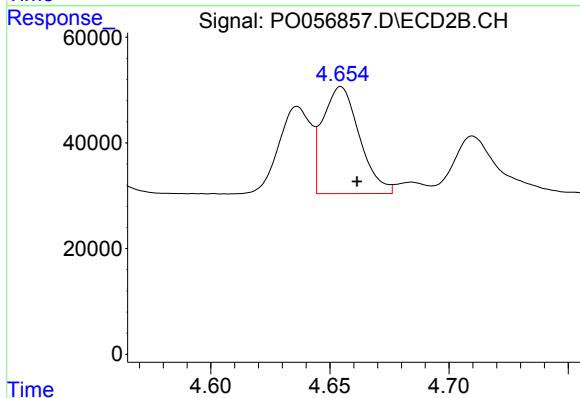


#12 AR-1232-2

R.T.: 4.655 min
Delta R.T.: -0.007 min
Response: 217313
Conc: 223.60 ng/ml

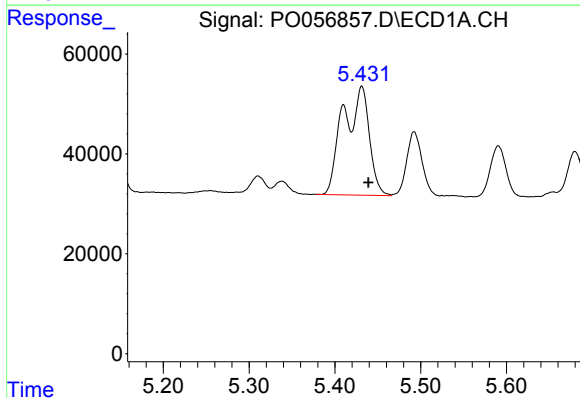


#13 AR-1232-3

R.T.: 5.431 min
Delta R.T.: -0.008 min
Response: 458588
Conc: 323.26 ng/ml

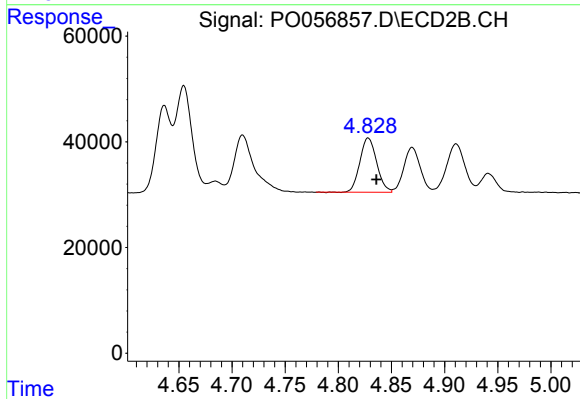

#13 AR-1232-3


R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 113089
Conc: 216.11 ng/ml

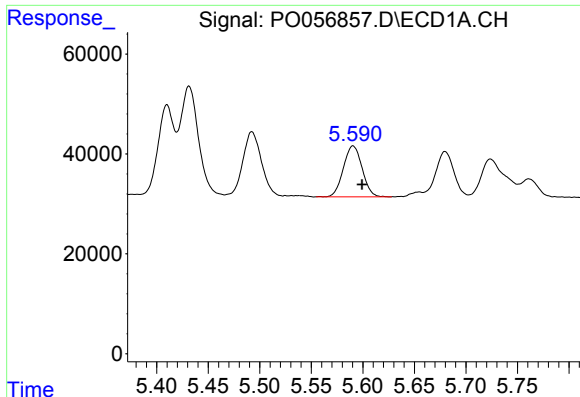

#14 AR-1232-4


R.T.: 5.591 min
Delta R.T.: -0.009 min
Response: 129007
Conc: 183.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

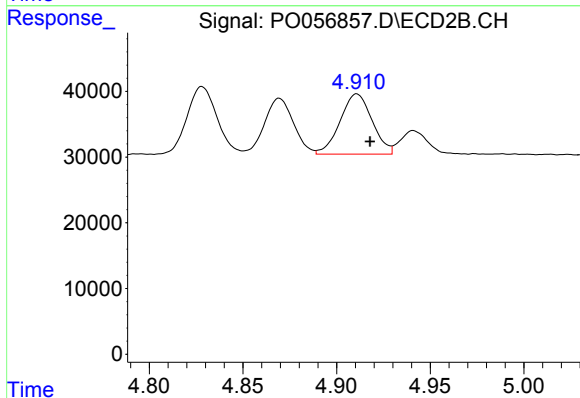


#14 AR-1232-4

R.T.: 4.911 min
Delta R.T.: -0.007 min
Response: 109176
Conc: 221.59 ng/ml

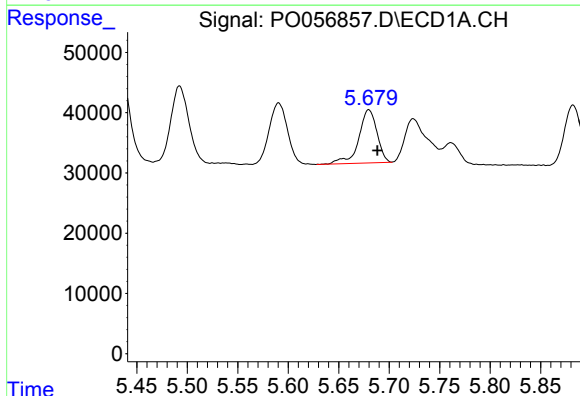


#15 AR-1232-5

R.T.: 5.680 min
Delta R.T.: -0.008 min
Response: 110375
Conc: 195.22 ng/ml

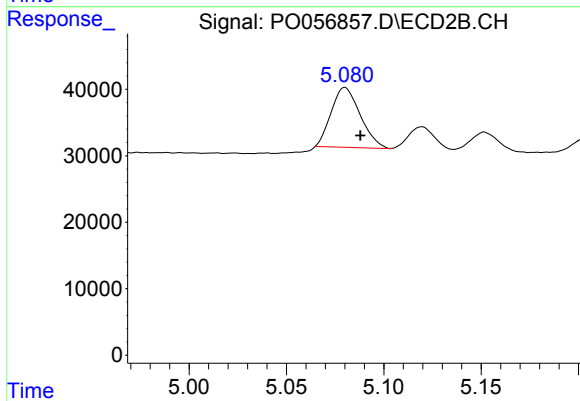

#15 AR-1232-5


R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 93590
Conc: 166.16 ng/ml

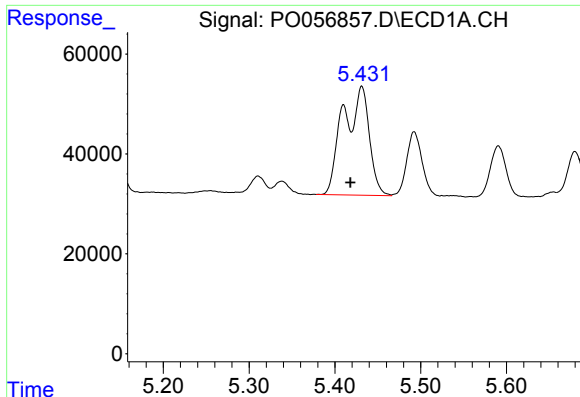

#16 AR-1242-1


R.T.: 5.431 min
Delta R.T.: 0.013 min
Response: 458588
Conc: 265.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

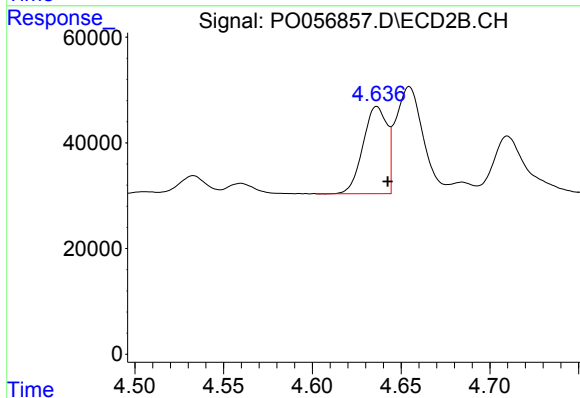


#16 AR-1242-1

R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 155344
Conc: 125.42 ng/ml

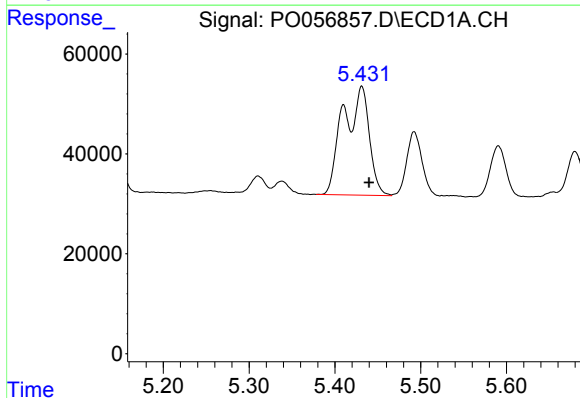


#17 AR-1242-2

R.T.: 5.431 min
Delta R.T.: -0.008 min
Response: 458588
Conc: 180.63 ng/ml

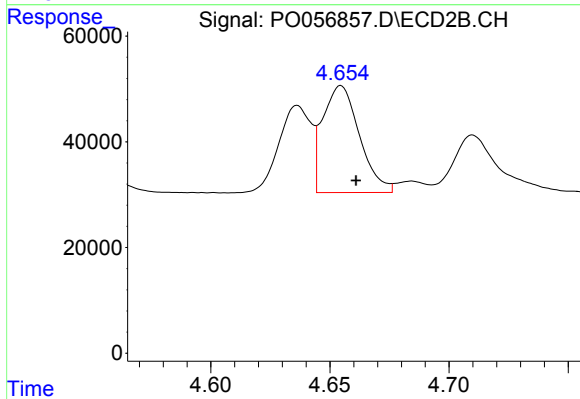

#17 AR-1242-2


R.T.: 4.655 min
Delta R.T.: -0.006 min
Response: 217313
Conc: 120.84 ng/ml

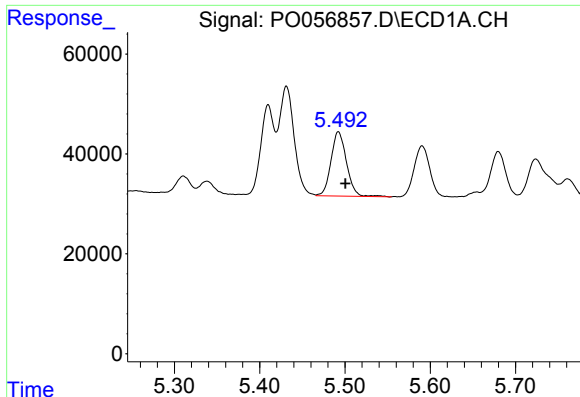

#18 AR-1242-3


R.T.: 5.493 min
Delta R.T.: -0.008 min
Response: 162707
Conc: 100.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

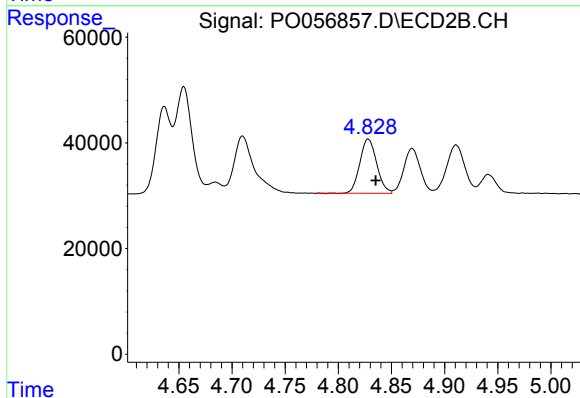


#18 AR-1242-3

R.T.: 4.828 min
Delta R.T.: -0.007 min
Response: 113089
Conc: 115.03 ng/ml

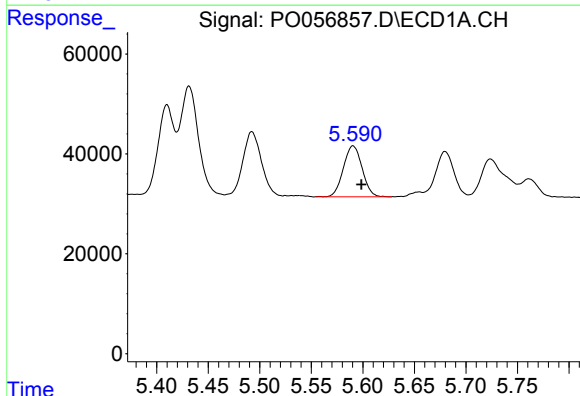


#19 AR-1242-4

R.T.: 5.591 min
Delta R.T.: -0.008 min
Response: 129007
Conc: 96.51 ng/ml

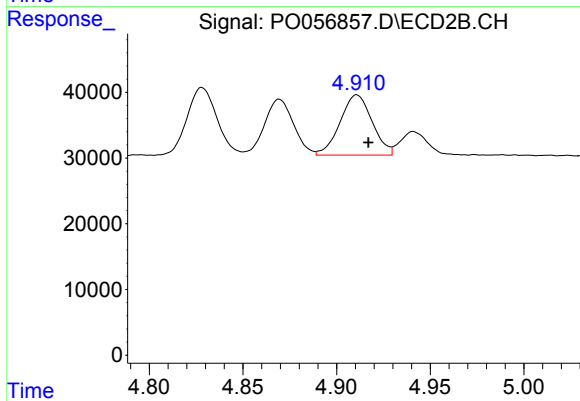

#19 AR-1242-4


R.T.: 4.911 min
Delta R.T.: -0.006 min
Response: 109176
Conc: 112.19 ng/ml

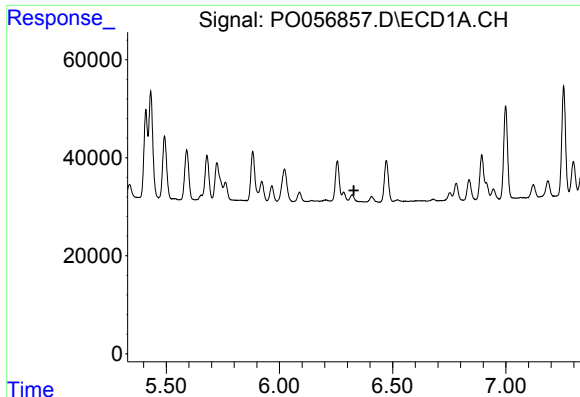

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

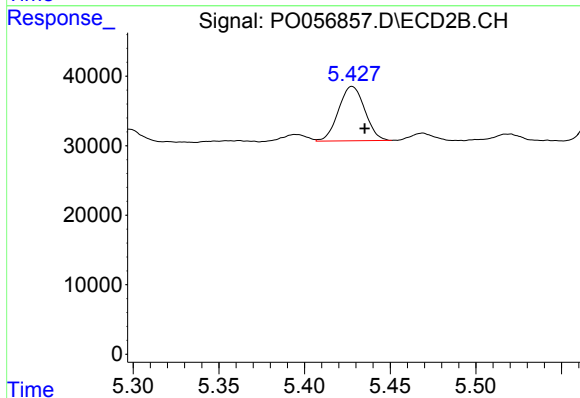


#20 AR-1242-5

R.T.: 5.428 min
Delta R.T.: -0.007 min
Response: 83610
Conc: 70.72 ng/ml

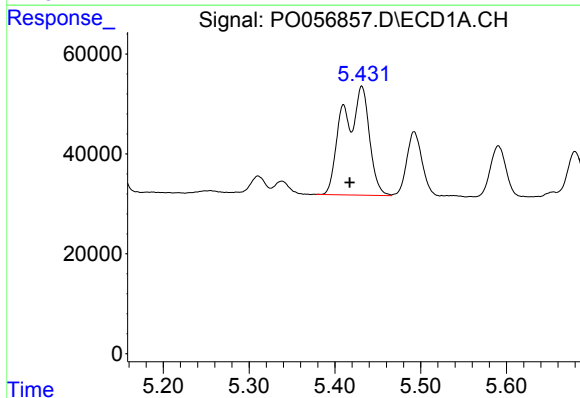


#21 AR-1248-1

R.T.: 5.431 min
Delta R.T.: 0.014 min
Response: 458588
Conc: 355.90 ng/ml

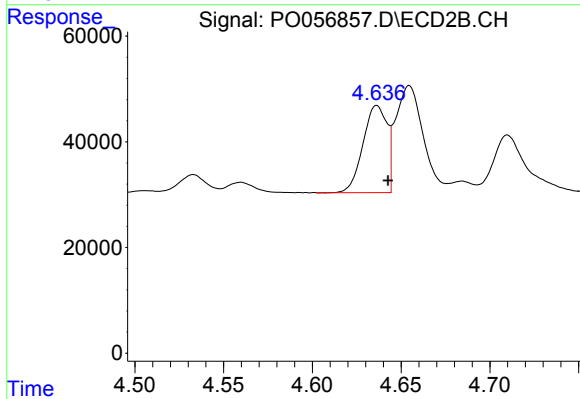

#21 AR-1248-1


R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 155344
Conc: 165.87 ng/ml

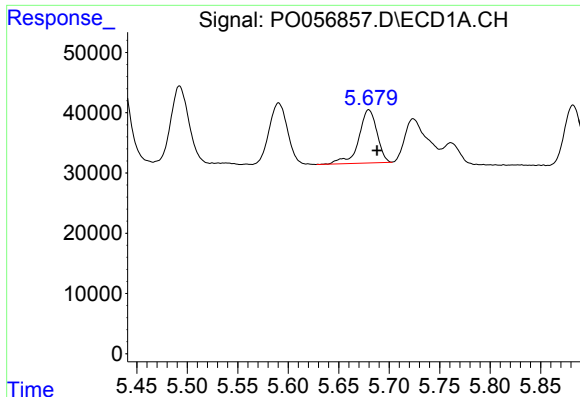

#22 AR-1248-2


R.T.: 5.680 min
Delta R.T.: -0.008 min
Response: 110375
Conc: 59.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

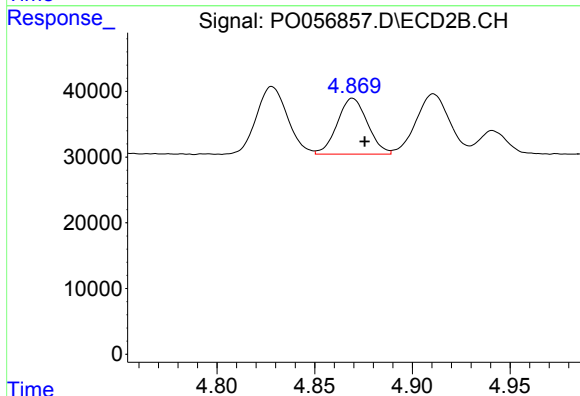


#22 AR-1248-2

R.T.: 4.869 min
Delta R.T.: -0.006 min
Response: 91375
Conc: 71.92 ng/ml

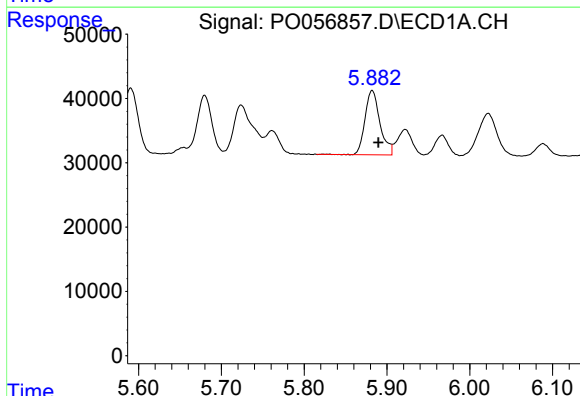


#23 AR-1248-3

R.T.: 5.882 min
Delta R.T.: -0.008 min
Response: 125144
Conc: 61.01 ng/ml

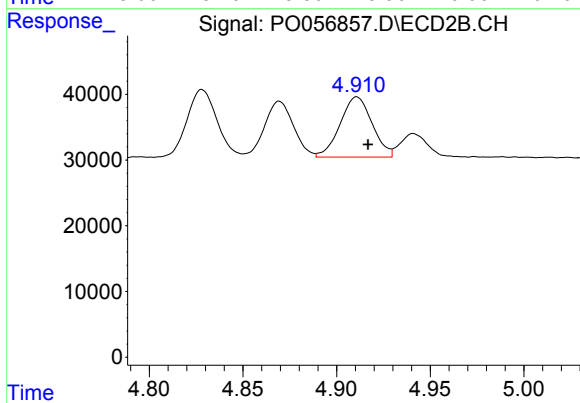

#23 AR-1248-3


R.T.: 4.911 min
Delta R.T.: -0.006 min
Response: 109176
Conc: 83.60 ng/ml

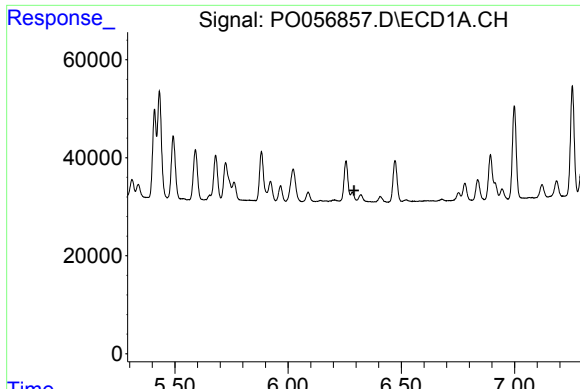

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

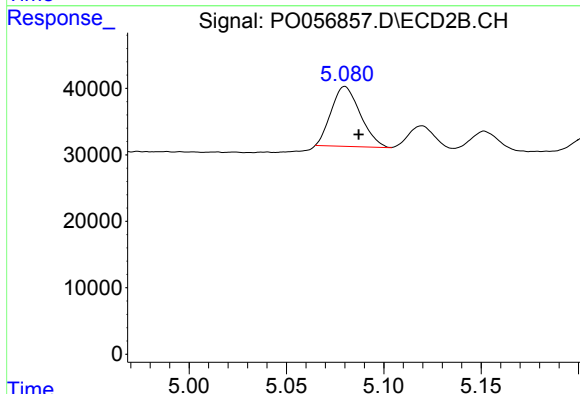


#24 AR-1248-4

R.T.: 5.080 min
Delta R.T.: -0.007 min
Response: 93590
Conc: 59.10 ng/ml

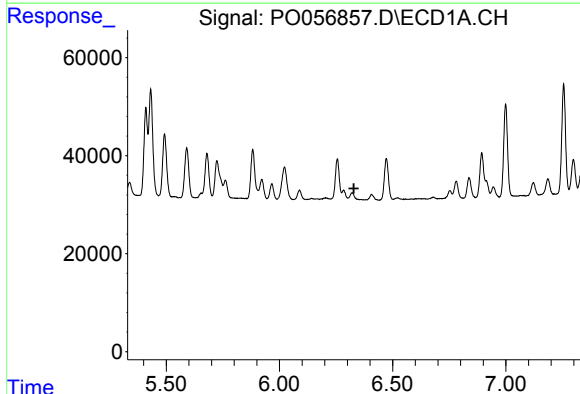


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

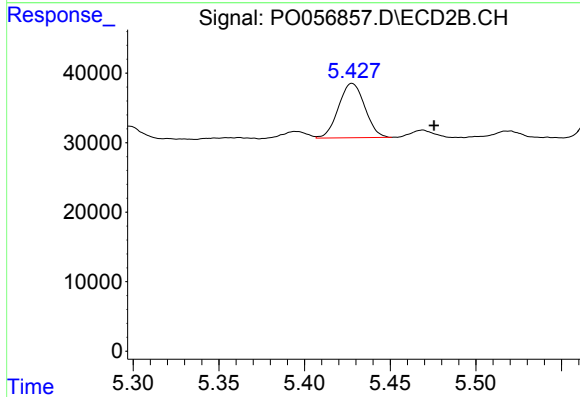

#25 AR-1248-5


R.T.: 5.428 min
Delta R.T.: -0.048 min
Response: 83610
Conc: 50.52 ng/ml

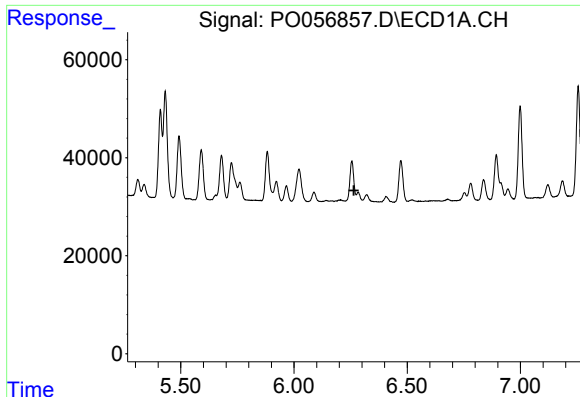

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

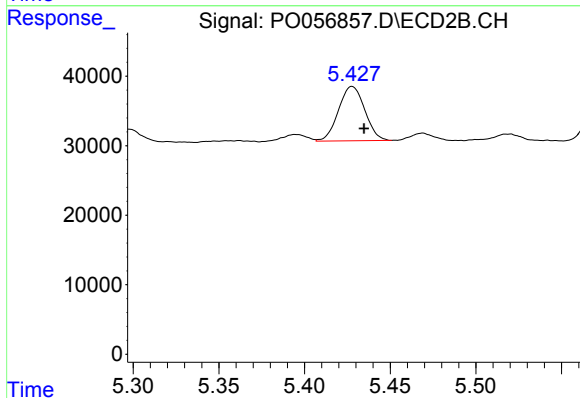


#26 AR-1254-1

R.T.: 5.428 min
Delta R.T.: -0.007 min
Response: 83610
Conc: 31.61 ng/ml

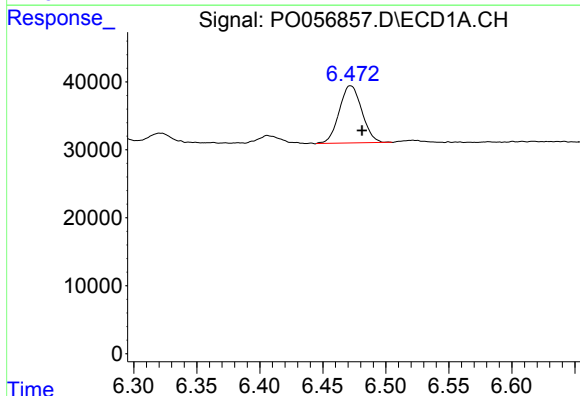


#27 AR-1254-2

R.T.: 6.472 min
Delta R.T.: -0.009 min
Response: 105067
Conc: 27.05 ng/ml

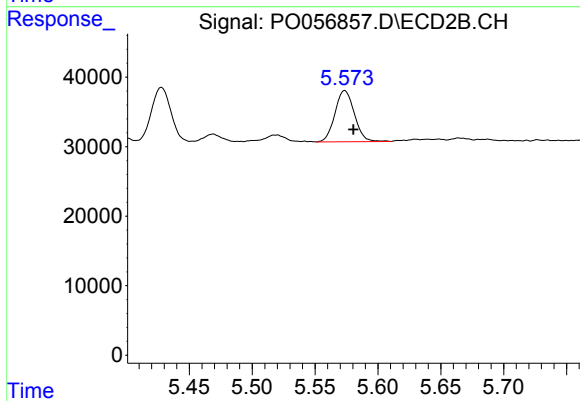

#27 AR-1254-2


R.T.: 5.574 min
Delta R.T.: -0.007 min
Response: 78928
Conc: 36.61 ng/ml

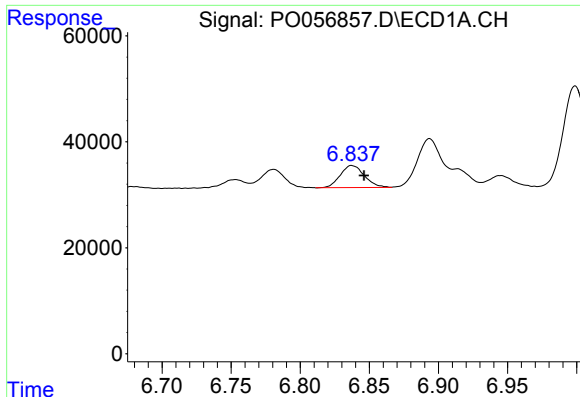

#28 AR-1254-3


R.T.: 6.838 min
Delta R.T.: -0.009 min
Response: 50613
Conc: 12.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

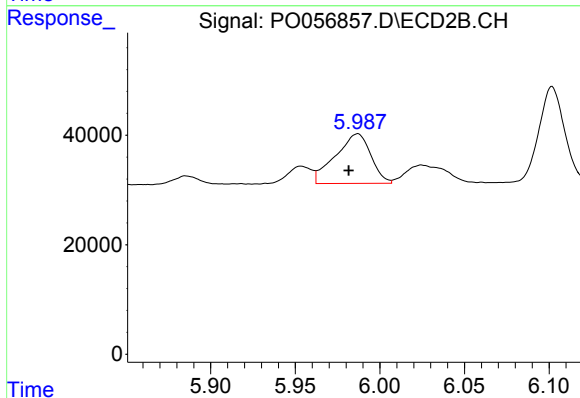


#28 AR-1254-3

R.T.: 5.987 min
Delta R.T.: 0.005 min
Response: 131940
Conc: 36.04 ng/ml

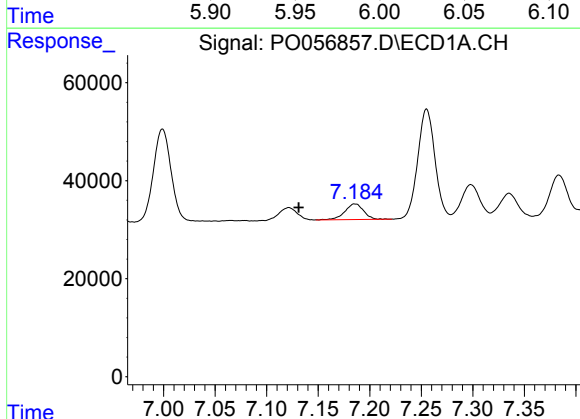


#29 AR-1254-4

R.T.: 7.186 min
Delta R.T.: 0.055 min
Response: 40178
Conc: 13.35 ng/ml

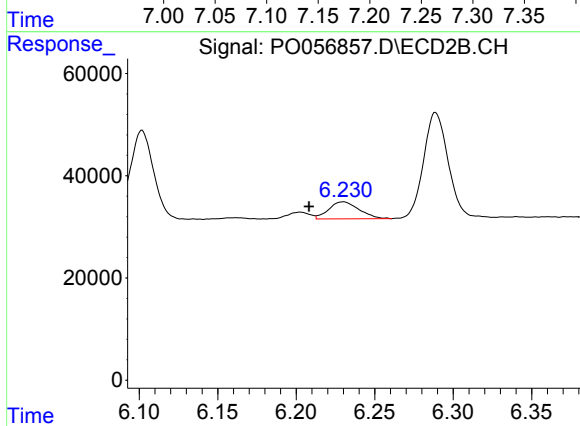

#29 AR-1254-4


R.T.: 6.230 min
Delta R.T.: 0.022 min
Response: 45237
Conc: 20.59 ng/ml

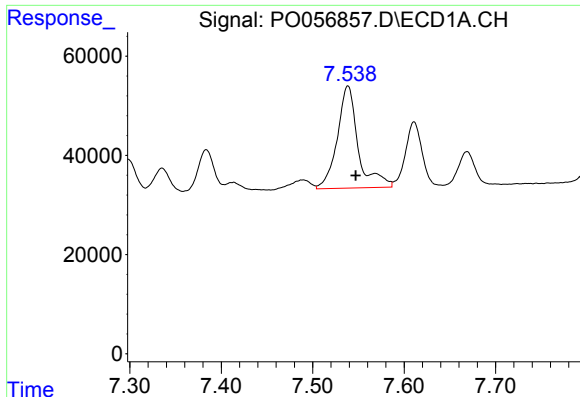

#30 AR-1254-5


R.T.: 7.538 min
Delta R.T.: -0.009 min
Response: 326426
Conc: 86.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

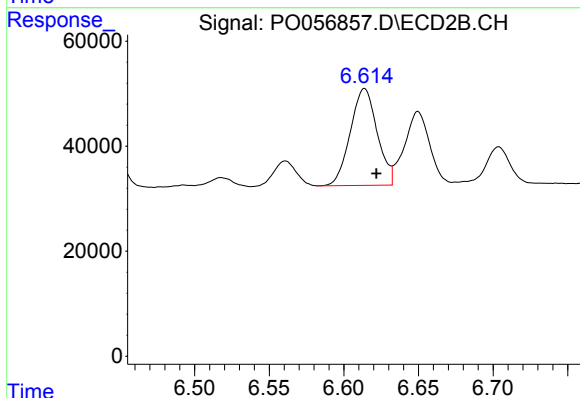


#30 AR-1254-5

R.T.: 6.614 min
Delta R.T.: -0.008 min
Response: 231583
Conc: 73.05 ng/ml

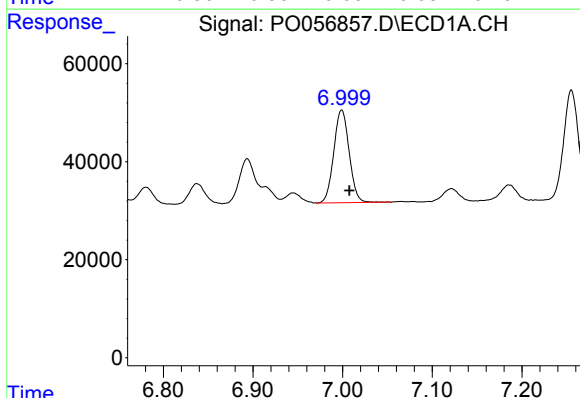


#31 AR-1260-1

R.T.: 6.999 min
Delta R.T.: -0.009 min
Response: 225357
Conc: 87.82 ng/ml

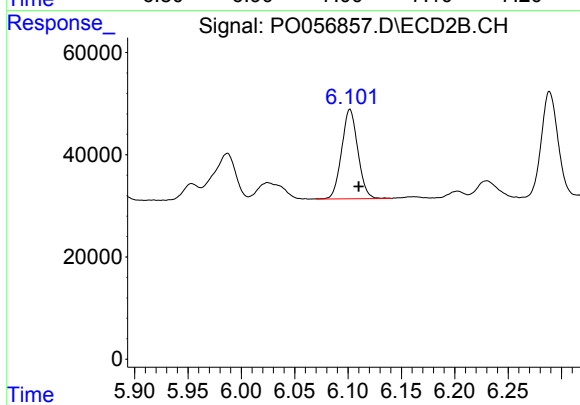

#31 AR-1260-1


R.T.: 6.102 min
Delta R.T.: -0.008 min
Response: 184866
Conc: 92.42 ng/ml

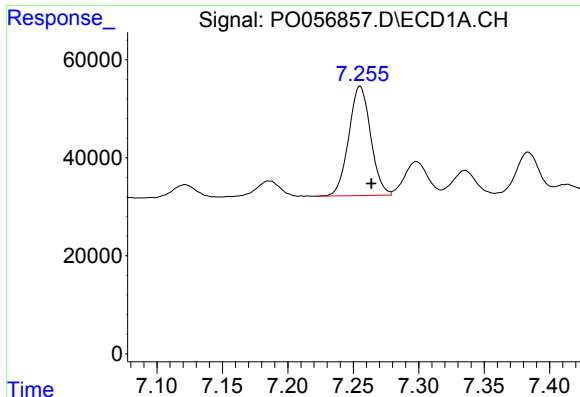

#32 AR-1260-2


R.T.: 7.255 min
Delta R.T.: -0.009 min
Response: 259845
Conc: 85.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

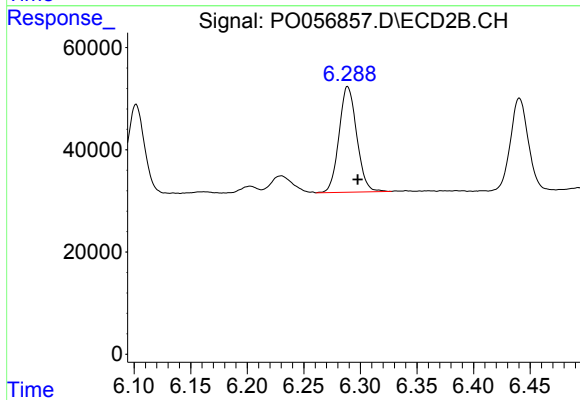


#32 AR-1260-2

R.T.: 6.289 min
Delta R.T.: -0.009 min
Response: 225039
Conc: 91.29 ng/ml

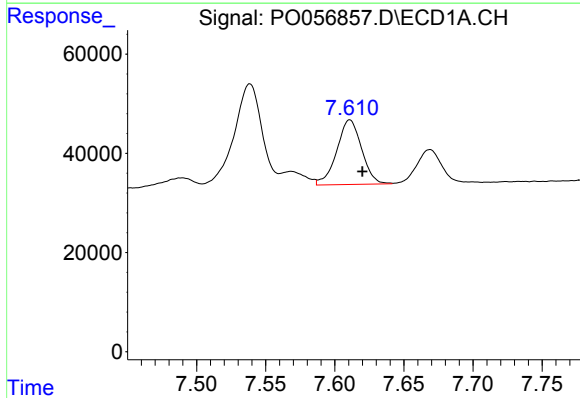


#33 AR-1260-3

R.T.: 7.611 min
Delta R.T.: -0.009 min
Response: 163225
Conc: 67.75 ng/ml

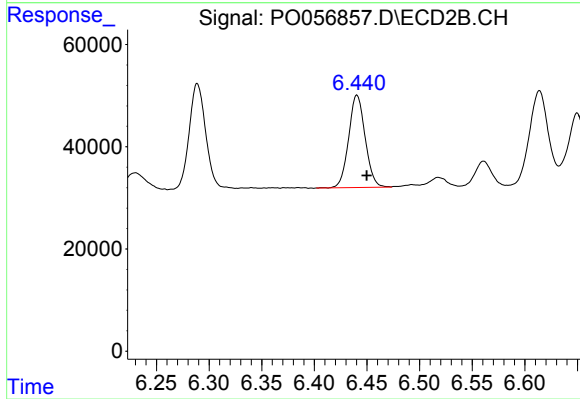

#33 AR-1260-3


R.T.: 6.441 min
Delta R.T.: -0.009 min
Response: 197007
Conc: 87.82 ng/ml

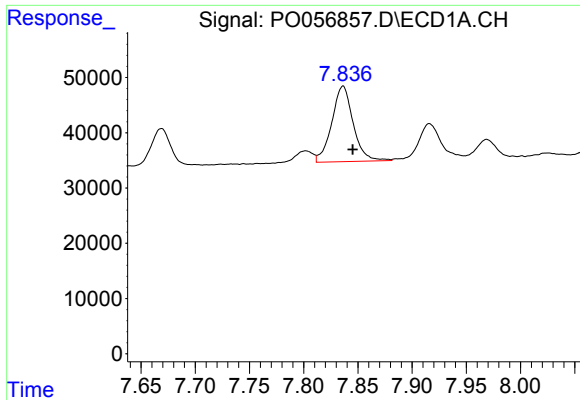

#34 AR-1260-4


R.T.: 7.836 min
Delta R.T.: -0.009 min
Response: 188100
Conc: 71.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

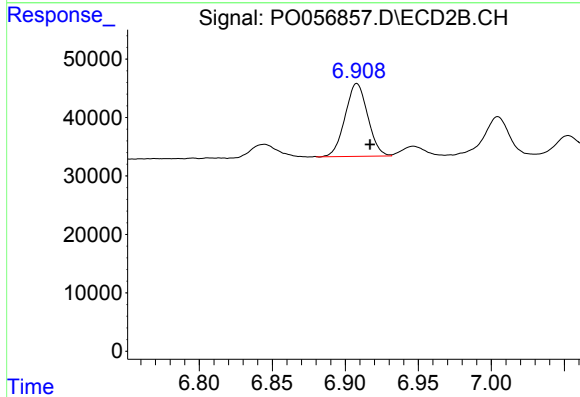


#34 AR-1260-4

R.T.: 6.908 min
Delta R.T.: -0.009 min
Response: 134754
Conc: 72.41 ng/ml

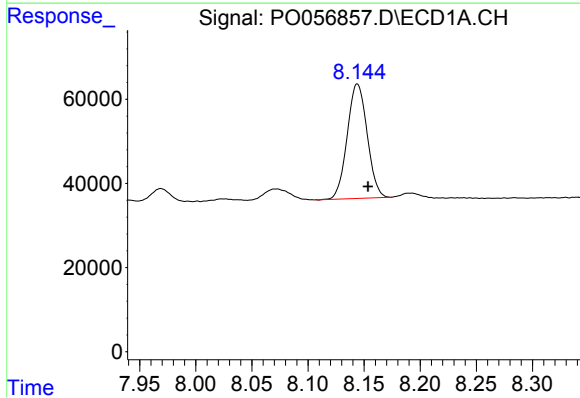


#35 AR-1260-5

R.T.: 8.144 min
Delta R.T.: -0.009 min
Response: 336979
Conc: 70.47 ng/ml

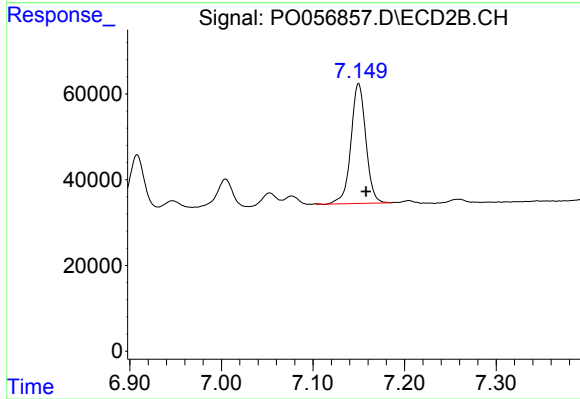

#35 AR-1260-5


R.T.: 7.150 min
Delta R.T.: -0.008 min
Response: 315944
Conc: 73.27 ng/ml

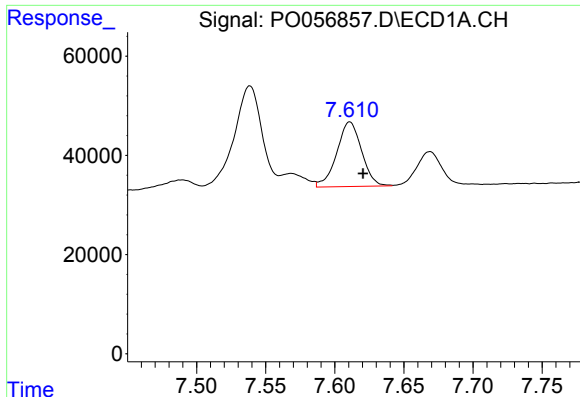

#36 AR-1262-1


R.T.: 7.611 min
Delta R.T.: -0.009 min
Response: 163225
Conc: 34.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

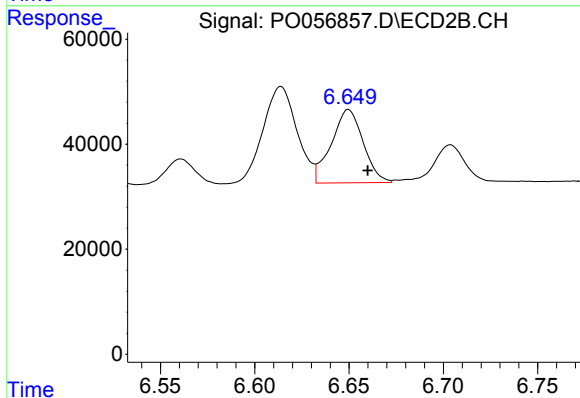


#36 AR-1262-1

R.T.: 6.650 min
Delta R.T.: -0.010 min
Response: 164517
Conc: 39.41 ng/ml

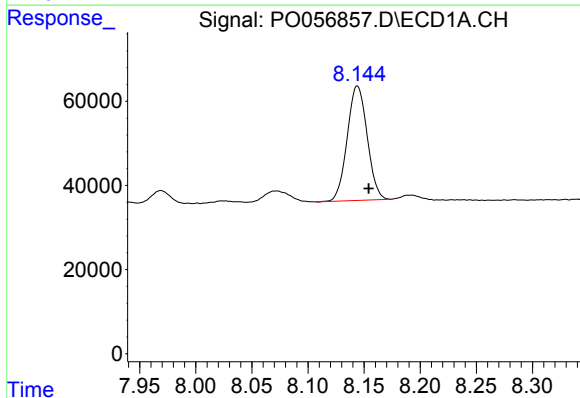


#37 AR-1262-2

R.T.: 8.144 min
Delta R.T.: -0.010 min
Response: 336979
Conc: 44.20 ng/ml

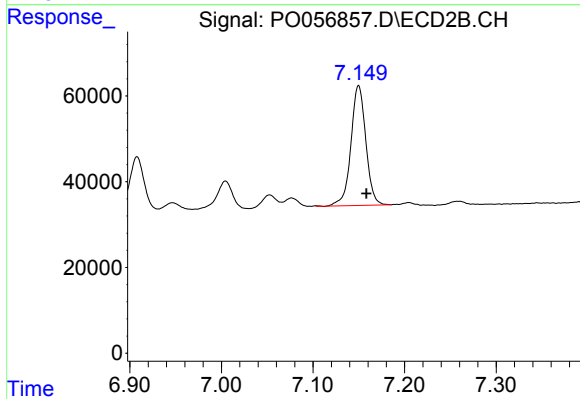

#37 AR-1262-2


R.T.: 7.150 min
Delta R.T.: -0.009 min
Response: 315944
Conc: 45.98 ng/ml

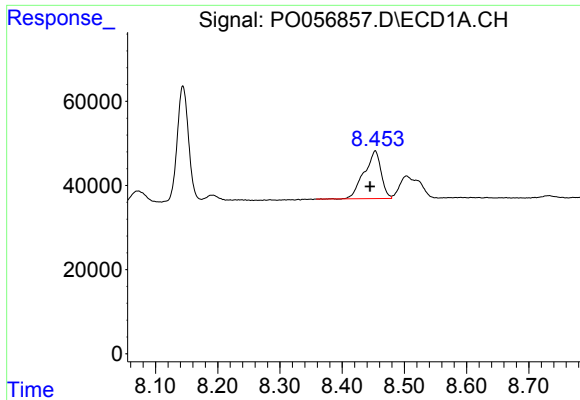

#38 AR-1262-3


R.T.: 8.453 min
Delta R.T.: 0.008 min
Response: 214957
Conc: 41.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

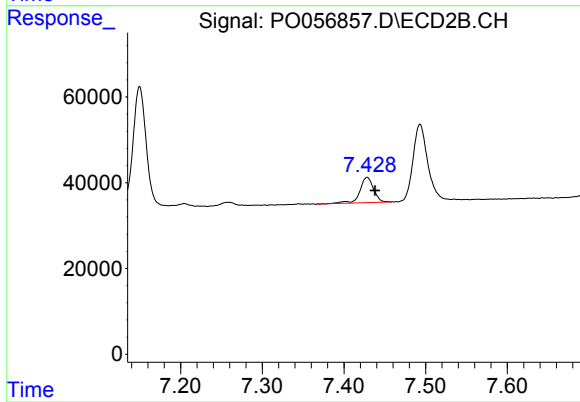


#38 AR-1262-3

R.T.: 7.428 min
Delta R.T.: -0.010 min
Response: 68200
Conc: 23.09 ng/ml

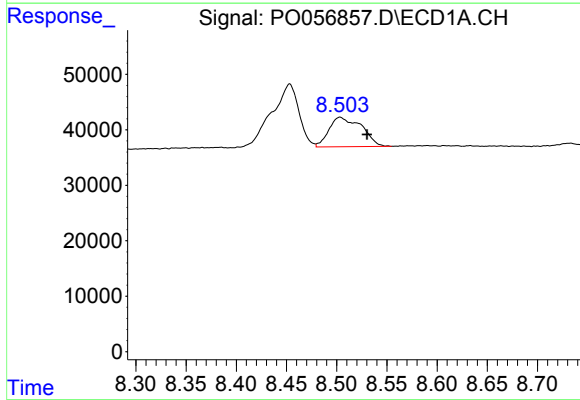


#39 AR-1262-4

R.T.: 8.504 min
Delta R.T.: -0.027 min
Response: 120139
Conc: 28.14 ng/ml

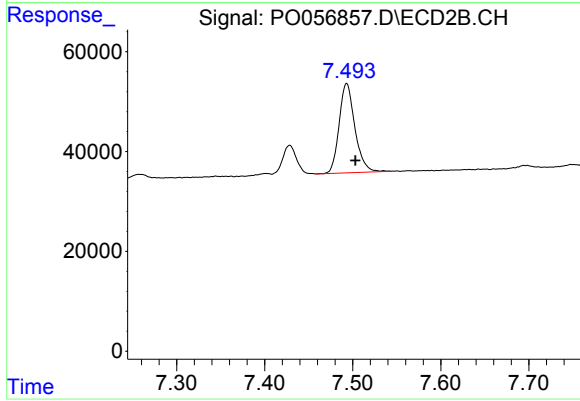

#39 AR-1262-4


R.T.: 7.493 min
Delta R.T.: -0.010 min
Response: 222506
Conc: 42.70 ng/ml

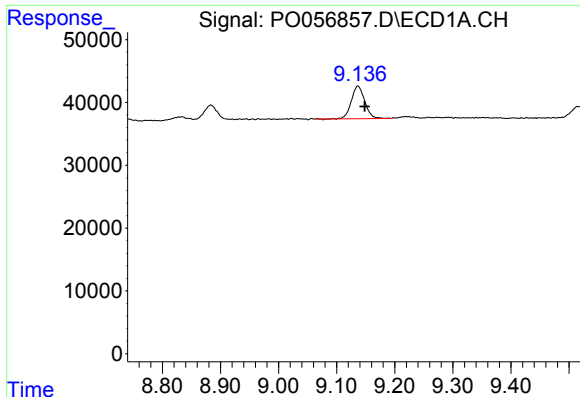

#40 AR-1262-5


R.T.: 9.137 min
Delta R.T.: -0.011 min
Response: 83394
Conc: 30.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

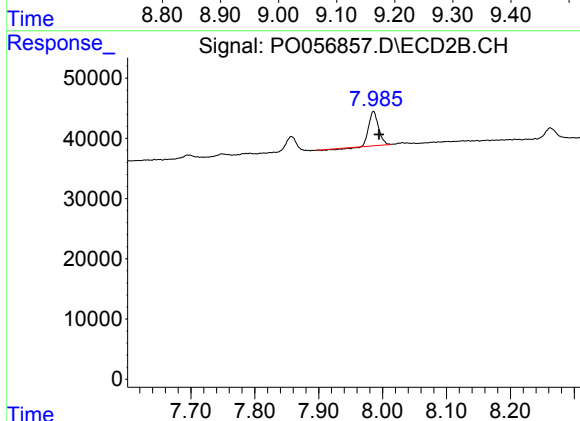


#40 AR-1262-5

R.T.: 7.986 min
Delta R.T.: -0.009 min
Response: 57396
Conc: 24.72 ng/ml

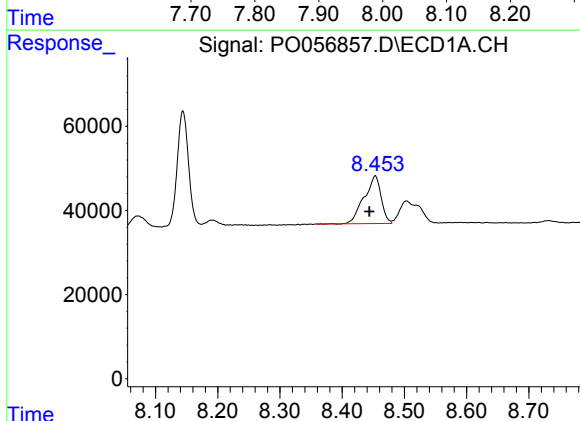


#41 AR-1268-1

R.T.: 8.453 min
Delta R.T.: 0.009 min
Response: 214957
Conc: 26.42 ng/ml

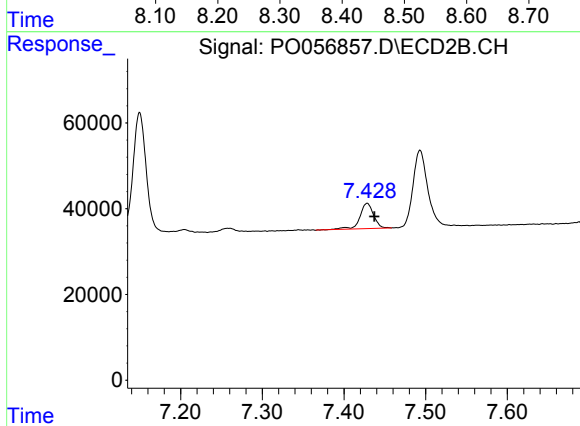

#41 AR-1268-1


R.T.: 7.428 min
Delta R.T.: -0.009 min
Response: 68200
Conc: 9.14 ng/ml

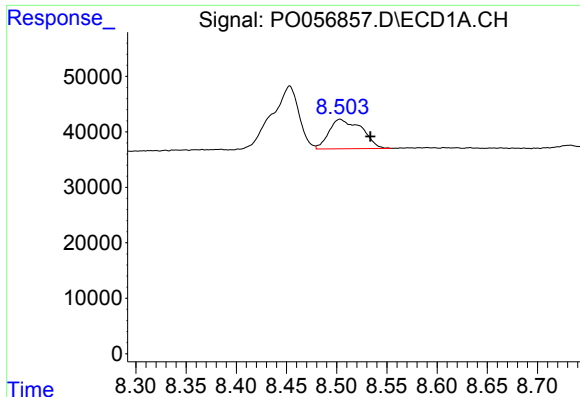

#42 AR-1268-2


R.T.: 8.504 min
Delta R.T.: -0.030 min
Response: 120139
Conc: 14.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

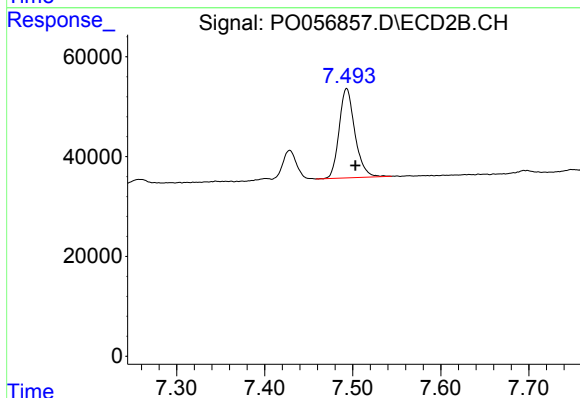


#42 AR-1268-2

R.T.: 7.493 min
Delta R.T.: -0.010 min
Response: 222506
Conc: 31.86 ng/ml

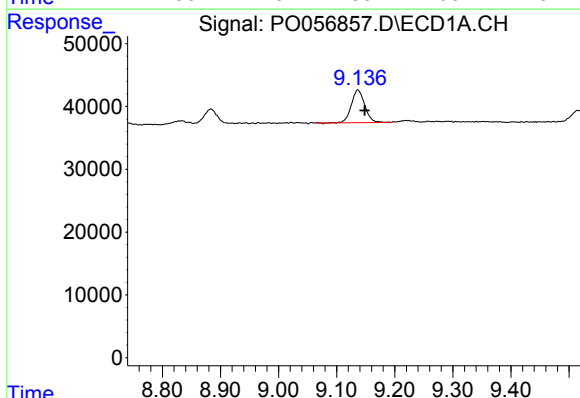


#44 AR-1268-4

R.T.: 9.137 min
Delta R.T.: -0.012 min
Response: 83394
Conc: 30.58 ng/ml

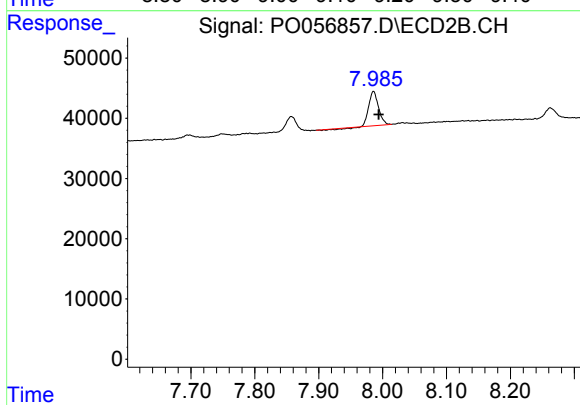

#44 AR-1268-4


R.T.: 7.986 min
Delta R.T.: -0.008 min
Response: 57396
Conc: 24.59 ng/ml

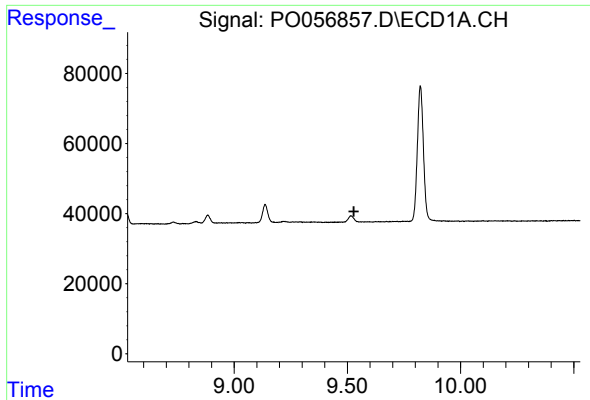

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

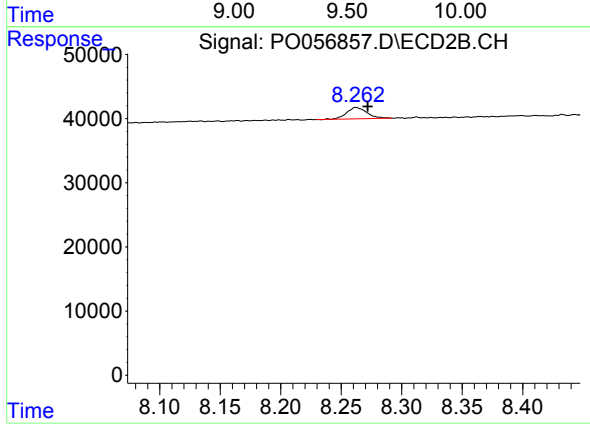

#45 AR-1268-5

R.T.: 8.262 min
Delta R.T.: -0.010 min
Response: 20674
Conc: 1.19 ng/ml