

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 23:09
 Operator : SM/SJ
 Sample : K3175-01MSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:20:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.250	3.569	1063796	835459	27.787	25.333
2)	SA Decachlor...	9.823	8.504	725234	499877	14.775	14.019
Target Compounds							
3)	L1 AR-1016-1	5.433	4.637	463019	153640	257.430	122.083 #
4)	L1 AR-1016-2	5.433	4.655	463019	219724	184.391	121.959 #
5)	L1 AR-1016-3	5.493	4.829	163967	113531	102.014	115.150
6)	L1 AR-1016-4	5.591	4.870	127608	93053	97.277	112.405
7)	L1 AR-1016-5	5.882	5.081	124832	91546	90.352	85.340
9)	L2 AR-1221-2	4.622	3.864	110240	28812	231.064	76.452 #
10)	L2 AR-1221-3	4.622	3.938	110240	83811	74.584	70.014
11)	L3 AR-1232-1	4.622	3.938	110240	83811	93.552	93.293
12)	L3 AR-1232-2	5.145	4.655	136184	219724	205.393	226.082
13)	L3 AR-1232-3	5.433	4.829	463019	113531	326.380	216.956 #
14)	L3 AR-1232-4	5.591	4.911	127608	108644	181.280	220.513
15)	L3 AR-1232-5	5.680	5.081	109608	91546	193.864	162.531
16)	L4 AR-1242-1	5.433	4.637	463019	153640	268.387	124.045 #
17)	L4 AR-1242-2	5.433	4.655	463019	219724	182.379	122.176 #
18)	L4 AR-1242-3	5.493	4.829	163967	113531	100.840	115.482
19)	L4 AR-1242-4	5.591	4.911	127608	108644	95.463	111.647
20)	L4 AR-1242-5	0.000	5.428	0	84191	N.D.	71.211 #
21)	L5 AR-1248-1	5.433	4.637	463019	153640	359.343	164.054 #
22)	L5 AR-1248-2	5.680	4.870	109608	93053	58.838	73.245
23)	L5 AR-1248-3	5.882	4.911	124832	108644	60.853	83.195 #
24)	L5 AR-1248-4	0.000	5.081	0	91546	N.D.	57.808 #
25)	L5 AR-1248-5	0.000	5.428	0	84191	N.D.	50.869 #
26)	L6 AR-1254-1	0.000	5.428	0	84191	N.D.	31.834 #
27)	L6 AR-1254-2	6.472	5.574	105859	78898	27.255	36.598 #
28)	L6 AR-1254-3	6.839	5.987	54701	136115	13.266	37.179 #
29)	L6 AR-1254-4	7.185	6.229	40299	45402	13.389	20.666 #
30)	L6 AR-1254-5	7.538	6.614	324148	235927	86.080	74.419
31)	L7 AR-1260-1	6.999	6.101	227403	188898	88.616	94.431
32)	L7 AR-1260-2	7.255	6.289	261699	230233	86.536	93.402
33)	L7 AR-1260-3	7.611	6.441	161750	200396	67.143	89.334 #
34)	L7 AR-1260-4	7.836	6.908	186719	138569	71.288	74.458
35)	L7 AR-1260-5	8.144	7.150	332317	325377	69.492	75.453
36)	L8 AR-1262-1	7.611	6.650	161750	171234	34.585	41.023
37)	L8 AR-1262-2	8.144	7.150	332317	325377	43.589	47.358
38)	L8 AR-1262-3	8.454	7.429	215711	70693	41.217	23.936 #
39)	L8 AR-1262-4	8.504	7.493	121690	226489	28.505	43.467 #
40)	L8 AR-1262-5	9.138	7.986	82142	59720	29.895	25.718
41)	L9 AR-1268-1	8.454	7.429	215711	70693	26.508	9.470 #
42)	L9 AR-1268-2	8.504	7.493	121690	226489	15.042	32.434 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 23:09
Operator : SM/SJ
Sample : K3175-01MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:20:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	9.138	7.986	82142	59720	30.121	25.584
45)	L9 AR-1268-5	0.000	8.265	0	22681	N.D.	1.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 23:09
Operator : SM/SJ
Sample : K3175-01MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:20:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

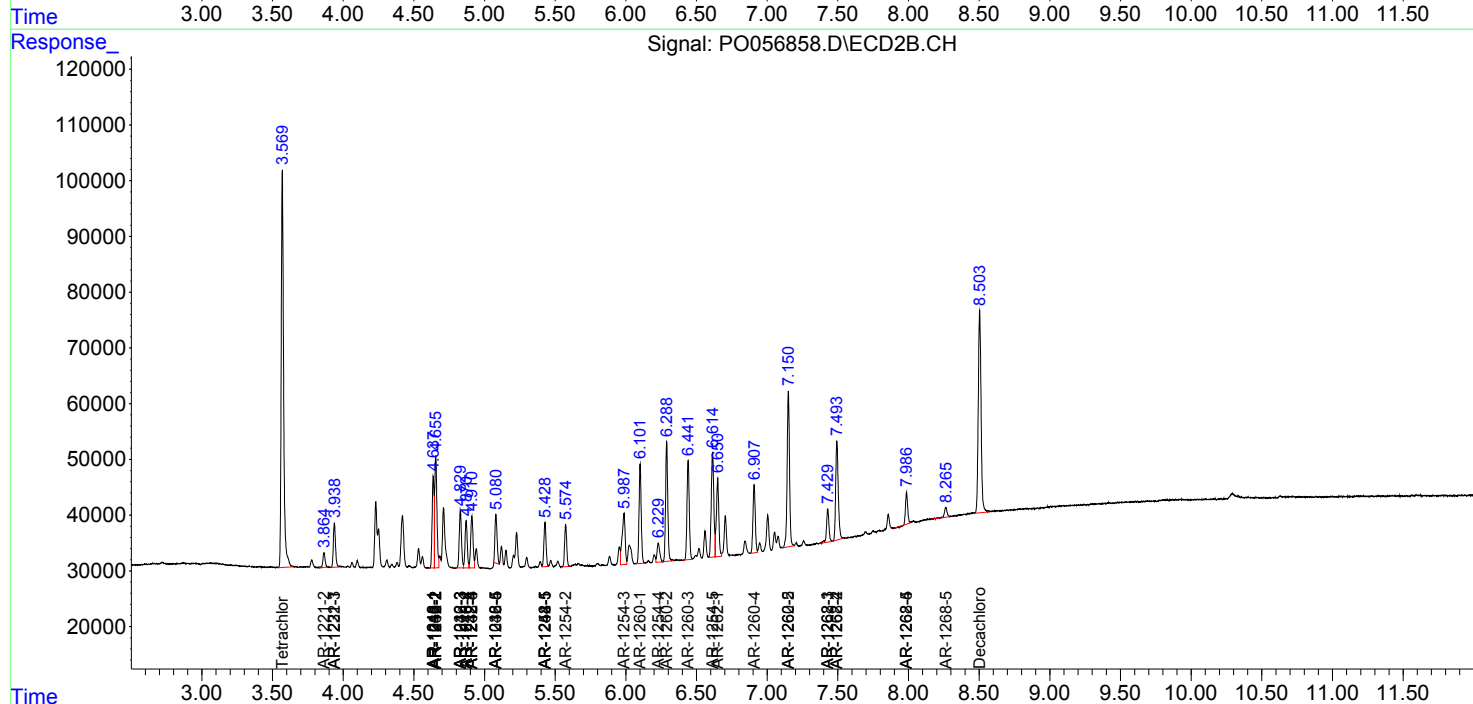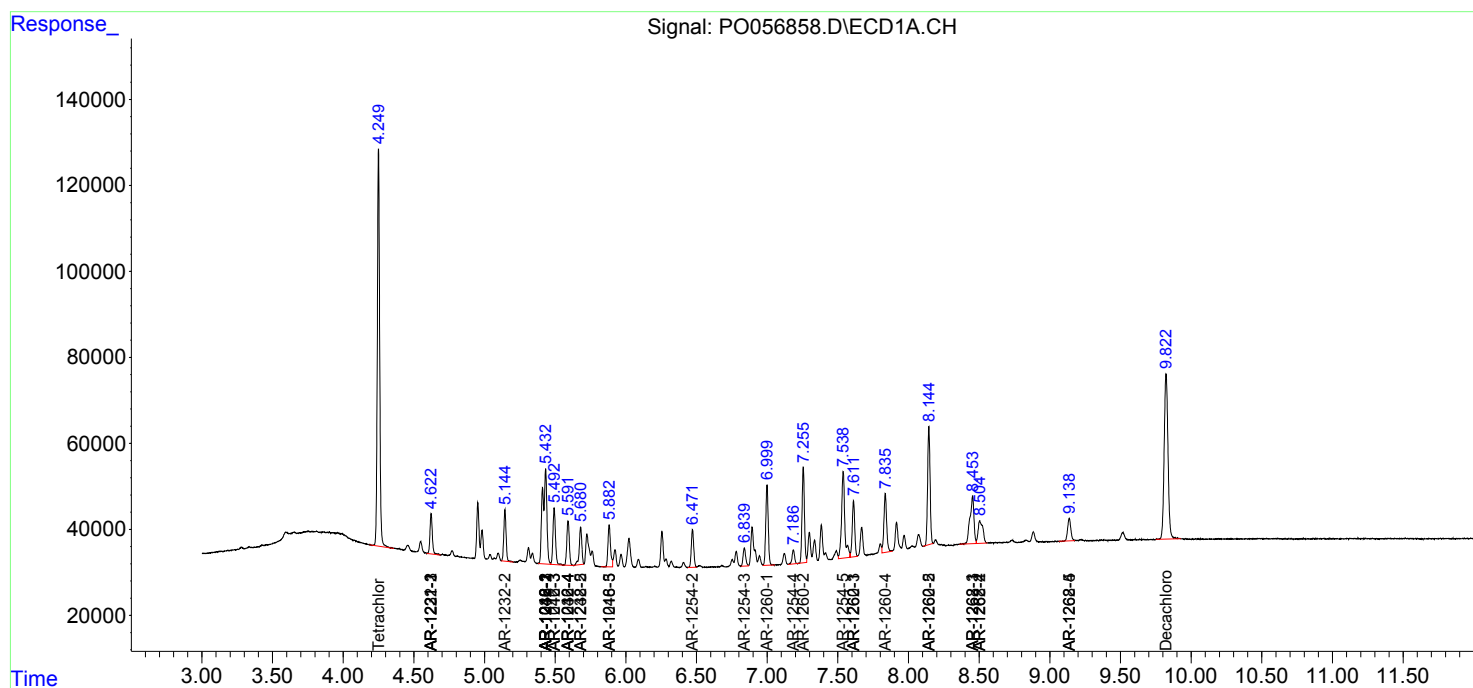


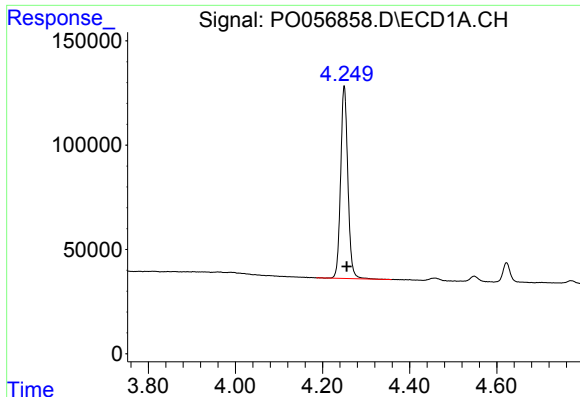

#1 Tetrachloro-m-xylene


R.T.: 4.250 min
Delta R.T.: -0.006 min
Response: 1063796
Conc: 27.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

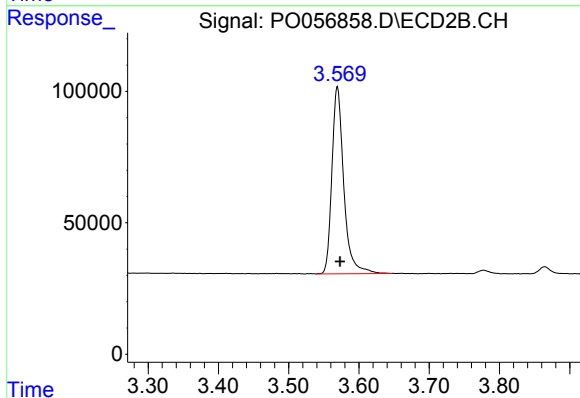


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.004 min
Response: 835459
Conc: 25.33 ng/ml

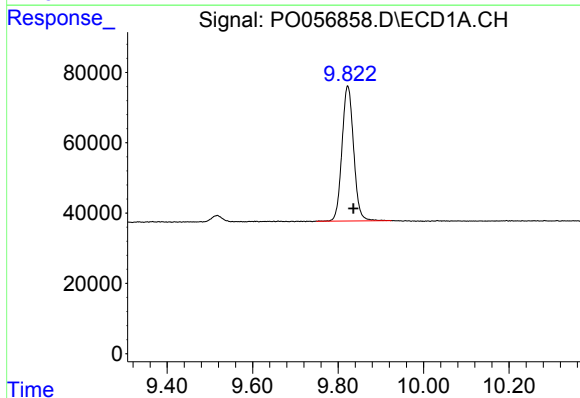


#2 Decachlorobiphenyl

R.T.: 9.823 min
Delta R.T.: -0.014 min
Response: 725234
Conc: 14.78 ng/ml

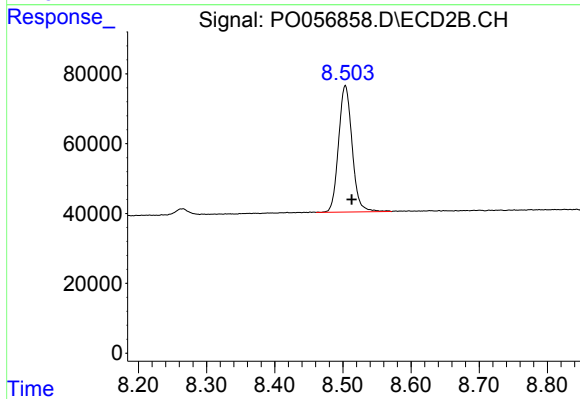

#2 Decachlorobiphenyl


R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 499877
Conc: 14.02 ng/ml

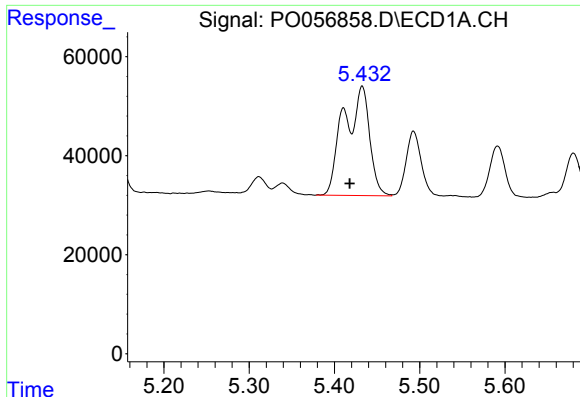

#3 AR-1016-1


R.T.: 5.433 min
Delta R.T.: 0.014 min
Response: 463019
Conc: 257.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

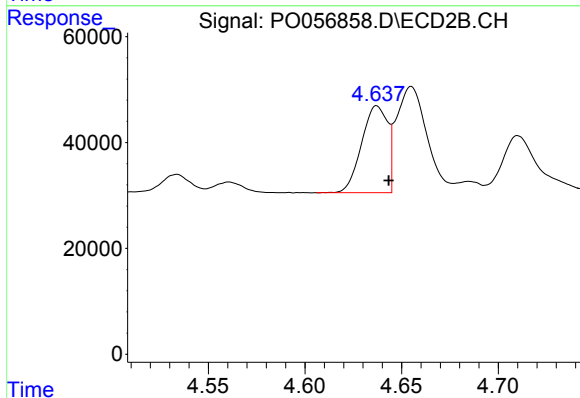


#3 AR-1016-1

R.T.: 4.637 min
Delta R.T.: -0.006 min
Response: 153640
Conc: 122.08 ng/ml

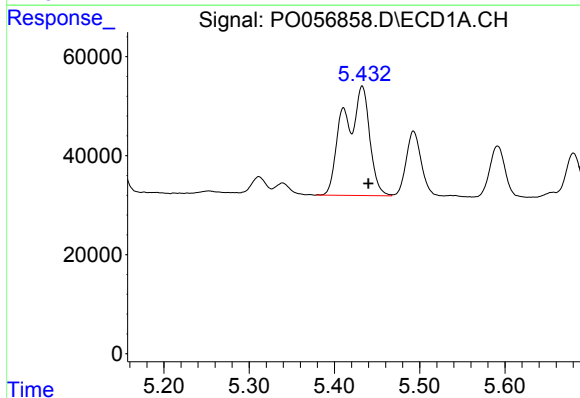


#4 AR-1016-2

R.T.: 5.433 min
Delta R.T.: -0.007 min
Response: 463019
Conc: 184.39 ng/ml

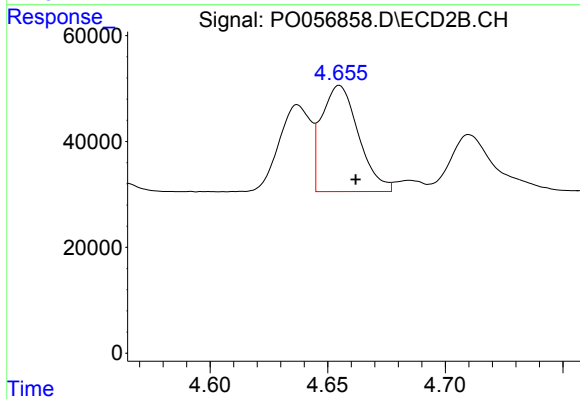

#4 AR-1016-2


R.T.: 4.655 min
Delta R.T.: -0.007 min
Response: 219724
Conc: 121.96 ng/ml

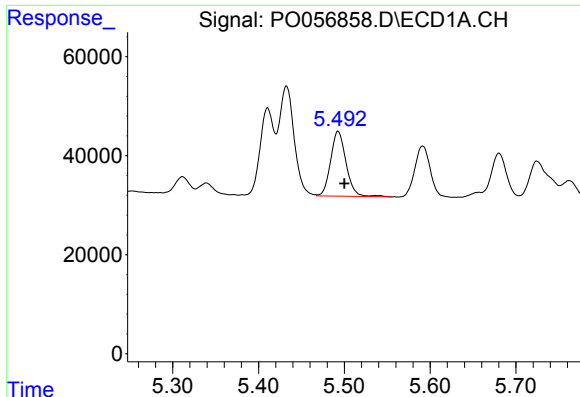

#5 AR-1016-3


R.T.: 5.493 min
Delta R.T.: -0.007 min
Response: 163967
Conc: 102.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

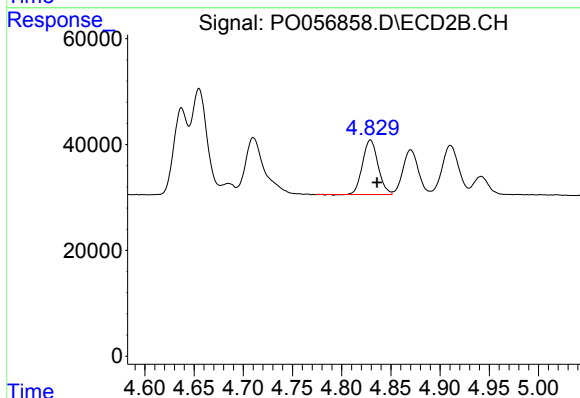


#5 AR-1016-3

R.T.: 4.829 min
Delta R.T.: -0.007 min
Response: 113531
Conc: 115.15 ng/ml

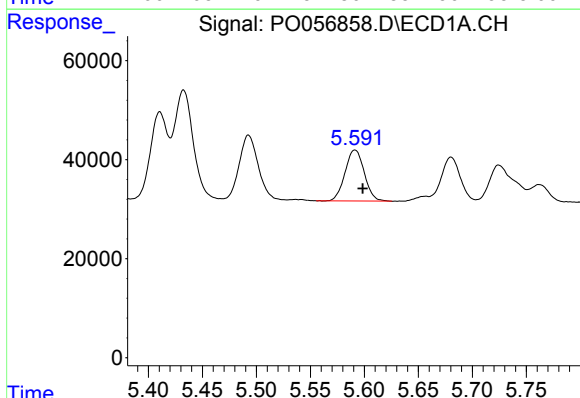


#6 AR-1016-4

R.T.: 5.591 min
Delta R.T.: -0.007 min
Response: 127608
Conc: 97.28 ng/ml

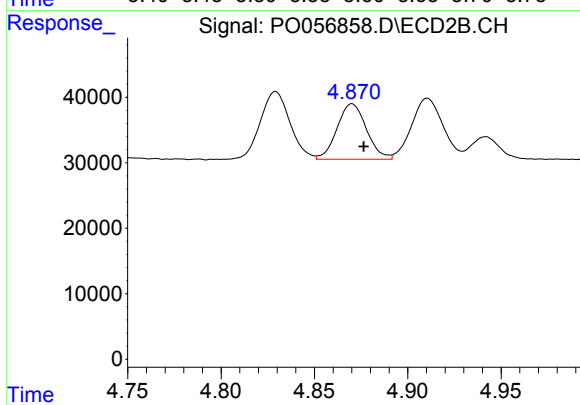

#6 AR-1016-4


R.T.: 4.870 min
Delta R.T.: -0.006 min
Response: 93053
Conc: 112.40 ng/ml

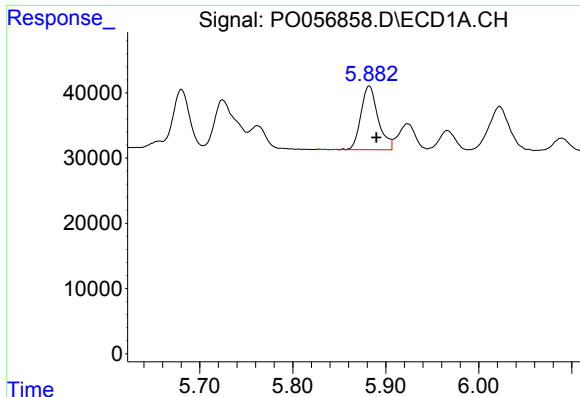

#7 AR-1016-5


R.T.: 5.882 min
Delta R.T.: -0.008 min
Response: 124832
Conc: 90.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

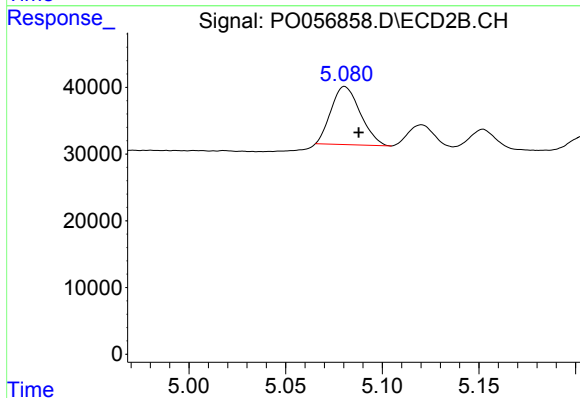


#7 AR-1016-5

R.T.: 5.081 min
Delta R.T.: -0.007 min
Response: 91546
Conc: 85.34 ng/ml

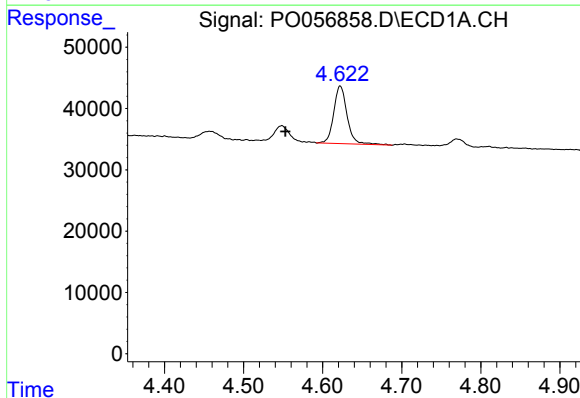


#9 AR-1221-2

R.T.: 4.622 min
Delta R.T.: 0.070 min
Response: 110240
Conc: 231.06 ng/ml

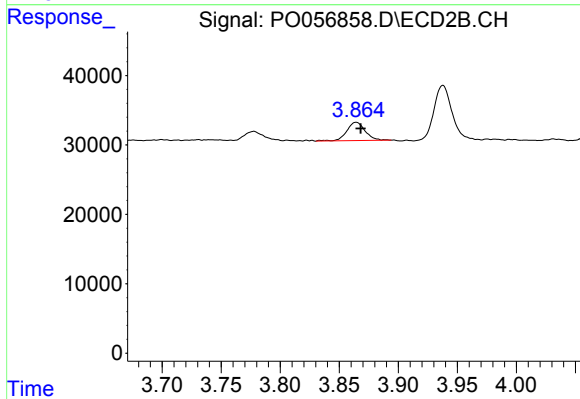

#9 AR-1221-2


R.T.: 3.864 min
Delta R.T.: -0.004 min
Response: 28812
Conc: 76.45 ng/ml

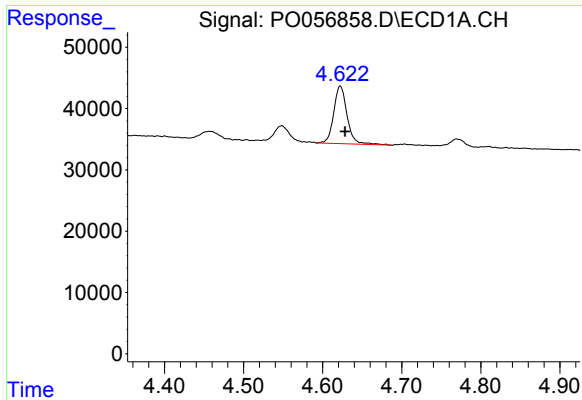

#10 AR-1221-3


R.T.: 4.622 min
Delta R.T.: -0.006 min
Response: 110240
Conc: 74.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

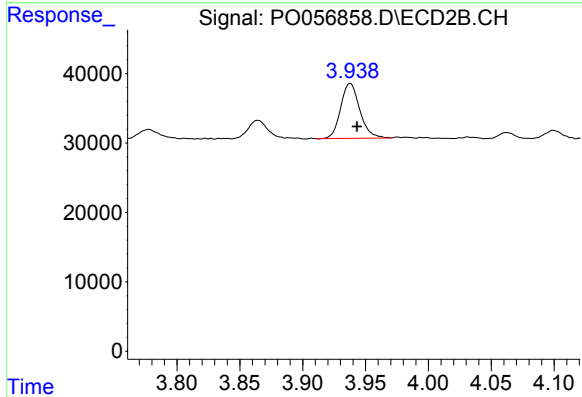


#10 AR-1221-3

R.T.: 3.938 min
Delta R.T.: -0.005 min
Response: 83811
Conc: 70.01 ng/ml

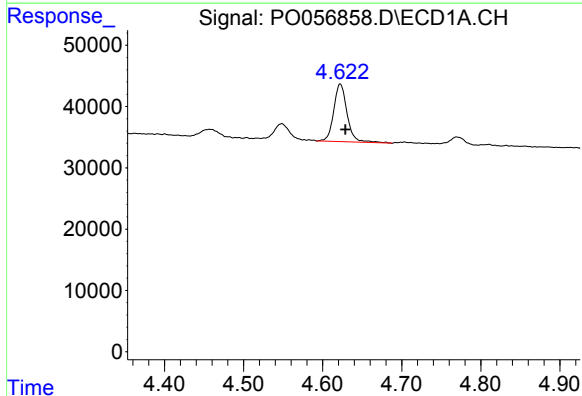


#11 AR-1232-1

R.T.: 4.622 min
Delta R.T.: -0.006 min
Response: 110240
Conc: 93.55 ng/ml

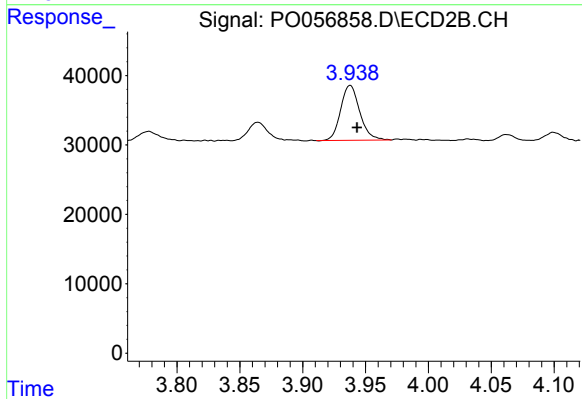

#11 AR-1232-1


R.T.: 3.938 min
Delta R.T.: -0.005 min
Response: 83811
Conc: 93.29 ng/ml

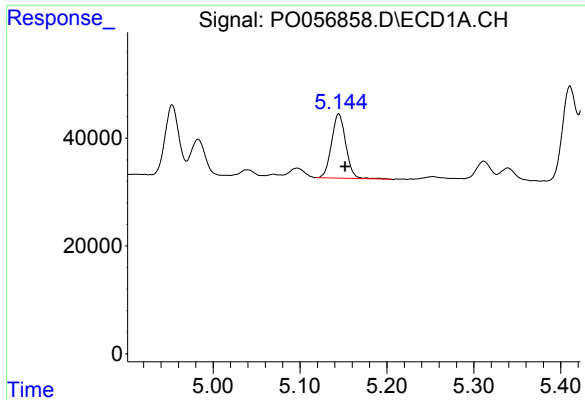

#12 AR-1232-2


R.T.: 5.145 min
Delta R.T.: -0.007 min
Response: 136184
Conc: 205.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

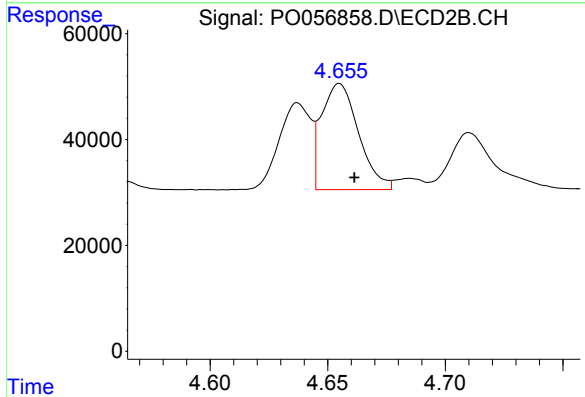


#12 AR-1232-2

R.T.: 4.655 min
Delta R.T.: -0.006 min
Response: 219724
Conc: 226.08 ng/ml

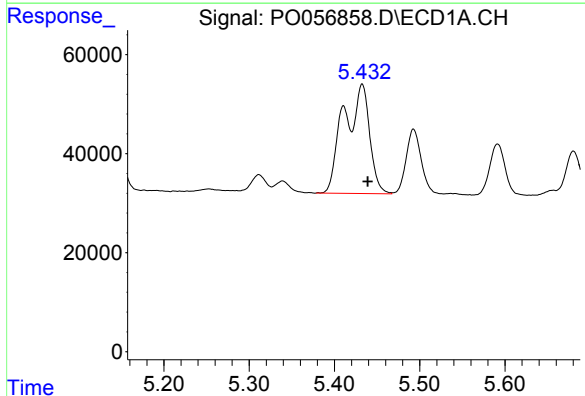


#13 AR-1232-3

R.T.: 5.433 min
Delta R.T.: -0.007 min
Response: 463019
Conc: 326.38 ng/ml

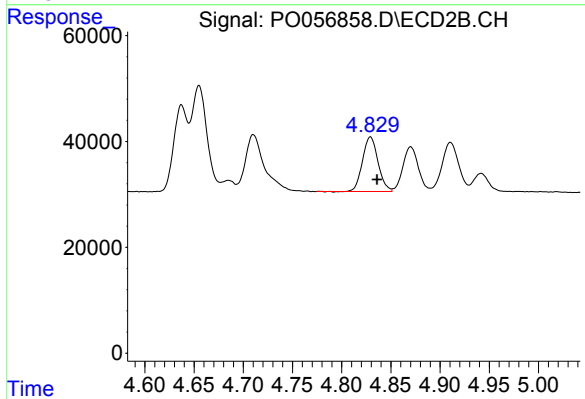

#13 AR-1232-3


R.T.: 4.829 min
Delta R.T.: -0.007 min
Response: 113531
Conc: 216.96 ng/ml

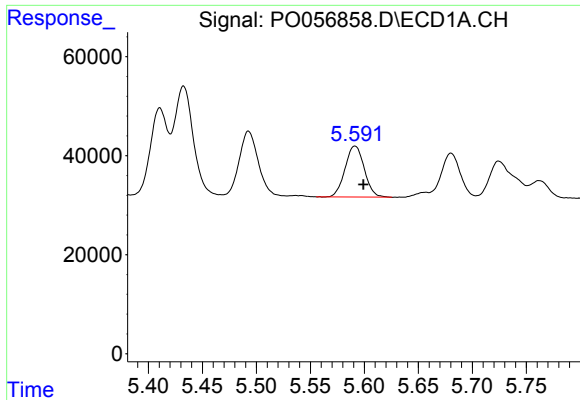

#14 AR-1232-4


R.T.: 5.591 min
Delta R.T.: -0.008 min
Response: 127608
Conc: 181.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

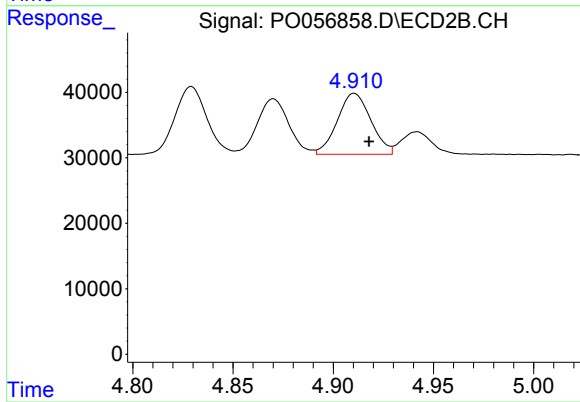


#14 AR-1232-4

R.T.: 4.911 min
Delta R.T.: -0.007 min
Response: 108644
Conc: 220.51 ng/ml

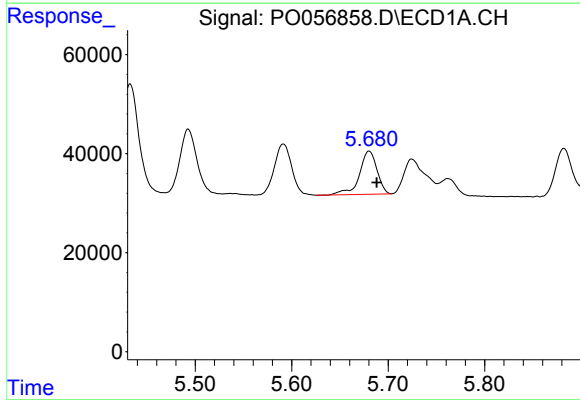


#15 AR-1232-5

R.T.: 5.680 min
Delta R.T.: -0.008 min
Response: 109608
Conc: 193.86 ng/ml

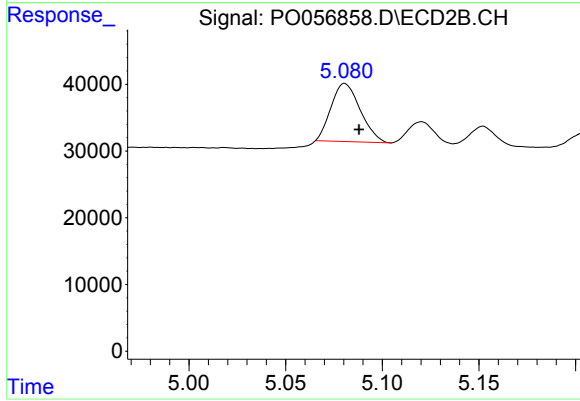

#15 AR-1232-5


R.T.: 5.081 min
Delta R.T.: -0.007 min
Response: 91546
Conc: 162.53 ng/ml

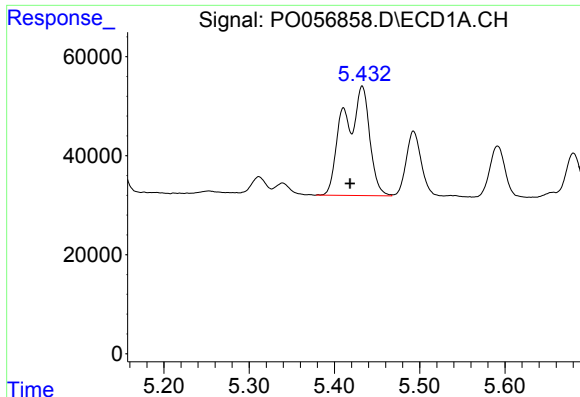

#16 AR-1242-1


R.T.: 5.433 min
Delta R.T.: 0.014 min
Response: 463019
Conc: 268.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

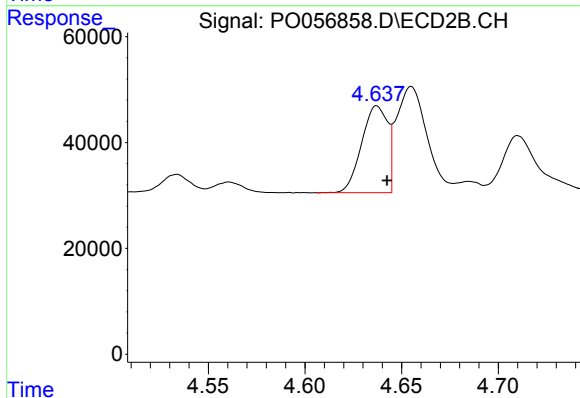


#16 AR-1242-1

R.T.: 4.637 min
Delta R.T.: -0.005 min
Response: 153640
Conc: 124.05 ng/ml

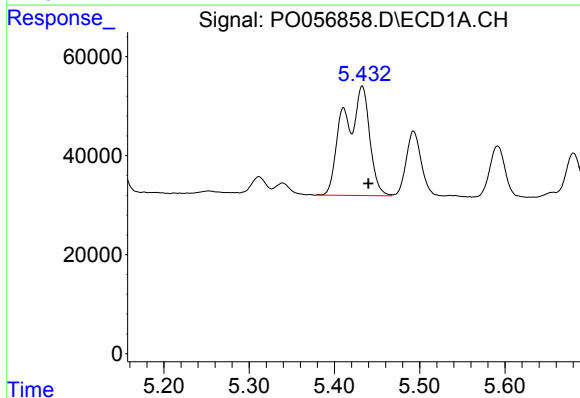


#17 AR-1242-2

R.T.: 5.433 min
Delta R.T.: -0.007 min
Response: 463019
Conc: 182.38 ng/ml

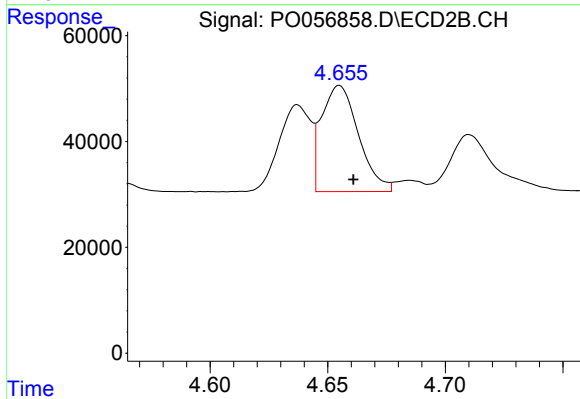

#17 AR-1242-2


R.T.: 4.655 min
Delta R.T.: -0.006 min
Response: 219724
Conc: 122.18 ng/ml

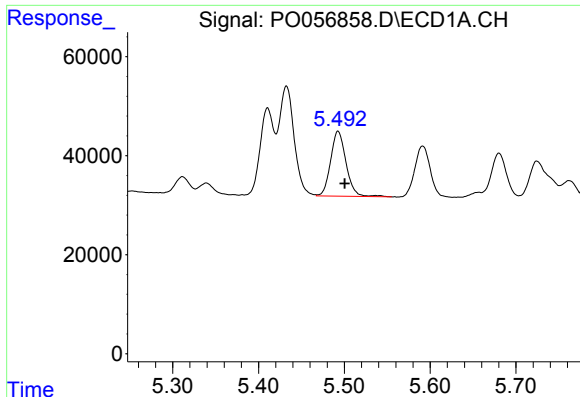

#18 AR-1242-3


R.T.: 5.493 min
Delta R.T.: -0.008 min
Response: 163967
Conc: 100.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

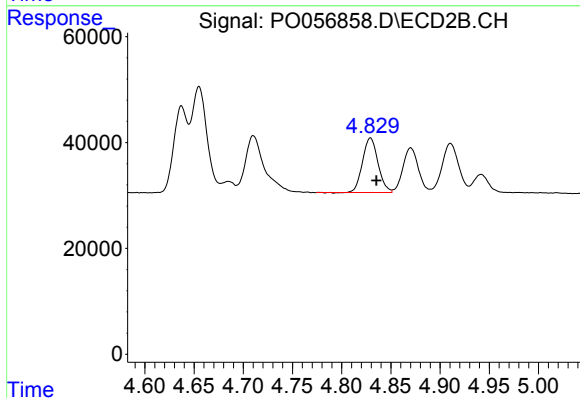


#18 AR-1242-3

R.T.: 4.829 min
Delta R.T.: -0.006 min
Response: 113531
Conc: 115.48 ng/ml

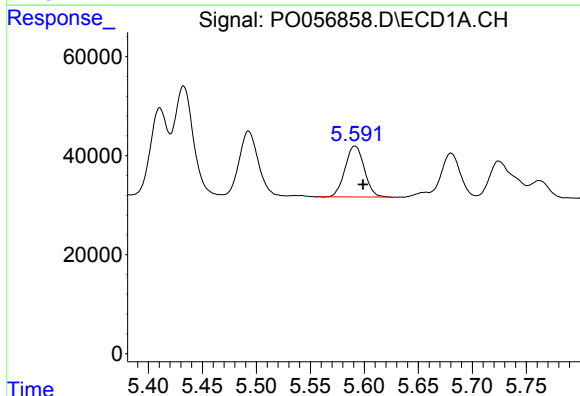


#19 AR-1242-4

R.T.: 5.591 min
Delta R.T.: -0.007 min
Response: 127608
Conc: 95.46 ng/ml

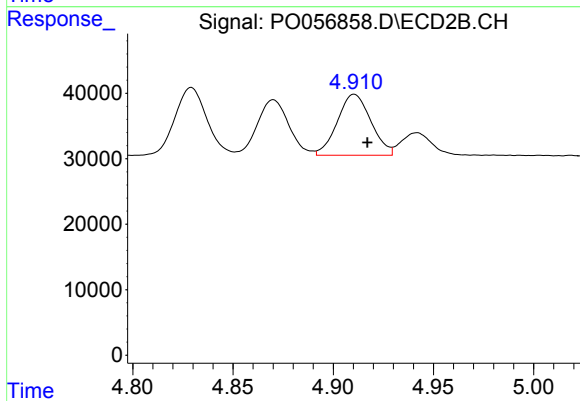

#19 AR-1242-4


R.T.: 4.911 min
Delta R.T.: -0.006 min
Response: 108644
Conc: 111.65 ng/ml

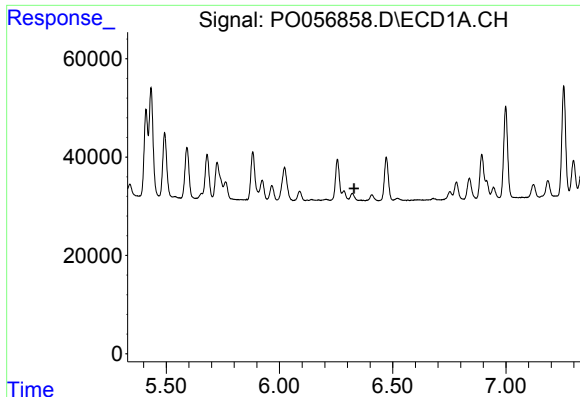

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

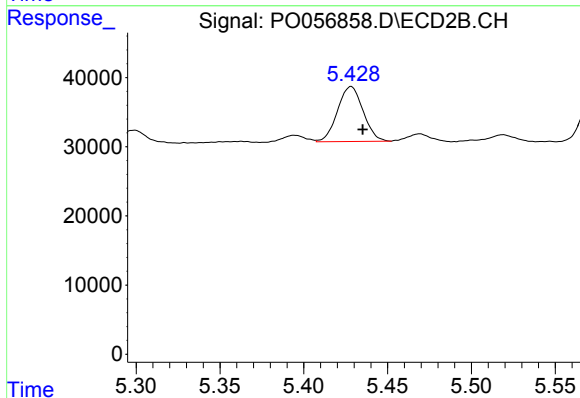


#20 AR-1242-5

R.T.: 5.428 min
Delta R.T.: -0.007 min
Response: 84191
Conc: 71.21 ng/ml

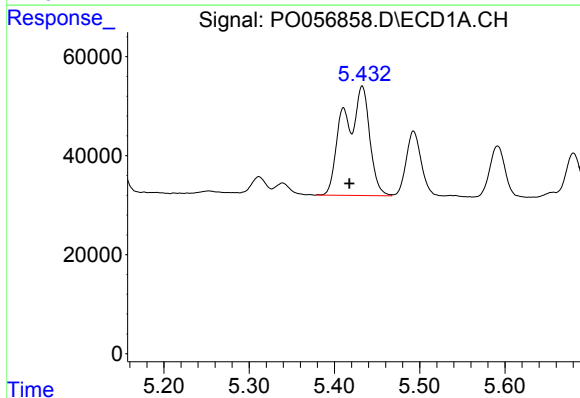


#21 AR-1248-1

R.T.: 5.433 min
Delta R.T.: 0.015 min
Response: 463019
Conc: 359.34 ng/ml

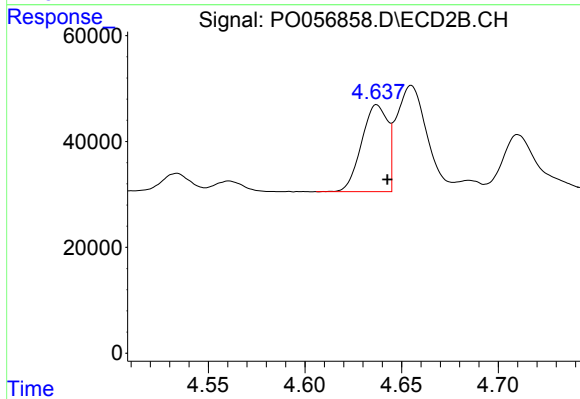

#21 AR-1248-1


R.T.: 4.637 min
Delta R.T.: -0.006 min
Response: 153640
Conc: 164.05 ng/ml

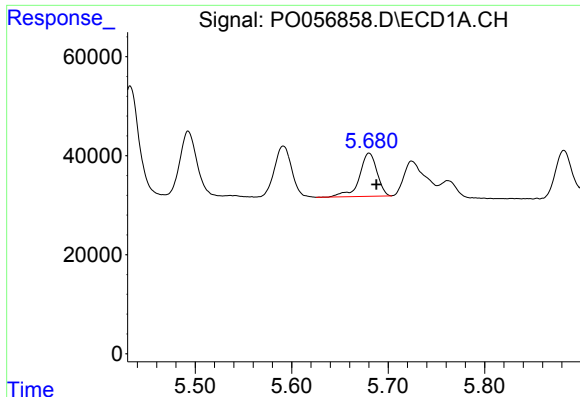

#22 AR-1248-2


R.T.: 5.680 min
Delta R.T.: -0.008 min
Response: 109608
Conc: 58.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

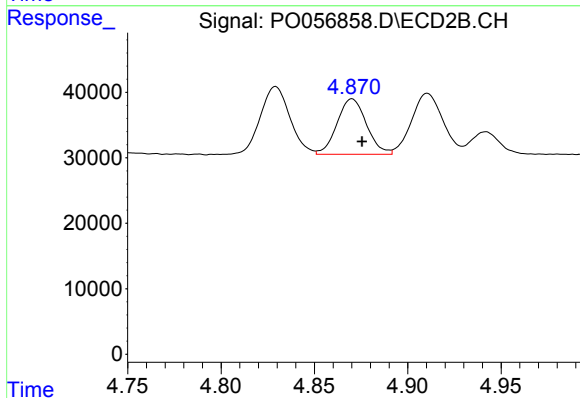


#22 AR-1248-2

R.T.: 4.870 min
Delta R.T.: -0.005 min
Response: 93053
Conc: 73.24 ng/ml

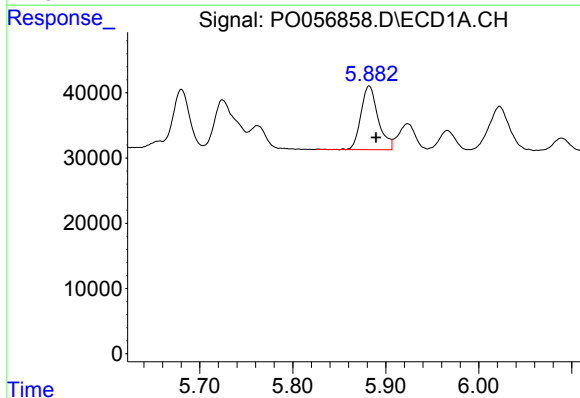


#23 AR-1248-3

R.T.: 5.882 min
Delta R.T.: -0.008 min
Response: 124832
Conc: 60.85 ng/ml

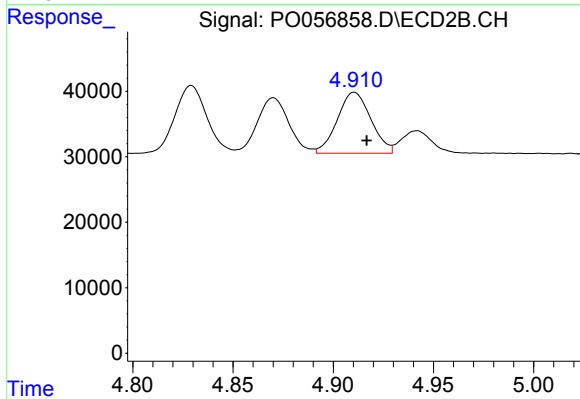

#23 AR-1248-3


R.T.: 4.911 min
Delta R.T.: -0.006 min
Response: 108644
Conc: 83.19 ng/ml

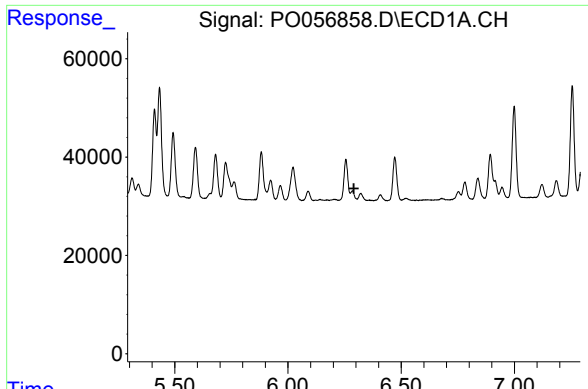

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

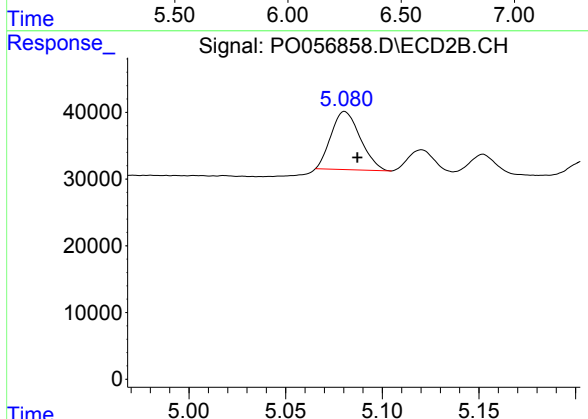


#24 AR-1248-4

R.T.: 5.081 min
Delta R.T.: -0.007 min
Response: 91546
Conc: 57.81 ng/ml

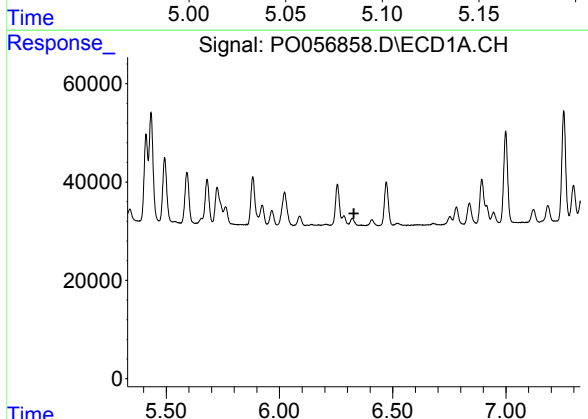


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

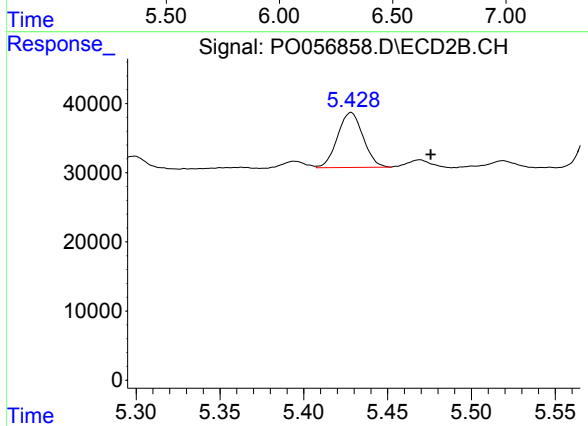

#25 AR-1248-5


R.T.: 5.428 min
Delta R.T.: -0.047 min
Response: 84191
Conc: 50.87 ng/ml

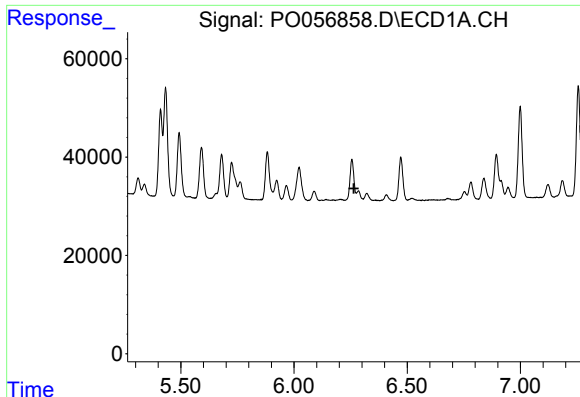

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

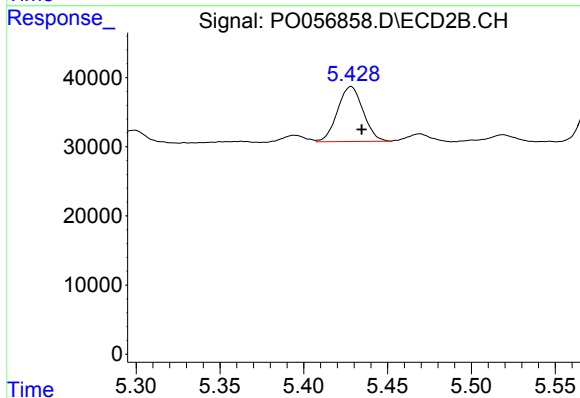


#26 AR-1254-1

R.T.: 5.428 min
Delta R.T.: -0.006 min
Response: 84191
Conc: 31.83 ng/ml

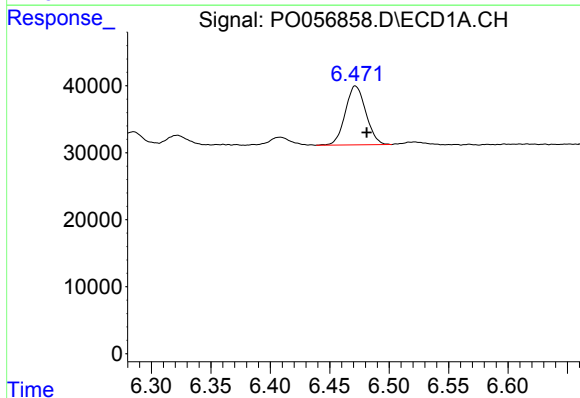


#27 AR-1254-2

R.T.: 6.472 min
Delta R.T.: -0.009 min
Response: 105859
Conc: 27.25 ng/ml

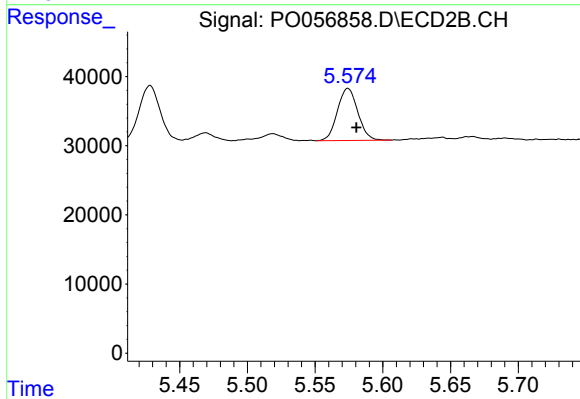

#27 AR-1254-2


R.T.: 5.574 min
Delta R.T.: -0.006 min
Response: 78898
Conc: 36.60 ng/ml

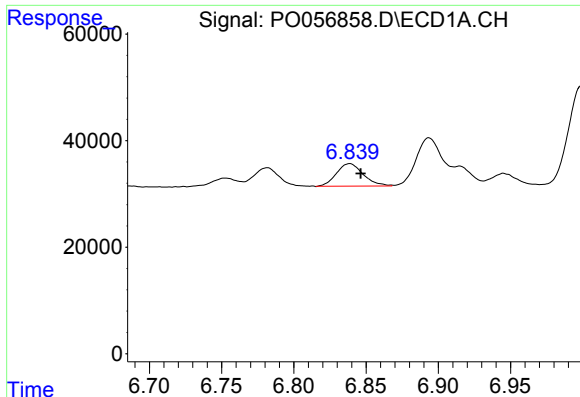

#28 AR-1254-3


R.T.: 6.839 min
Delta R.T.: -0.008 min
Response: 54701
Conc: 13.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

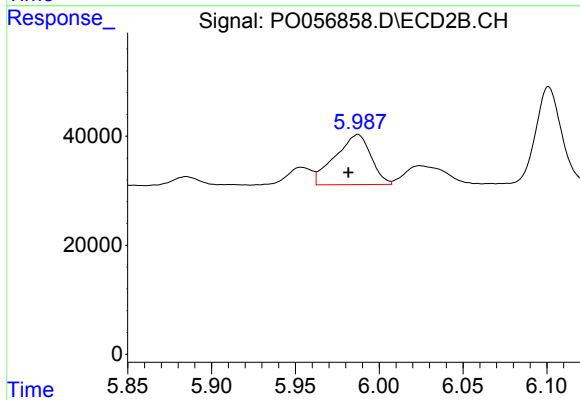


#28 AR-1254-3

R.T.: 5.987 min
Delta R.T.: 0.006 min
Response: 136115
Conc: 37.18 ng/ml

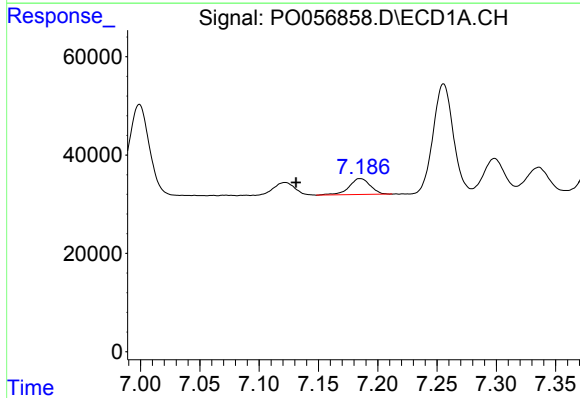


#29 AR-1254-4

R.T.: 7.185 min
Delta R.T.: 0.054 min
Response: 40299
Conc: 13.39 ng/ml

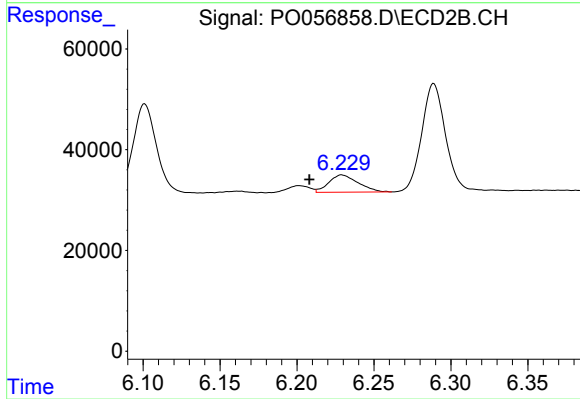

#29 AR-1254-4


R.T.: 6.229 min
Delta R.T.: 0.021 min
Response: 45402
Conc: 20.67 ng/ml

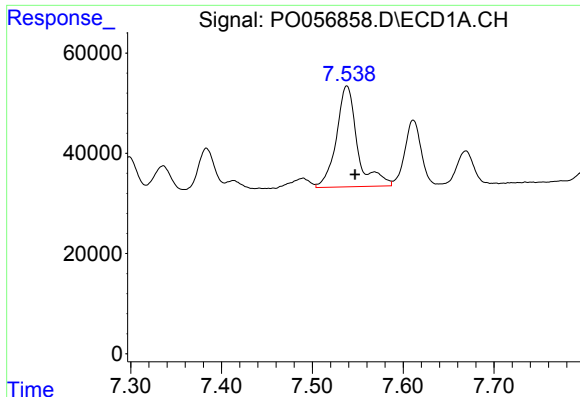

#30 AR-1254-5


R.T.: 7.538 min
Delta R.T.: -0.009 min
Response: 324148
Conc: 86.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

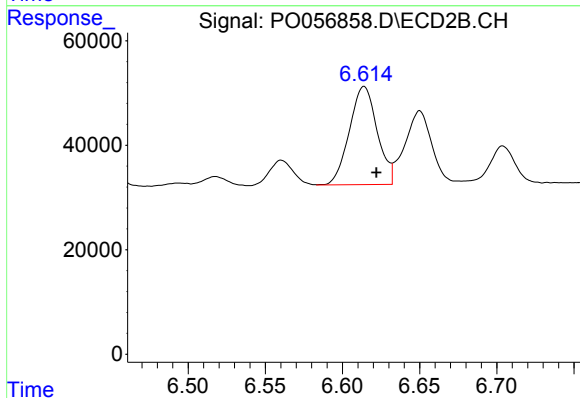


#30 AR-1254-5

R.T.: 6.614 min
Delta R.T.: -0.008 min
Response: 235927
Conc: 74.42 ng/ml

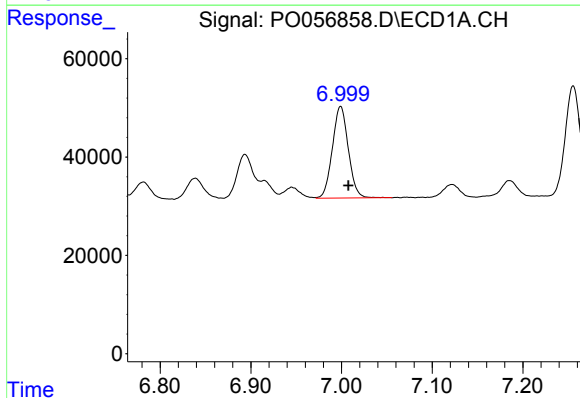


#31 AR-1260-1

R.T.: 6.999 min
Delta R.T.: -0.009 min
Response: 227403
Conc: 88.62 ng/ml

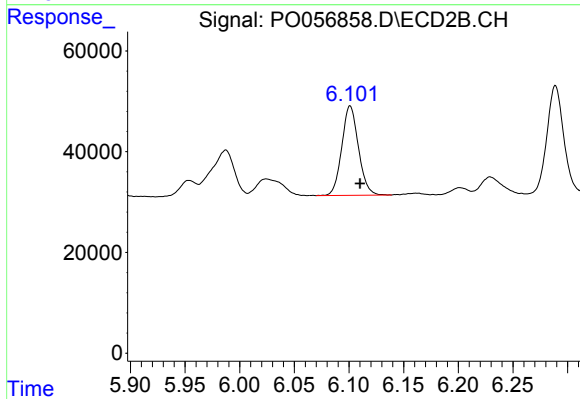

#31 AR-1260-1


R.T.: 6.101 min
Delta R.T.: -0.009 min
Response: 188898
Conc: 94.43 ng/ml

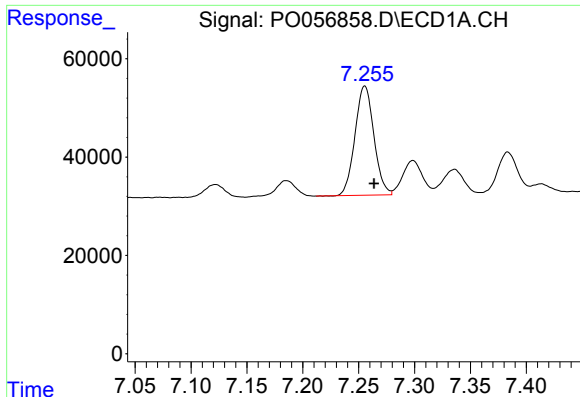

#32 AR-1260-2


R.T.: 7.255 min
Delta R.T.: -0.008 min
Response: 261699
Conc: 86.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

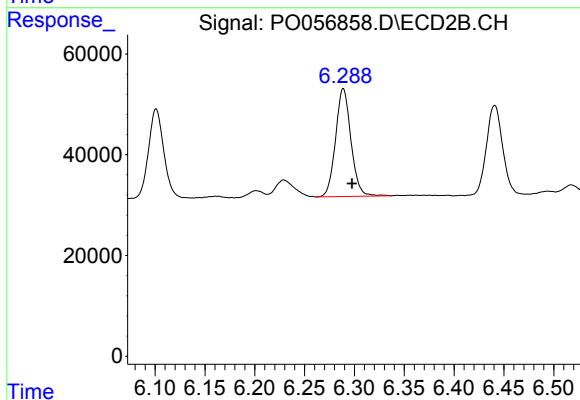


#32 AR-1260-2

R.T.: 6.289 min
Delta R.T.: -0.009 min
Response: 230233
Conc: 93.40 ng/ml

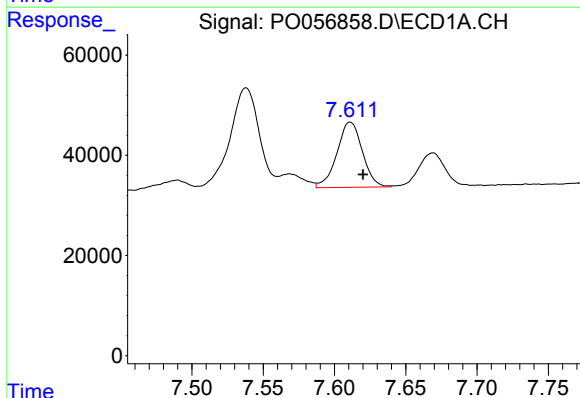


#33 AR-1260-3

R.T.: 7.611 min
Delta R.T.: -0.009 min
Response: 161750
Conc: 67.14 ng/ml

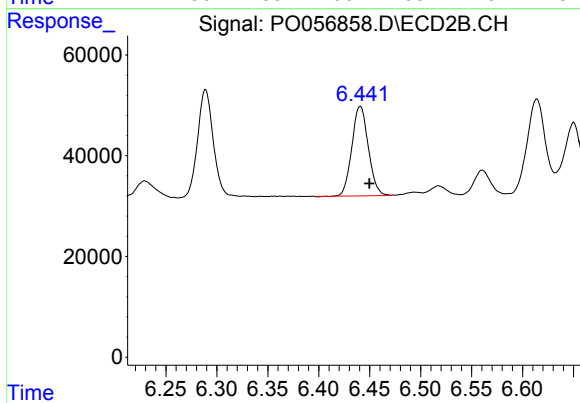

#33 AR-1260-3


R.T.: 6.441 min
Delta R.T.: -0.009 min
Response: 200396
Conc: 89.33 ng/ml

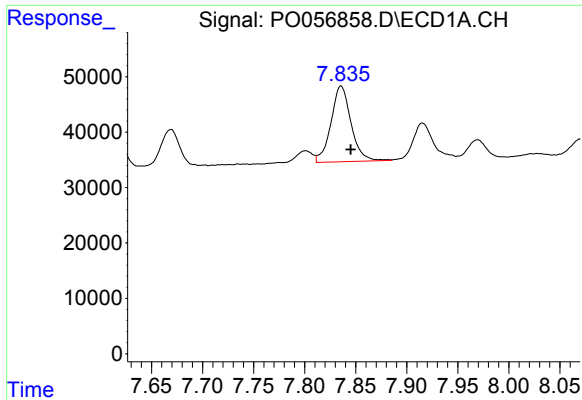

#34 AR-1260-4


R.T.: 7.836 min
Delta R.T.: -0.009 min
Response: 186719
Conc: 71.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

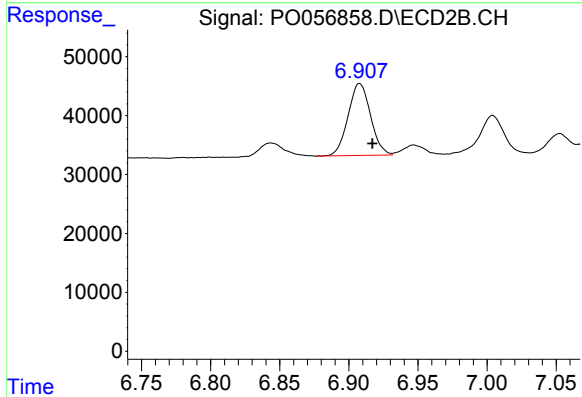


#34 AR-1260-4

R.T.: 6.908 min
Delta R.T.: -0.009 min
Response: 138569
Conc: 74.46 ng/ml

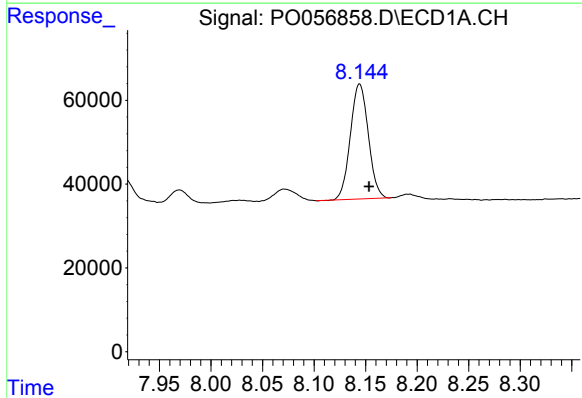


#35 AR-1260-5

R.T.: 8.144 min
Delta R.T.: -0.009 min
Response: 332317
Conc: 69.49 ng/ml

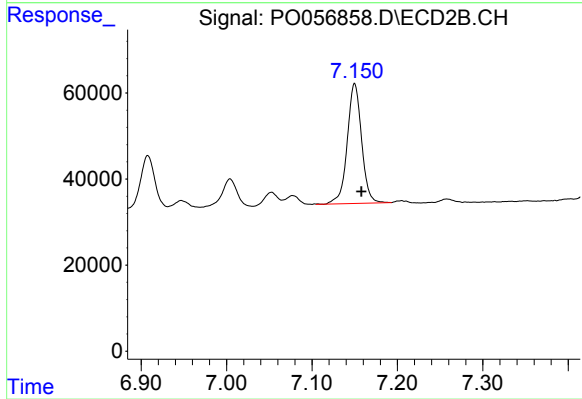

#35 AR-1260-5


R.T.: 7.150 min
Delta R.T.: -0.008 min
Response: 325377
Conc: 75.45 ng/ml

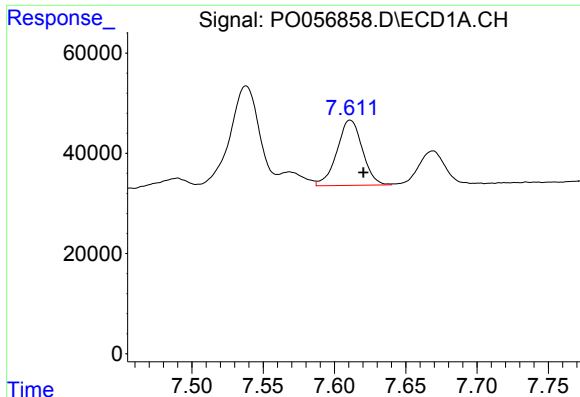

#36 AR-1262-1


R.T.: 7.611 min
Delta R.T.: -0.009 min
Response: 161750
Conc: 34.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

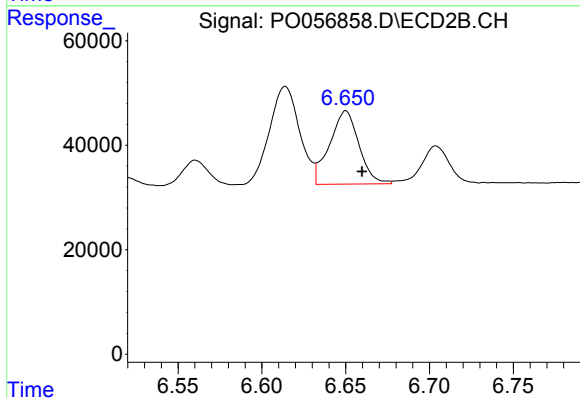


#36 AR-1262-1

R.T.: 6.650 min
Delta R.T.: -0.010 min
Response: 171234
Conc: 41.02 ng/ml

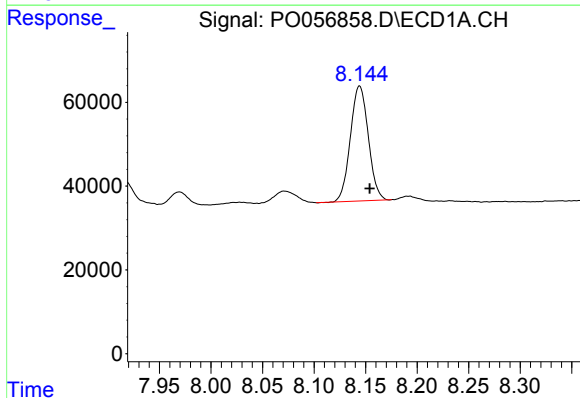


#37 AR-1262-2

R.T.: 8.144 min
Delta R.T.: -0.010 min
Response: 332317
Conc: 43.59 ng/ml

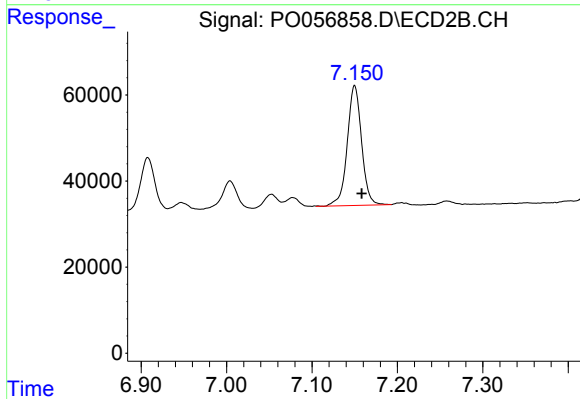

#37 AR-1262-2


R.T.: 7.150 min
Delta R.T.: -0.008 min
Response: 325377
Conc: 47.36 ng/ml

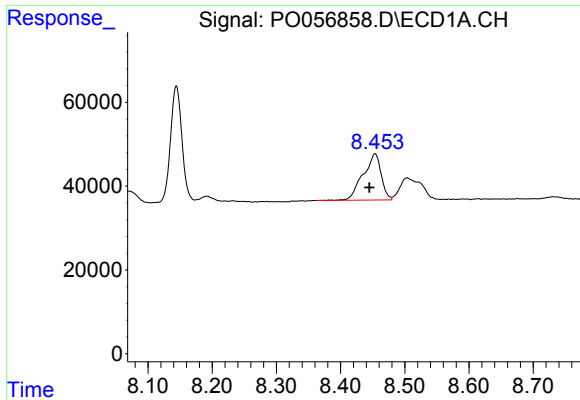

#38 AR-1262-3


R.T.: 8.454 min
Delta R.T.: 0.009 min
Response: 215711
Conc: 41.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

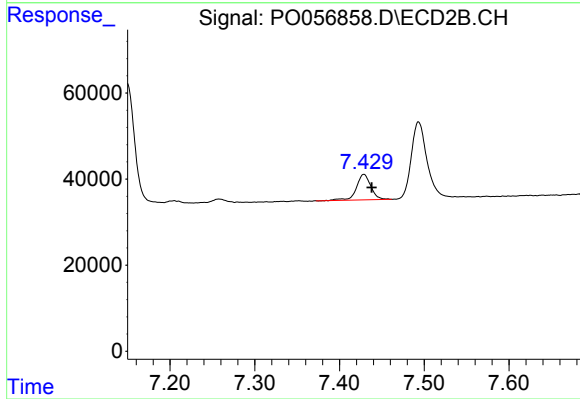


#38 AR-1262-3

R.T.: 7.429 min
Delta R.T.: -0.009 min
Response: 70693
Conc: 23.94 ng/ml

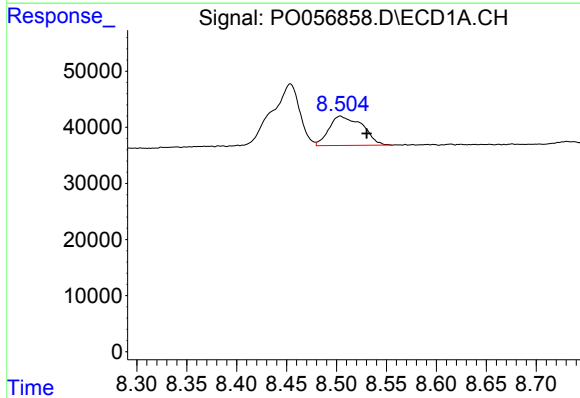


#39 AR-1262-4

R.T.: 8.504 min
Delta R.T.: -0.026 min
Response: 121690
Conc: 28.50 ng/ml

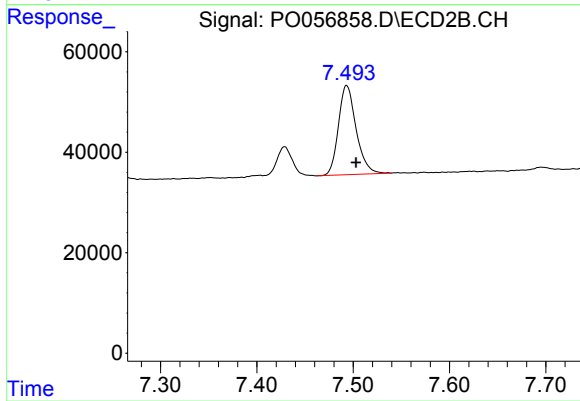

#39 AR-1262-4


R.T.: 7.493 min
Delta R.T.: -0.010 min
Response: 226489
Conc: 43.47 ng/ml

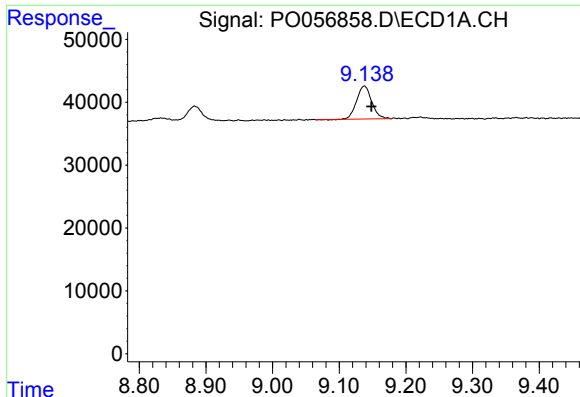

#40 AR-1262-5


R.T.: 9.138 min
Delta R.T.: -0.011 min
Response: 82142
Conc: 29.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

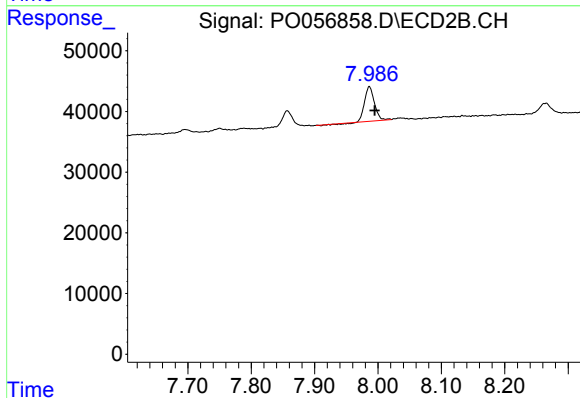


#40 AR-1262-5

R.T.: 7.986 min
Delta R.T.: -0.008 min
Response: 59720
Conc: 25.72 ng/ml

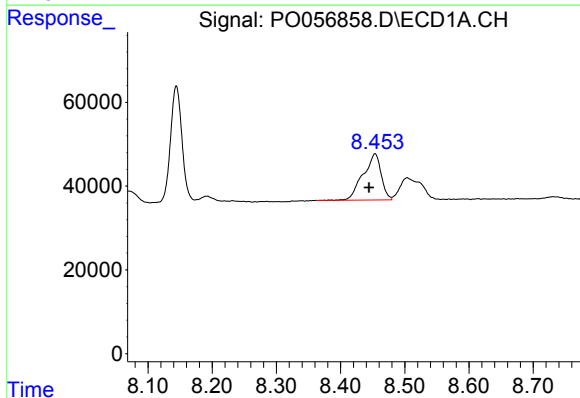


#41 AR-1268-1

R.T.: 8.454 min
Delta R.T.: 0.009 min
Response: 215711
Conc: 26.51 ng/ml

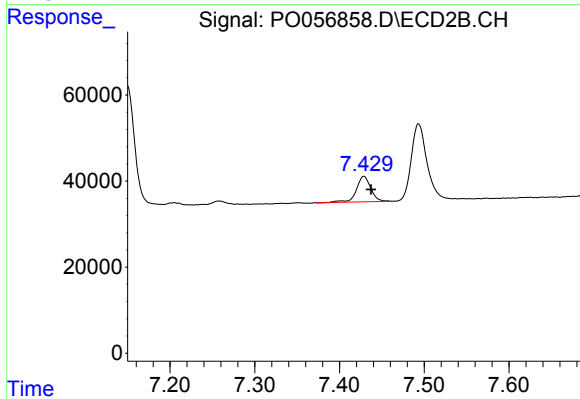

#41 AR-1268-1


R.T.: 7.429 min
Delta R.T.: -0.008 min
Response: 70693
Conc: 9.47 ng/ml

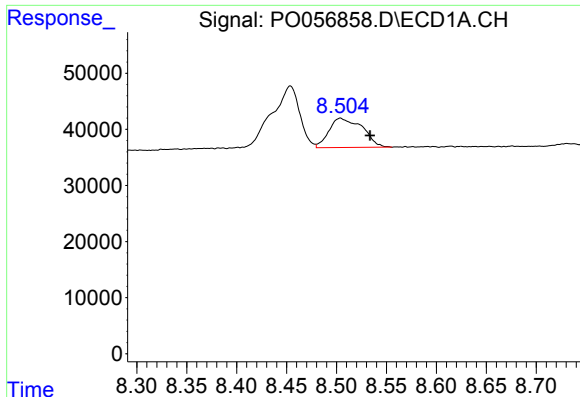

#42 AR-1268-2


R.T.: 8.504 min
Delta R.T.: -0.029 min
Response: 121690
Conc: 15.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

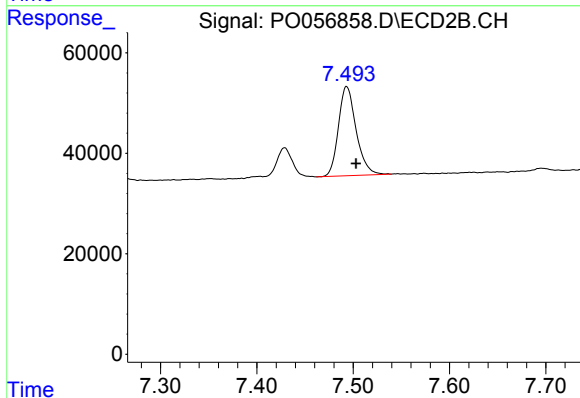


#42 AR-1268-2

R.T.: 7.493 min
Delta R.T.: -0.010 min
Response: 226489
Conc: 32.43 ng/ml

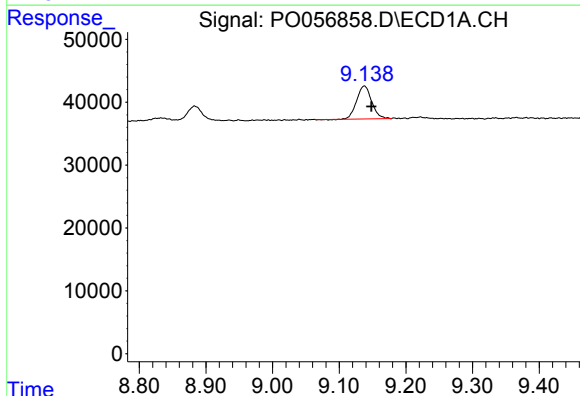


#44 AR-1268-4

R.T.: 9.138 min
Delta R.T.: -0.011 min
Response: 82142
Conc: 30.12 ng/ml

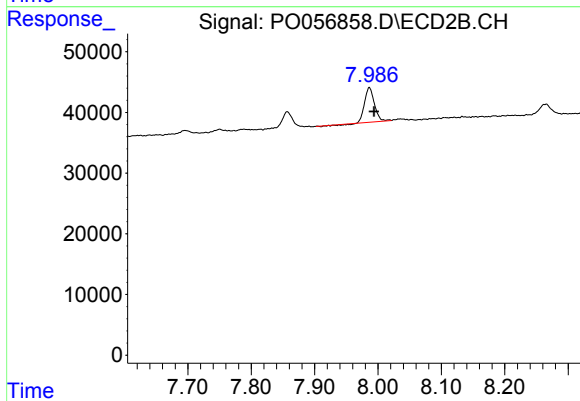

#44 AR-1268-4


R.T.: 7.986 min
Delta R.T.: -0.007 min
Response: 59720
Conc: 25.58 ng/ml

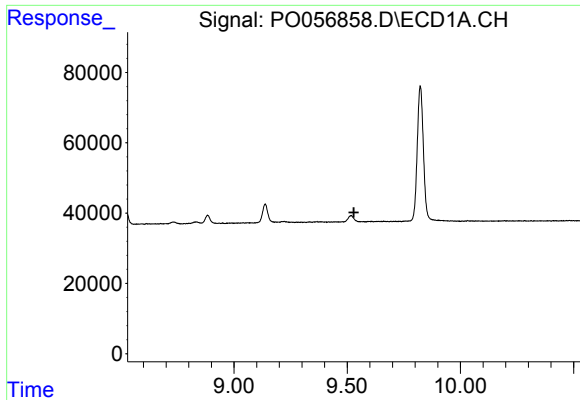

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

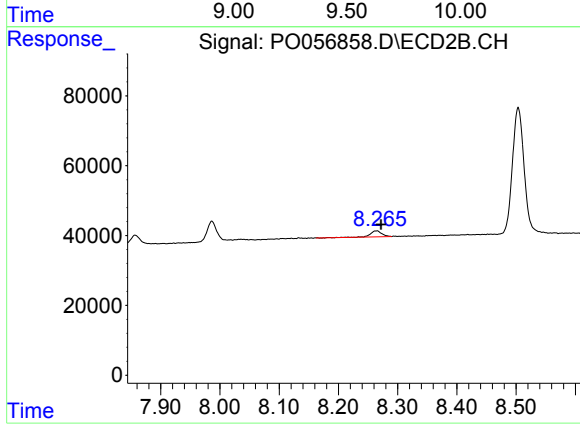

#45 AR-1268-5

R.T.: 8.265 min
Delta R.T.: -0.007 min
Response: 22681
Conc: 1.31 ng/ml